

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081320\
 Data File : PD058946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2020 15:52
 Operator : DD\AJ
 Sample : PB130946BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:14:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	19032235	28719243	19.680	19.830
27)	SA Decachlor...	7.840	8.859	37709792	45738090	35.801	33.351
Target Compounds							
8)	B Heptachlo...	0.000	5.760f	0	1016935	N.D.	0.611
16)	A 4,4'-DDD	0.000	6.624f	0	2759468	N.D.	2.105


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081320\
Data File : PD058946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2020 15:52
Operator : DD\AJ
Sample : PB130946BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:14:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

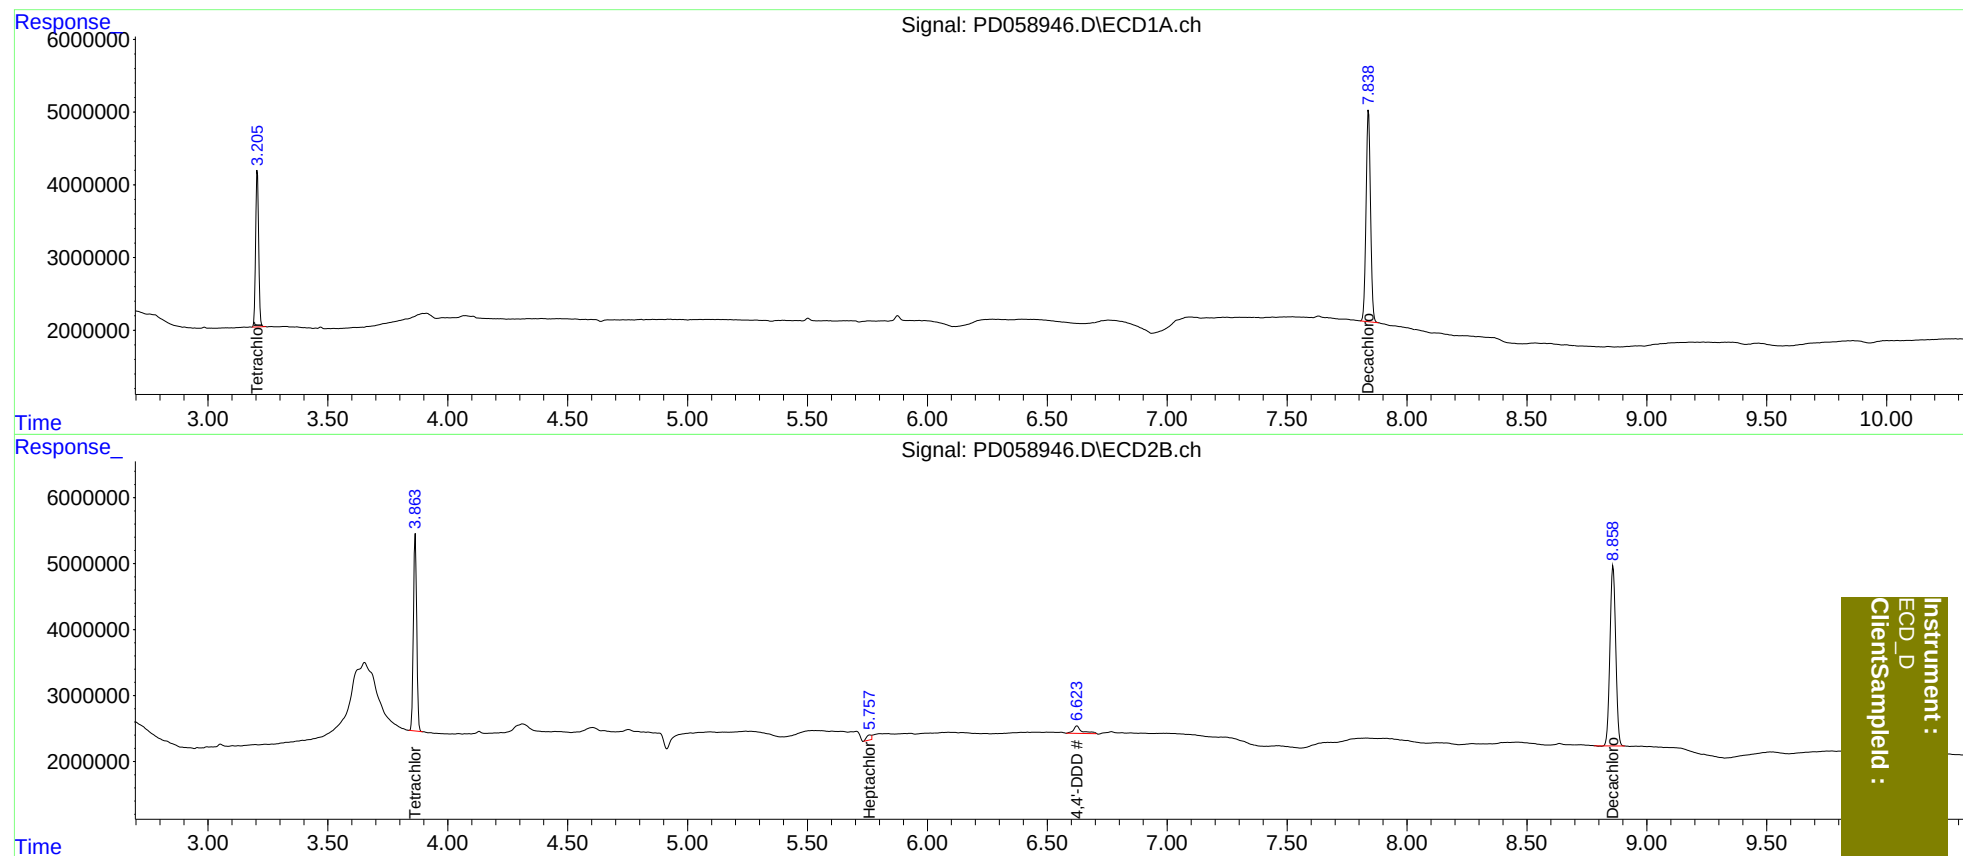


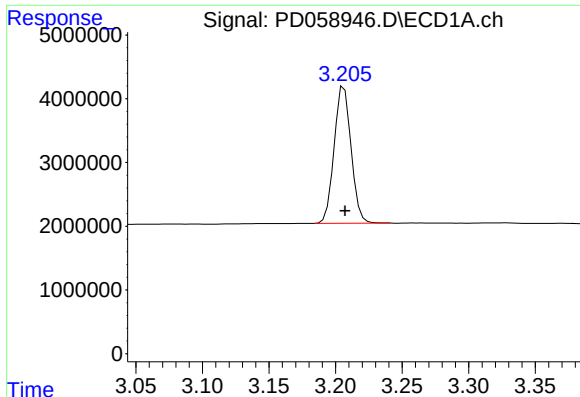

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 19032235
Conc: 19.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

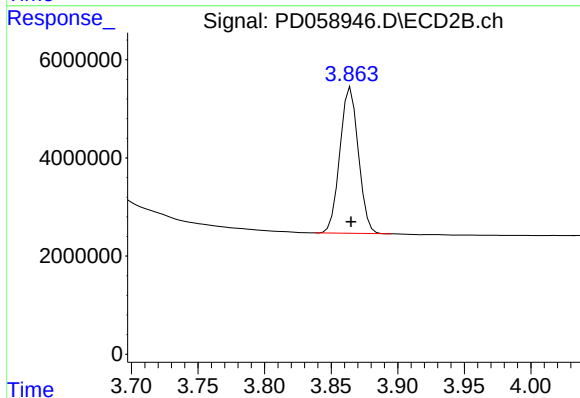


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 28719243
Conc: 19.83 ng/ml

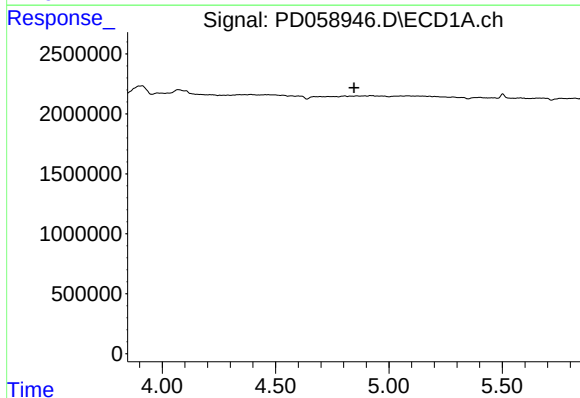


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

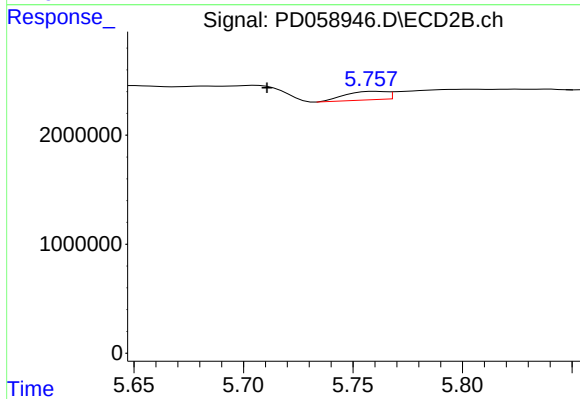

#8 Heptachlor epoxide


R.T.: 5.760 min
Delta R.T.: 0.049 min
Response: 1016935
Conc: 0.61 ng/ml

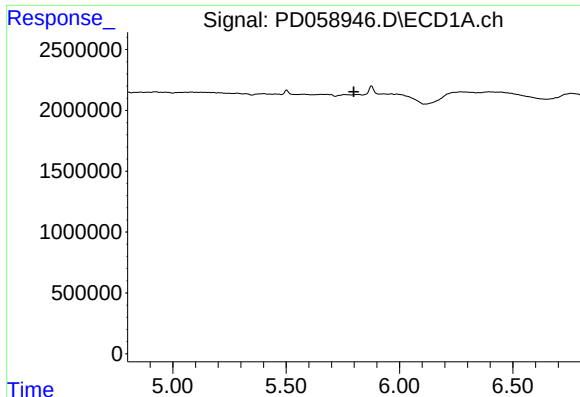

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

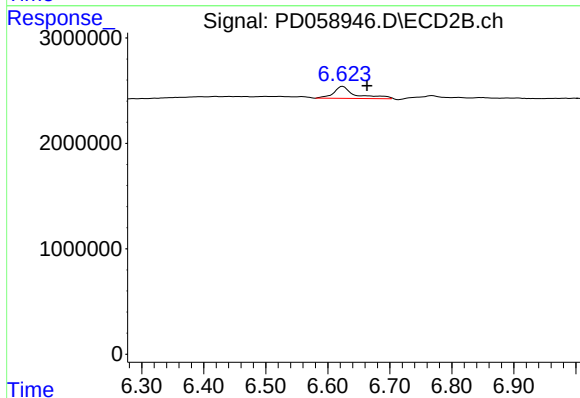


#16 4,4'-DDD

R.T.: 6.624 min
Delta R.T.: -0.039 min
Response: 2759468
Conc: 2.11 ng/ml

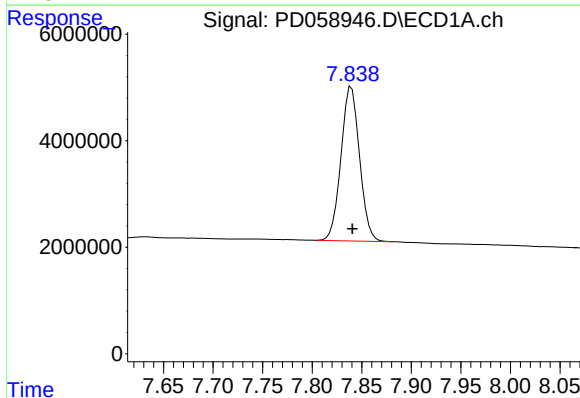

#27 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 37709792
Conc: 35.80 ng/ml

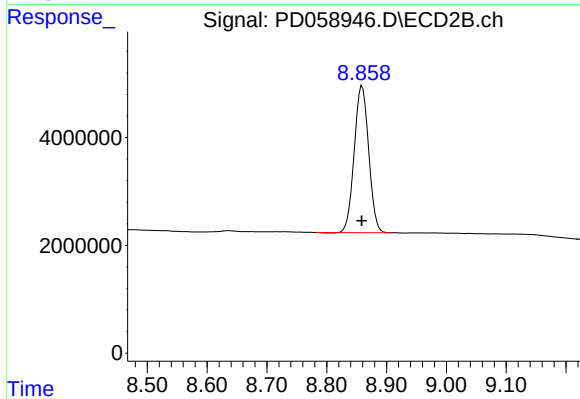

#27 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 45738090
Conc: 33.35 ng/ml