

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081324\
 Data File : PD084353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 09:52
 Operator : AR\AJ
 Sample : PIBLK049
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK212

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:11:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.929	21994400	136.1E6	26.235	25.848
27)	SA Decachlor...	9.116	8.141	45664118	98473516	26.254	26.204
Target Compounds							
7)	B delta-BHC	4.811	0.000	1636902	0	0.948	N.D. #
8)	B Heptachlo...	5.716	0.000	1583194	0	0.931	N.D. #
10)	B trans-Chl...	6.027f	0.000	1028107	0	0.623	N.D. #
11)	B cis-Chlor...	6.027f	0.000	1028107	0	0.597	N.D. #
15)	B Endosulfa...	6.812	0.000	2072520	0	1.257	N.D. #
26)	Toxaphene-5	0.000	7.440f	0	38561842	N.D.	703.186


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081324\
Data File : PD084353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 09:52
Operator : AR\AJ
Sample : PIBLK049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:11:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

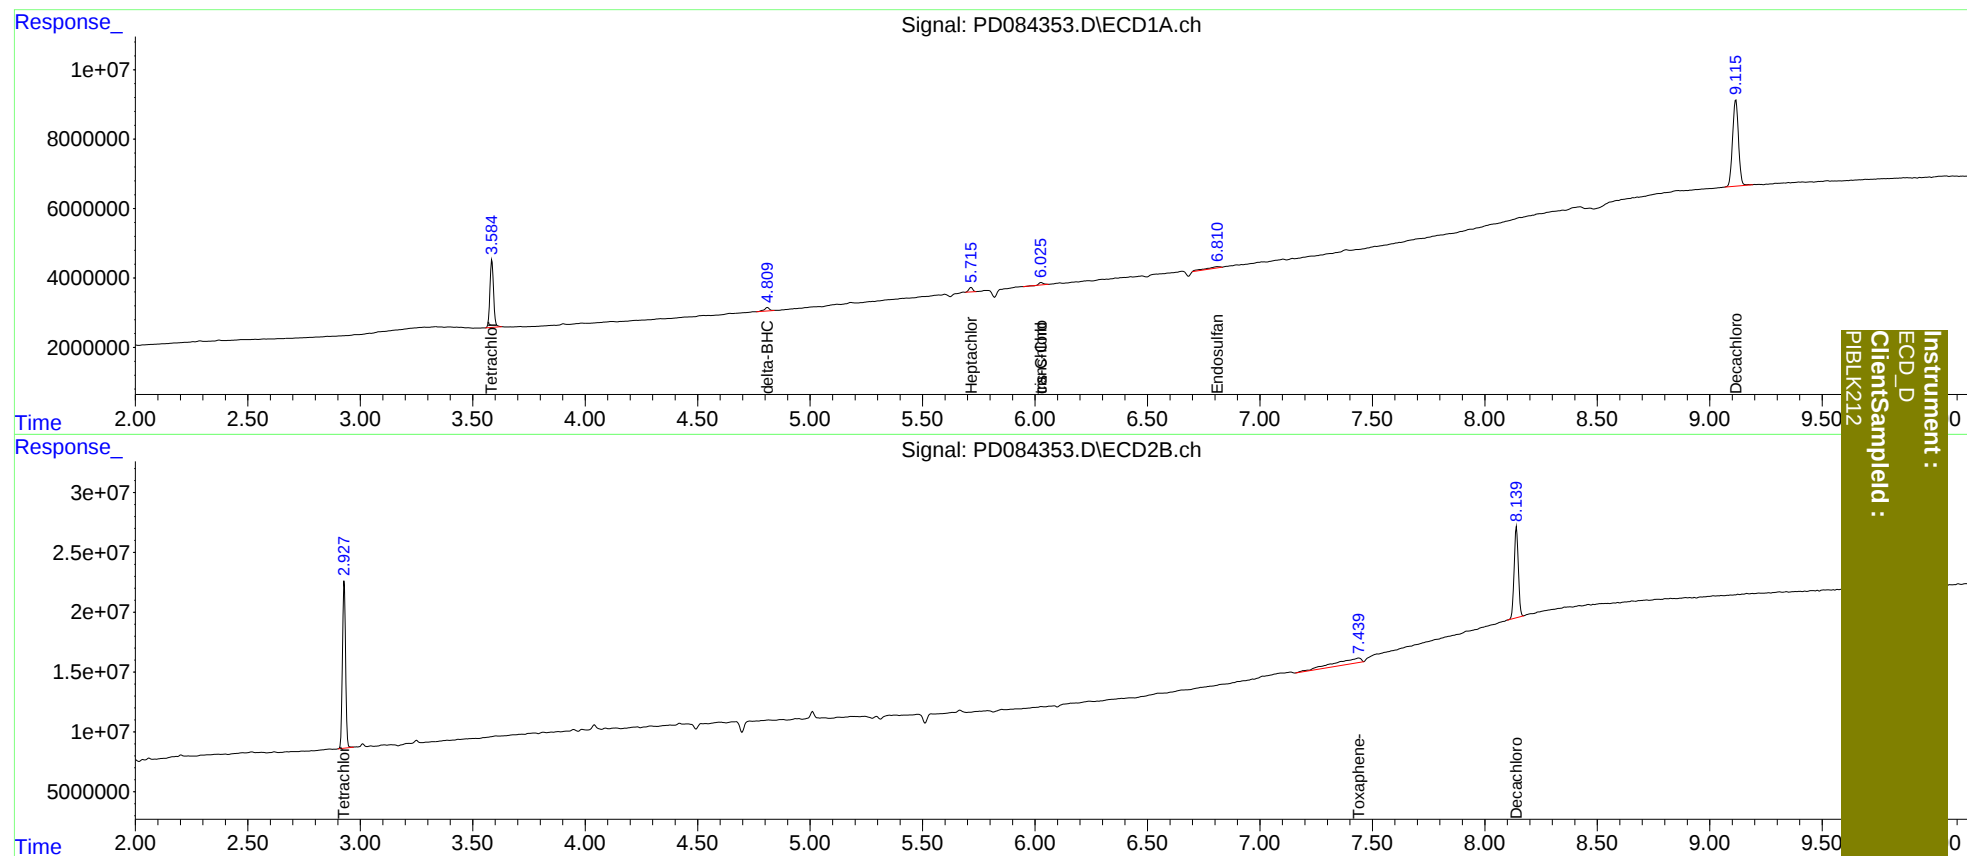


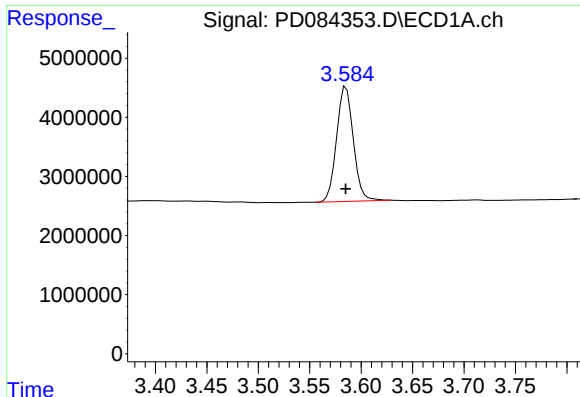

#1 Tetrachloro-m-xylene


R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 21994400
Conc: 26.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK212

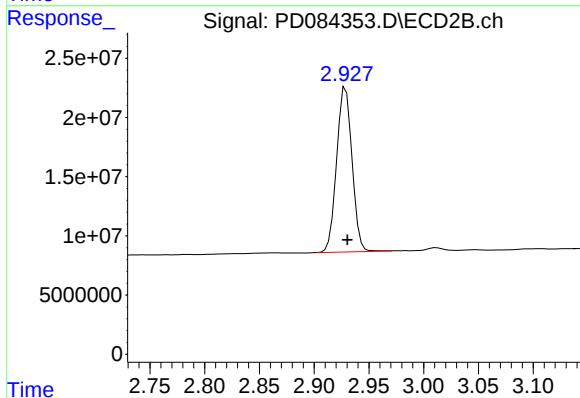


#1 Tetrachloro-m-xylene

R.T.: 2.929 min
Delta R.T.: -0.001 min
Response: 136065538
Conc: 25.85 ng/ml

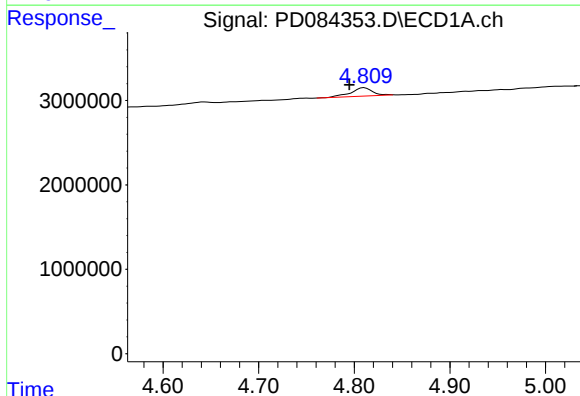


#7 delta-BHC

R.T.: 4.811 min
Delta R.T.: 0.016 min
Response: 1636902
Conc: 0.95 ng/ml

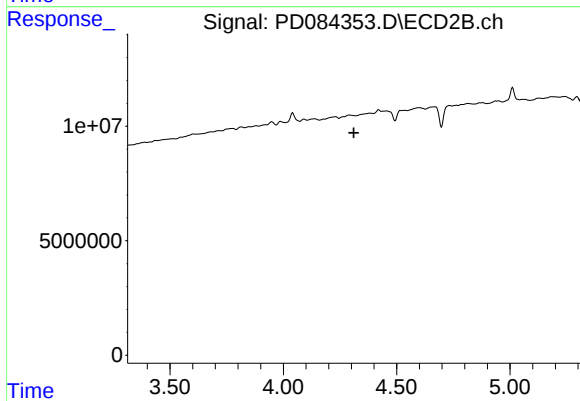

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.311 min
Response: 0
Conc: N.D.

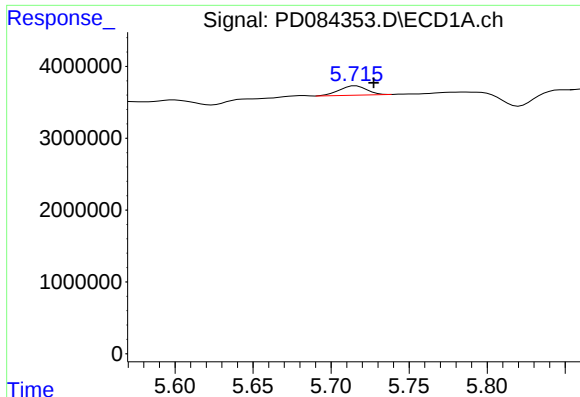

#8 Heptachlor epoxide


R.T.: 5.716 min
Delta R.T.: -0.012 min
Response: 1583194
Conc: 0.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK212

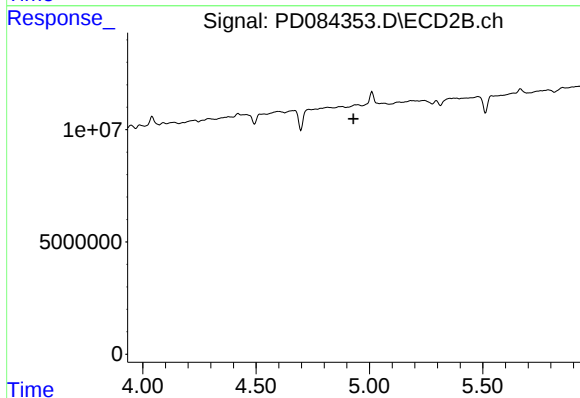


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.930 min
Response: 0
Conc: N.D.

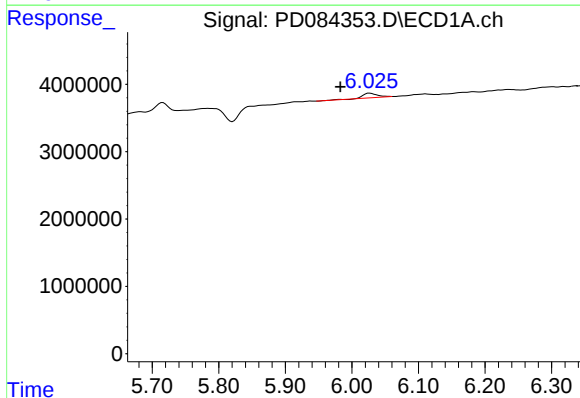


#10 trans-Chlordane

R.T.: 6.027 min
Delta R.T.: 0.045 min
Response: 1028107
Conc: 0.62 ng/ml

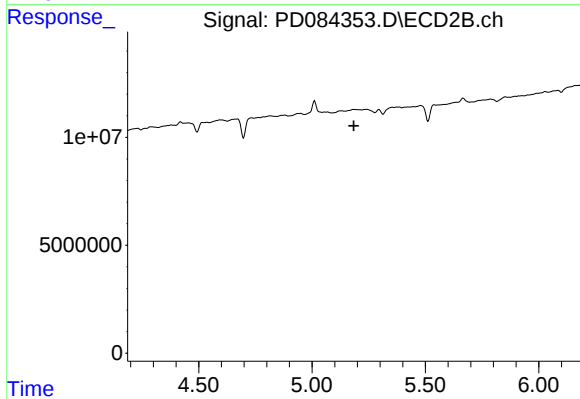

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

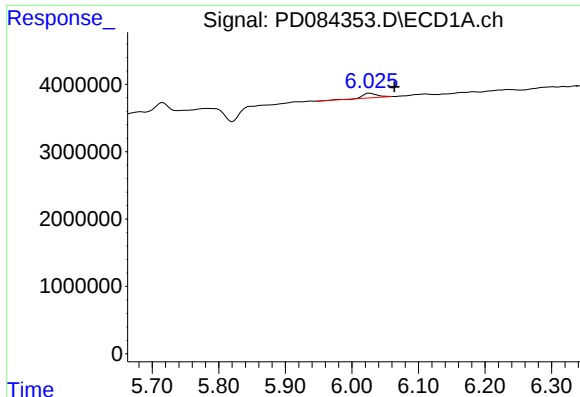

#11 cis-Chlordane


R.T.: 6.027 min
Delta R.T.: -0.037 min
Response: 1028107
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK212

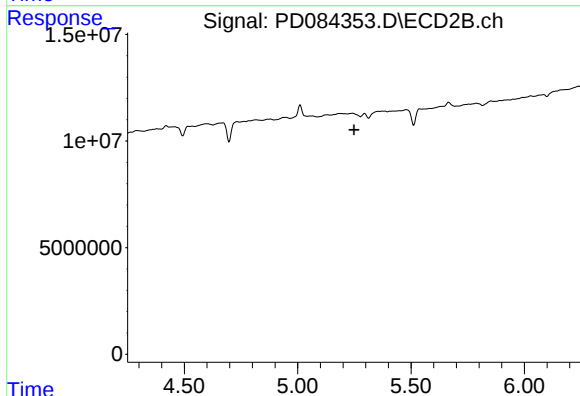


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

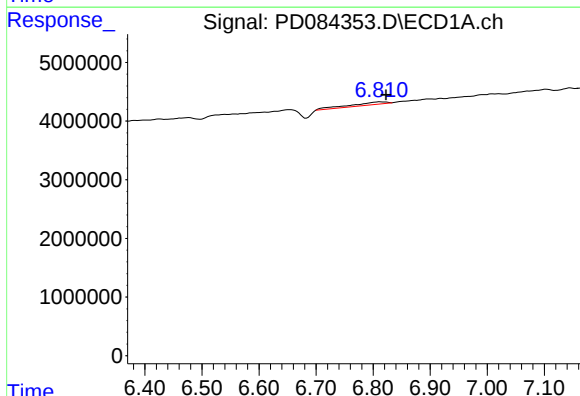


#15 Endosulfan II

R.T.: 6.812 min
Delta R.T.: -0.011 min
Response: 2072520
Conc: 1.26 ng/ml

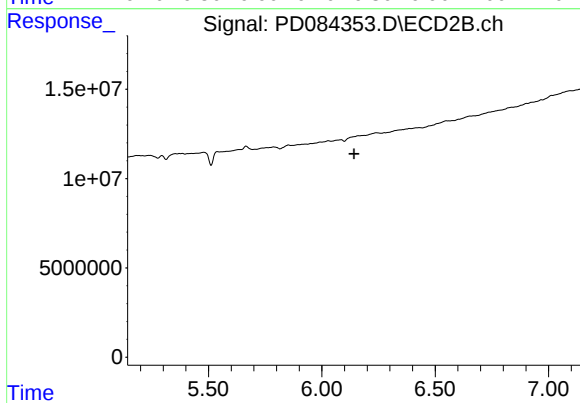

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.142 min
Response: 0
Conc: N.D.

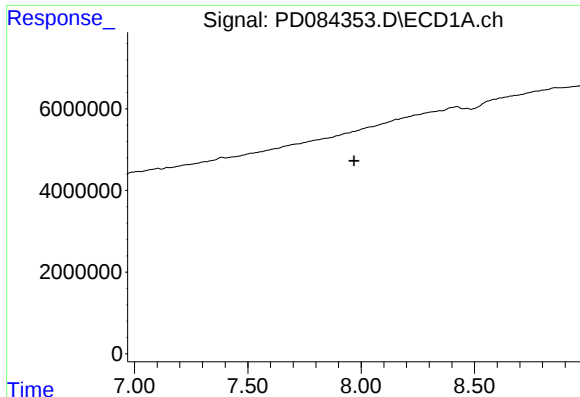

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK212

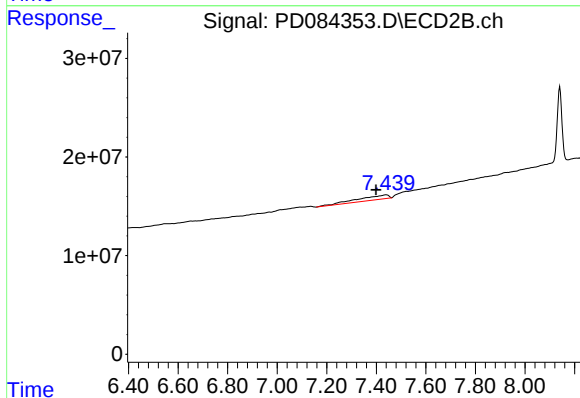


#26 Toxaphene-5

R.T.: 7.440 min
Delta R.T.: 0.041 min
Response: 38561842
Conc: 703.19 ng/ml

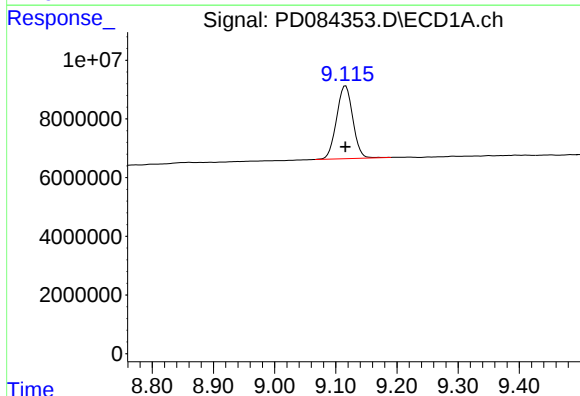

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 45664118
Conc: 26.25 ng/ml

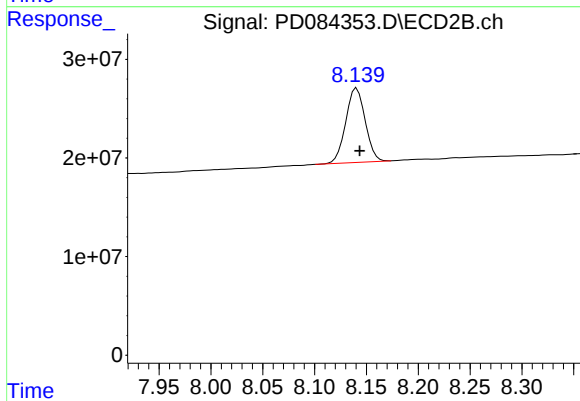

#27 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: -0.003 min
Response: 98473516
Conc: 26.20 ng/ml