

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081324\
 Data File : PD084390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 23:08
 Operator : AR\AJ
 Sample : P3502-23
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXW0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/14/2024
 Supervised By : Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:47:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.929	9336010	64710035	11.136m	12.293
27)	SA Decachlor...	9.114	8.139	13842085	28153172	7.958	7.492
Target Compounds							
3)	MA gamma-BHC...	4.362	3.778	1179300	2968178	0.757m	0.385m#
7)	B delta-BHC	4.805	4.306	3415907	6275384	1.978	0.748m#
15)	B Endosulfa...	6.818	6.135	1059634	5770671	0.643m	1.111m#
21)	B Endrin ke...	7.639	7.054	98811721	16976677	59.666	3.260m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081324\
Data File : PD084390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 23:08
Operator : AR\AJ
Sample : P3502-23
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:47:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

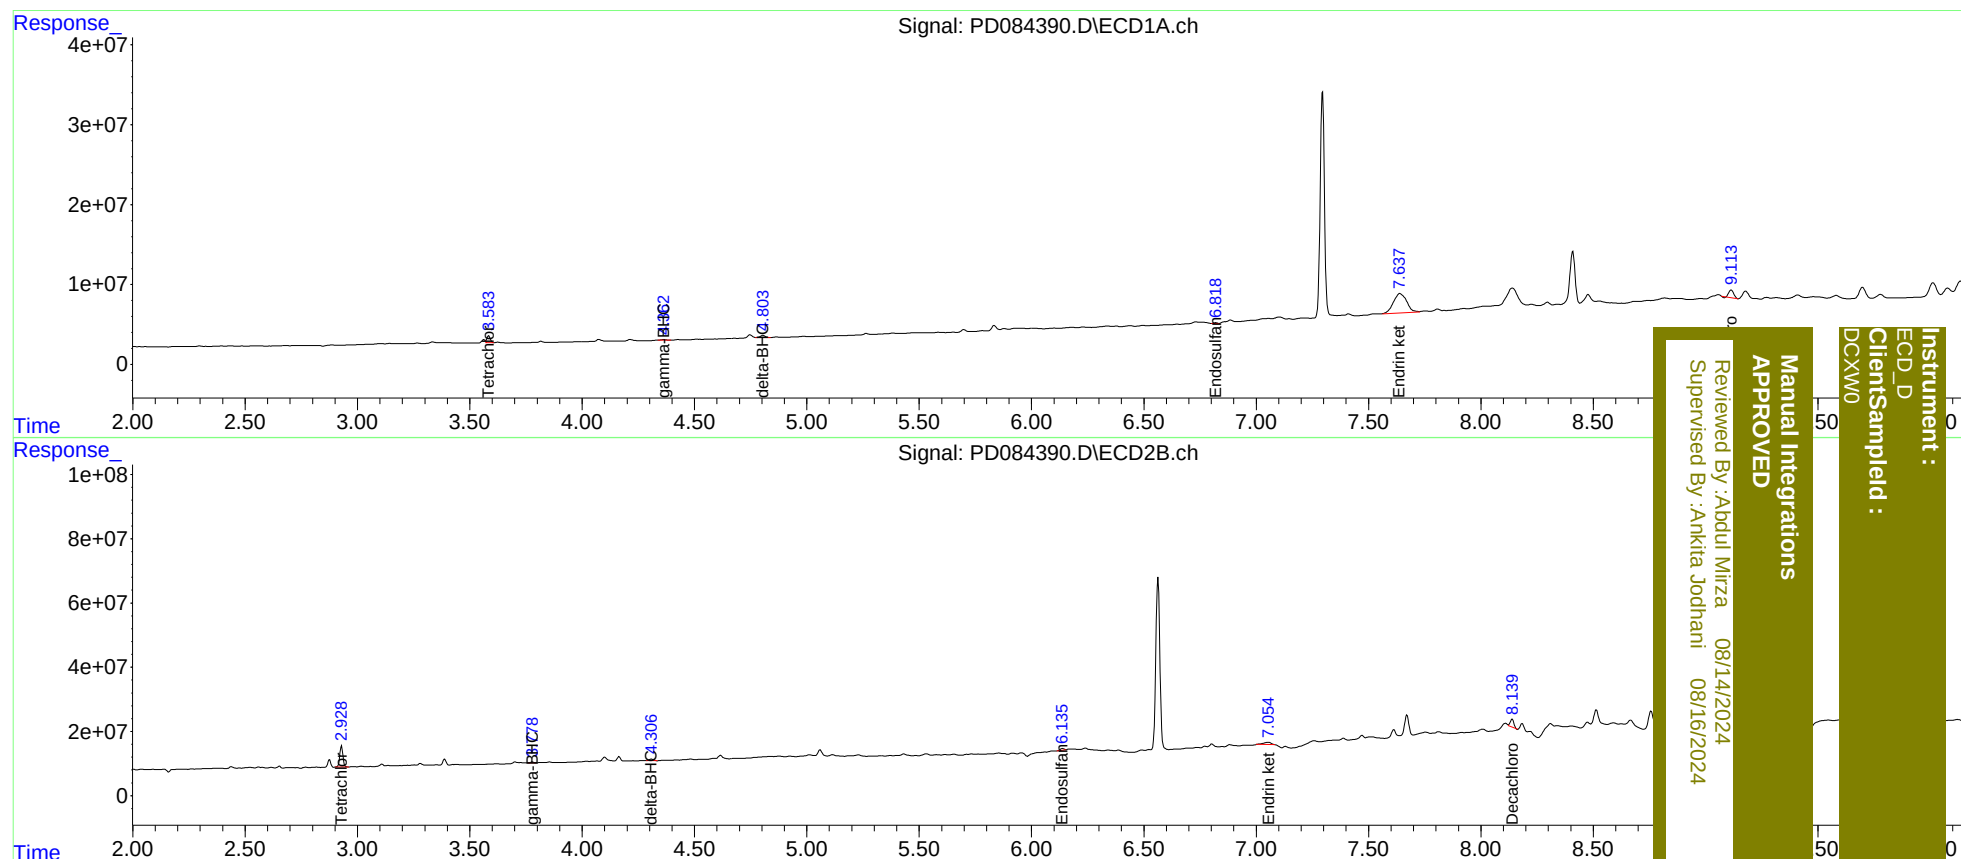

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/14/2024
Supervised By: Ankita Jodhani 08/16/2024

Instrument :
ECD_D
Client Sampled :
DCXW0