

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081325\
 Data File : PD089873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 18:22
 Operator : AR\AJ
 Sample : Q2830-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BIN0009-DRIVEWAY-TP-EASTSIDE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/13/2025
 Supervised By : mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:14:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.877	45213972	352.3E6	18.331	22.242m
28) SA Decachlor...	9.068	8.064	46771661	288.1E6	12.586	14.350m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081325\
Data File : PD089873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 18:22
Operator : AR\AJ
Sample : Q2830-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BIN0009-DRIVEWAY-TP-EASTSIDE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:14:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

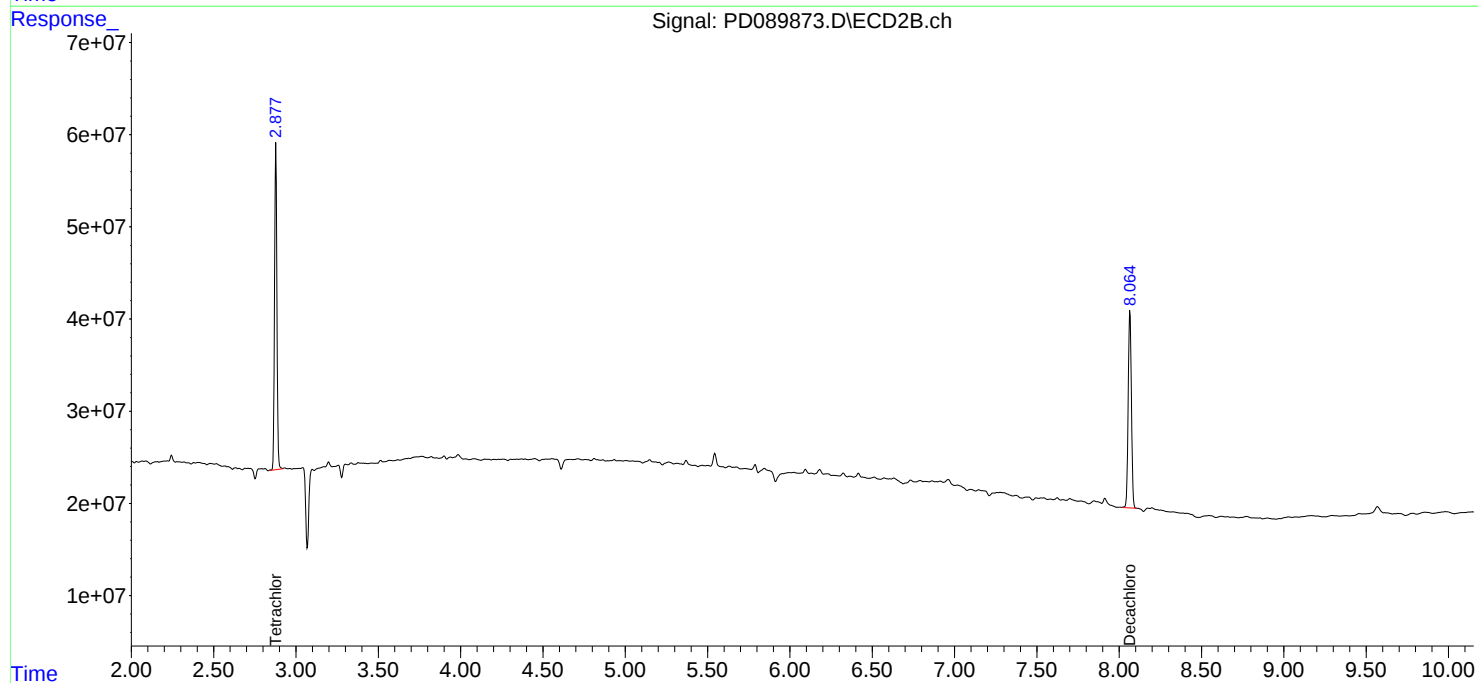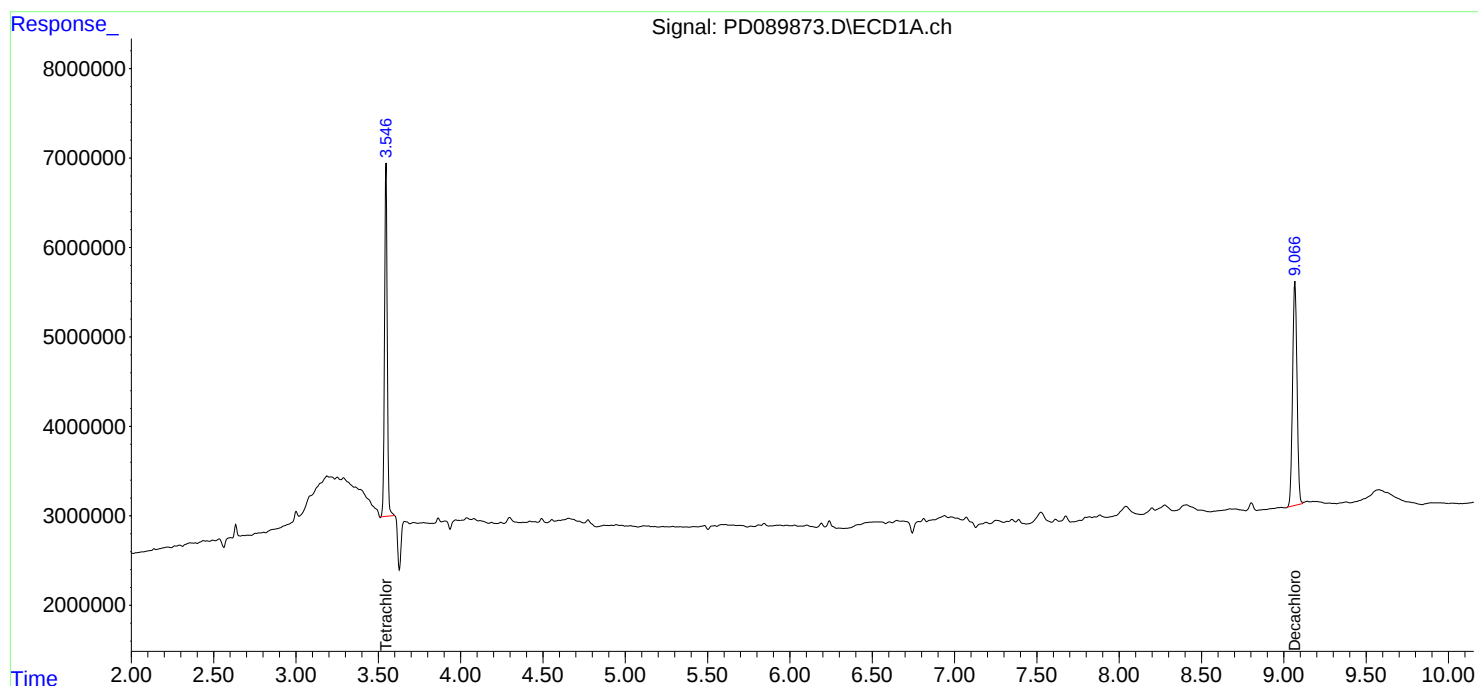

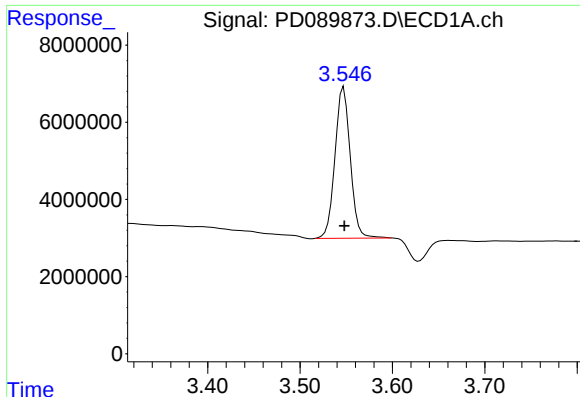


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 45213972
Conc: 18.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
BIN0009-DRIVEWAY-TP-EASTSIDE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

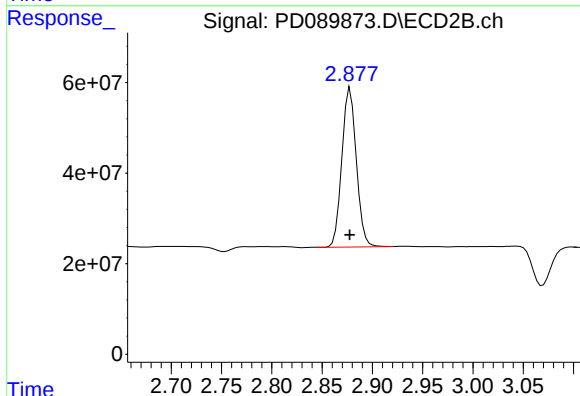


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 352260877
Conc: 22.24 ng/ml m

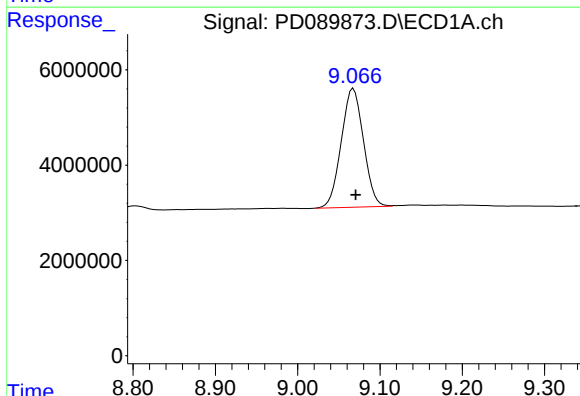

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.003 min
Response: 46771661
Conc: 12.59 ng/ml

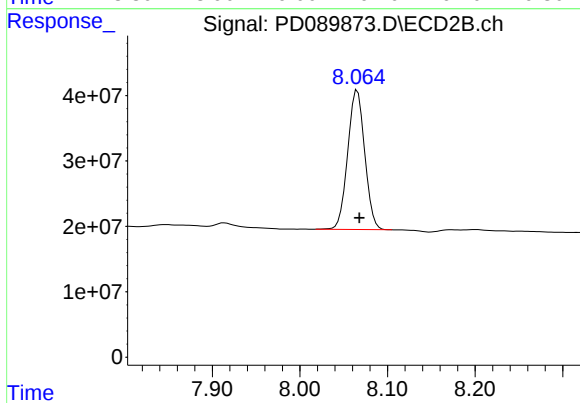

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: -0.004 min
Response: 288128999
Conc: 14.35 ng/ml m