

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081420\
 Data File : PD058953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 09:13
 Operator : DD\AJ
 Sample : PB130958BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:11:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	19361477	29476070	20.020	20.353
27)	SA Decachlor...	7.844	8.861	38386622	47052202	36.444	34.309
Target Compounds							
16)	A 4,4'-DDD	0.000	6.625f	0	1464741	N.D.	1.117

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081420\
Data File : PD058953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 09:13
Operator : DD\AJ
Sample : PB130958BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:11:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

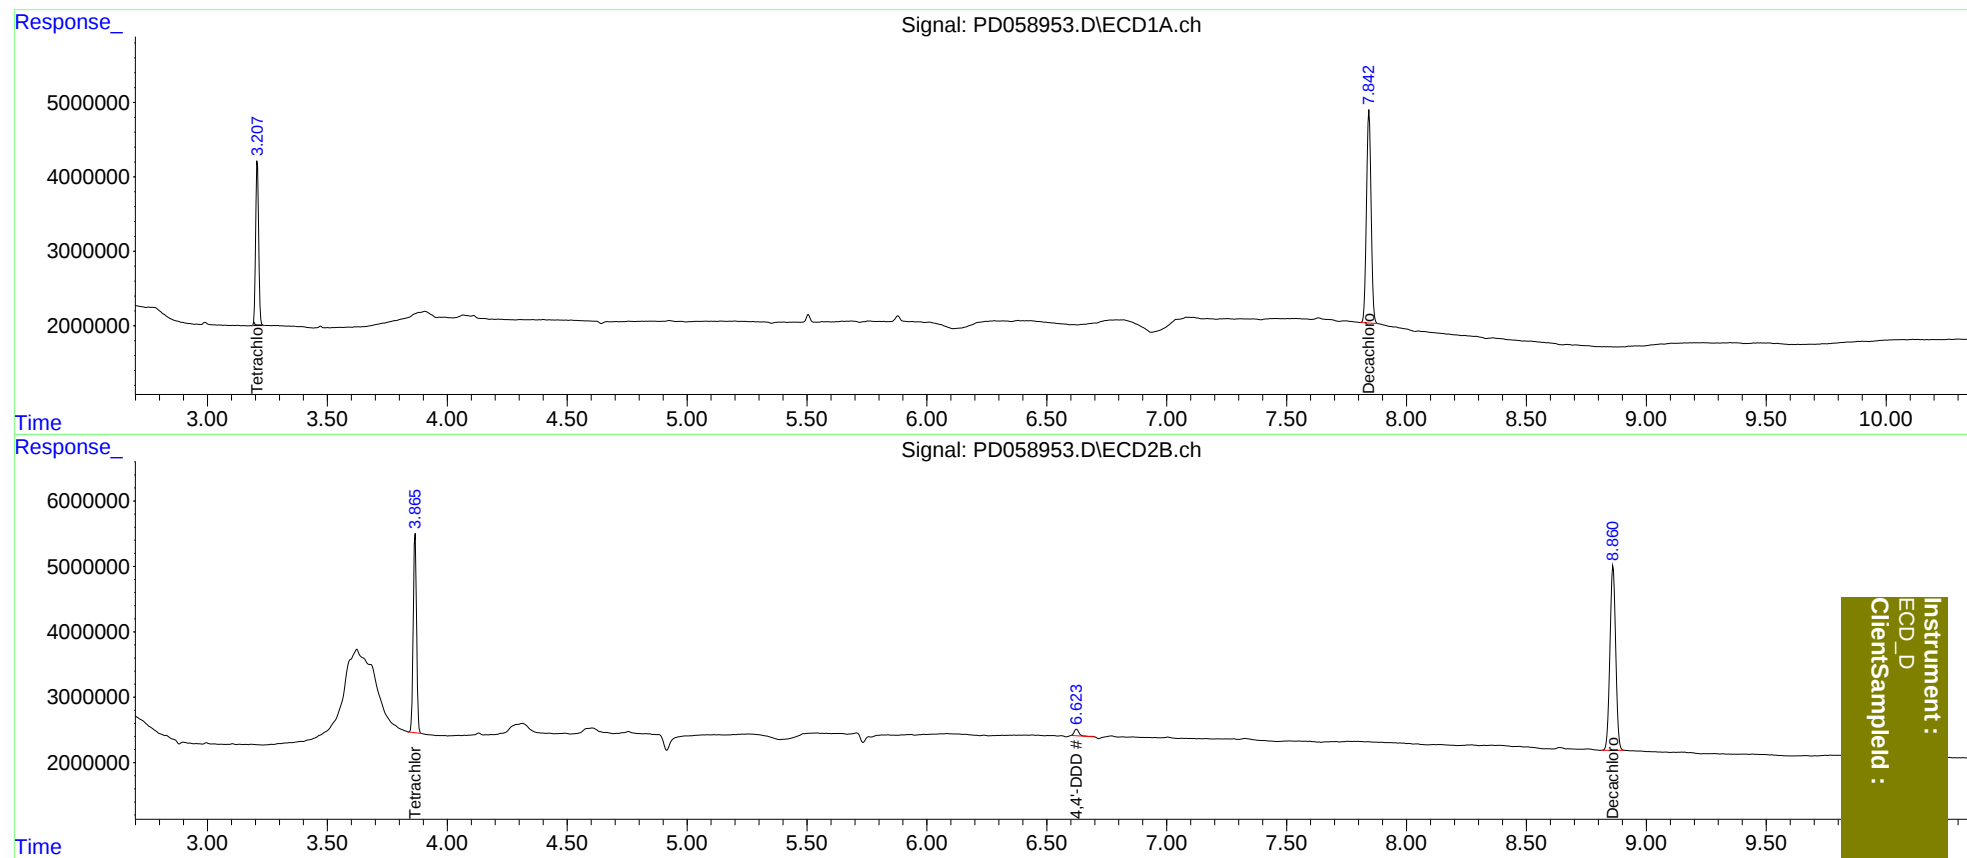


Instrument :
ECD_D
ClientSampleId :

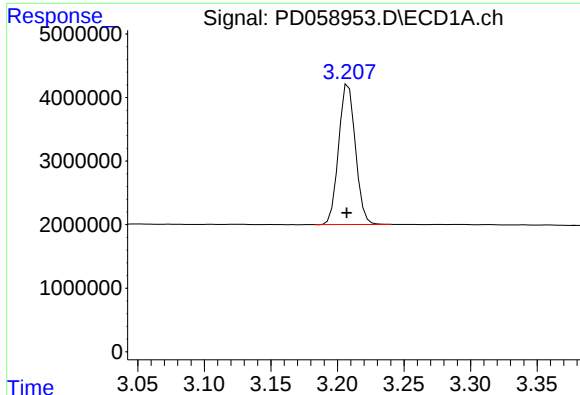

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.001 min
Response: 19361477
Conc: 20.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

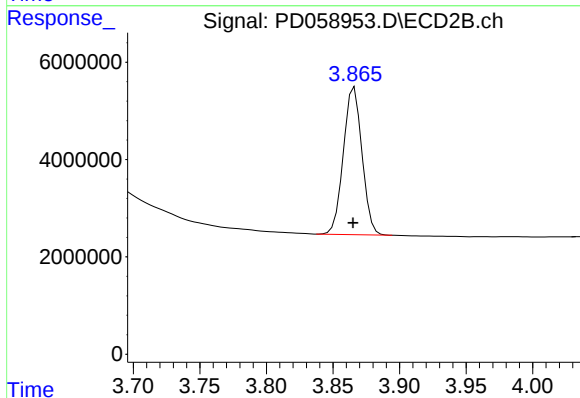


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.001 min
Response: 29476070
Conc: 20.35 ng/ml

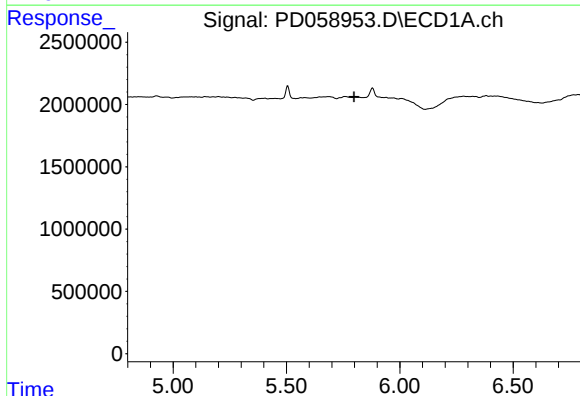


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.798 min
Response: 0
Conc: N.D.

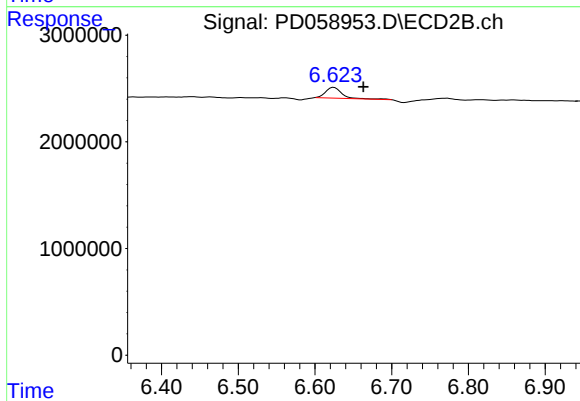

#16 4,4'-DDD

R.T.: 6.625 min
Delta R.T.: -0.039 min
Response: 1464741
Conc: 1.12 ng/ml

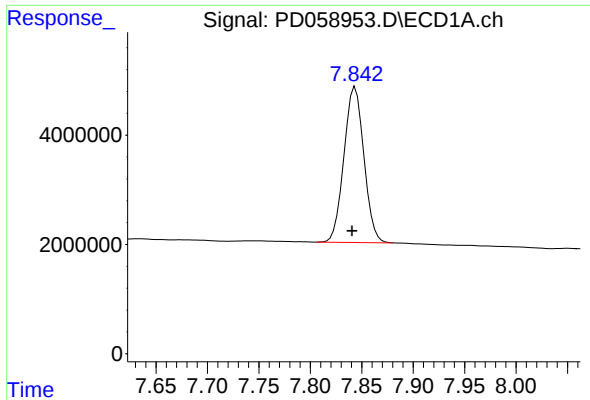

#27 Decachlorobiphenyl


R.T.: 7.844 min

Delta R.T.: 0.003 min

Response: 38386622

Conc: 36.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

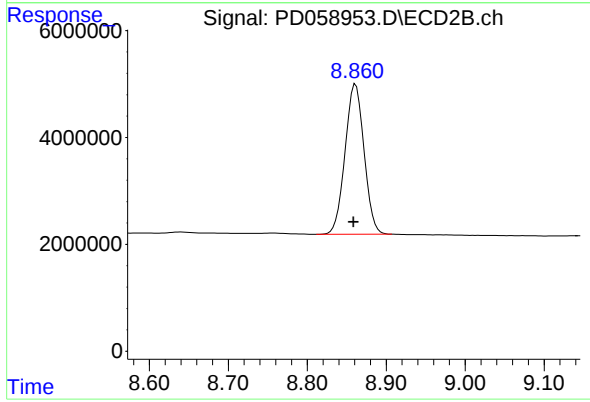

#27 Decachlorobiphenyl

R.T.: 8.861 min

Delta R.T.: 0.003 min

Response: 47052202

Conc: 34.31 ng/ml