

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081420\
 Data File : PD058958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 10:24
 Operator : DD\AJ
 Sample : L3647-06MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB7H5MS

Manual Integrations
 APPROVED

Ankita
 8/17/2020 11:00:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:58:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	18703259	29460306	19.340	20.342
27)	SA Decachlor...	7.840	8.861	30845196	37128448	29.284	27.073
Target Compounds							
3)	MA gamma-BHC...	3.900	4.527	62835963	86439915	45.212	45.477m
4)	MA Heptachlor	4.179	5.029	61372834	94292509	51.345	50.264
5)	MB Aldrin	4.414	5.328	62533003	85825229	50.384	46.491
10)	B trans-Chl...	5.064	5.942	654434	1649038	0.566m	0.990m#
11)	B cis-Chlor...	5.126	6.019	1649728	869539	1.417	0.516 #
13)	MA Dieldrin	5.410	6.320	132.1E6	180.9E6	108.773	108.059
14)	MA Endrin	5.661	6.535	110.5E6	147.4E6	111.236	108.632
17)	MA 4,4'-DDT	6.032	6.960	104.1E6	125.7E6	115.740	95.267m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081420\
Data File : PD058958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 10:24
Operator : DD\AJ
Sample : L3647-06MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:58:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

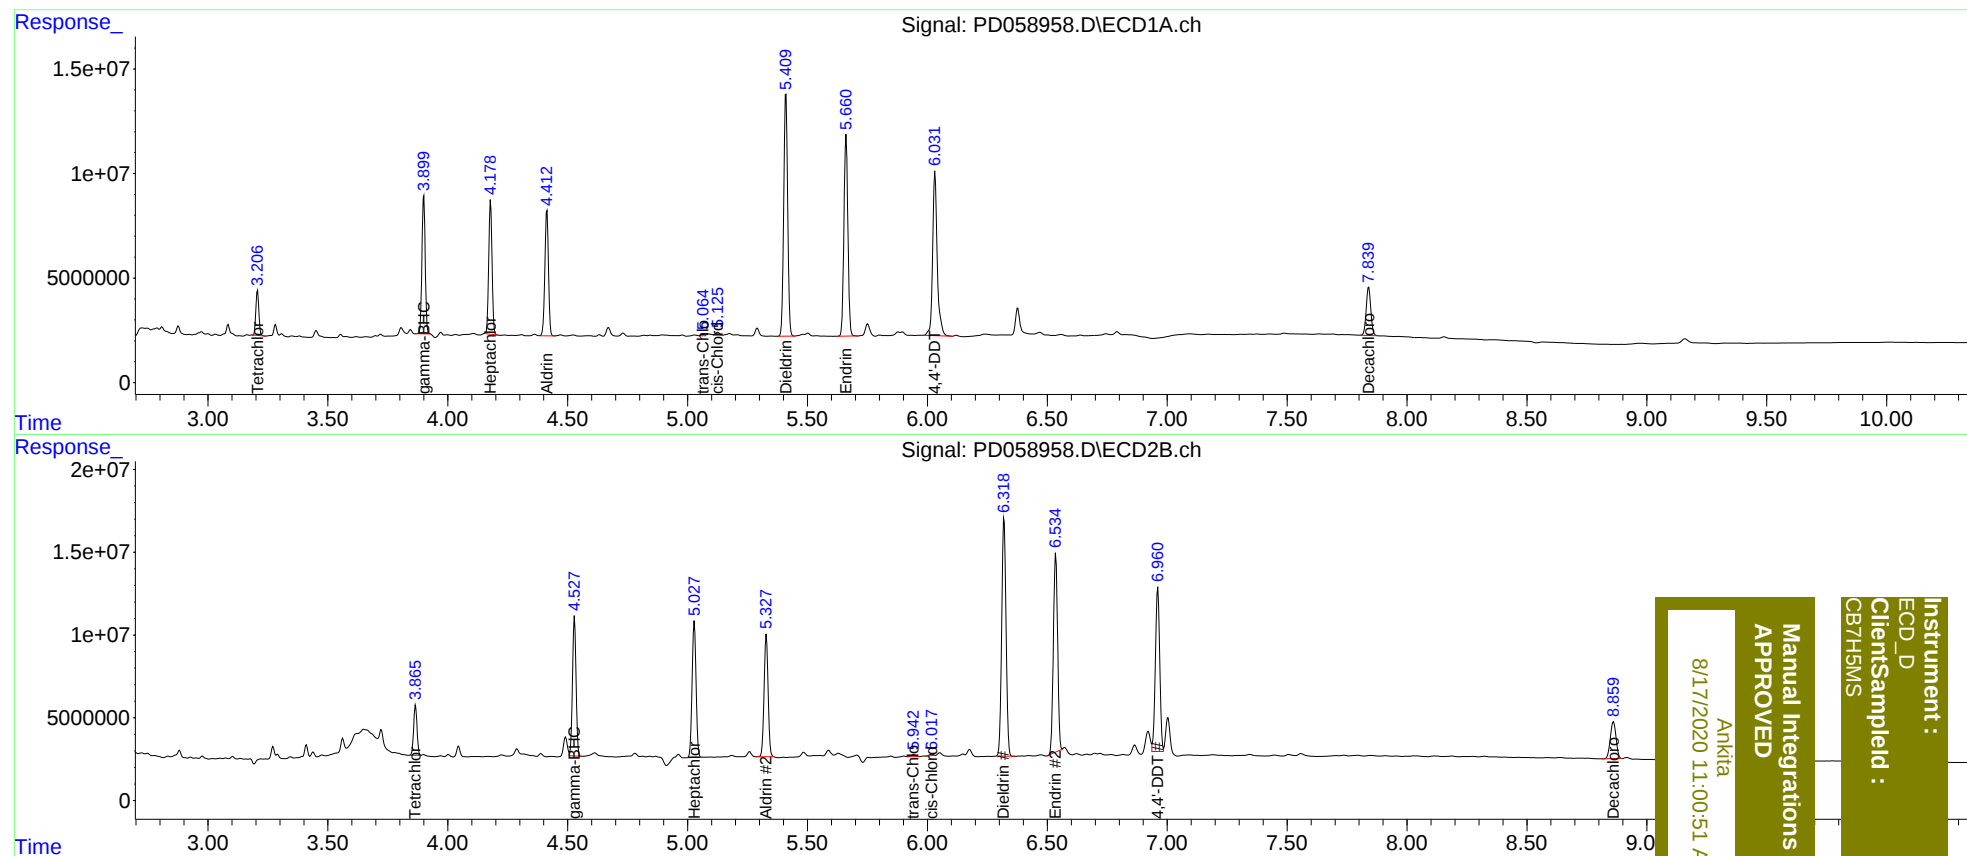

8/17/2020 11:00:51 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
CB7H5MS