

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 01:23
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:26:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 06:24:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds						
6) B	beta-BHC	4.499	4.900f	8709319	22675676	7.003 N.D. #
8) B	Heptachlo...	0.000	5.900	0	68667268	N.D. 2.685 #
9) A	Endosulfan I	0.000	6.261	0	10681769	N.D. 0.453 #
10) B	gamma-Chl...	0.000	6.109f	0	59633968	N.D. 2.283 #
11) B	alpha-Chl...	0.000	6.206	0	22216683	N.D. 0.876 #
25)	Chlordane-3	0.000	6.109f	0	59633968	N.D. 17.111 #
26)	Chlordane-4	0.000	6.206	0	22216683	N.D. 5.464 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 01:23
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:26:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 06:24:32 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50 μ m

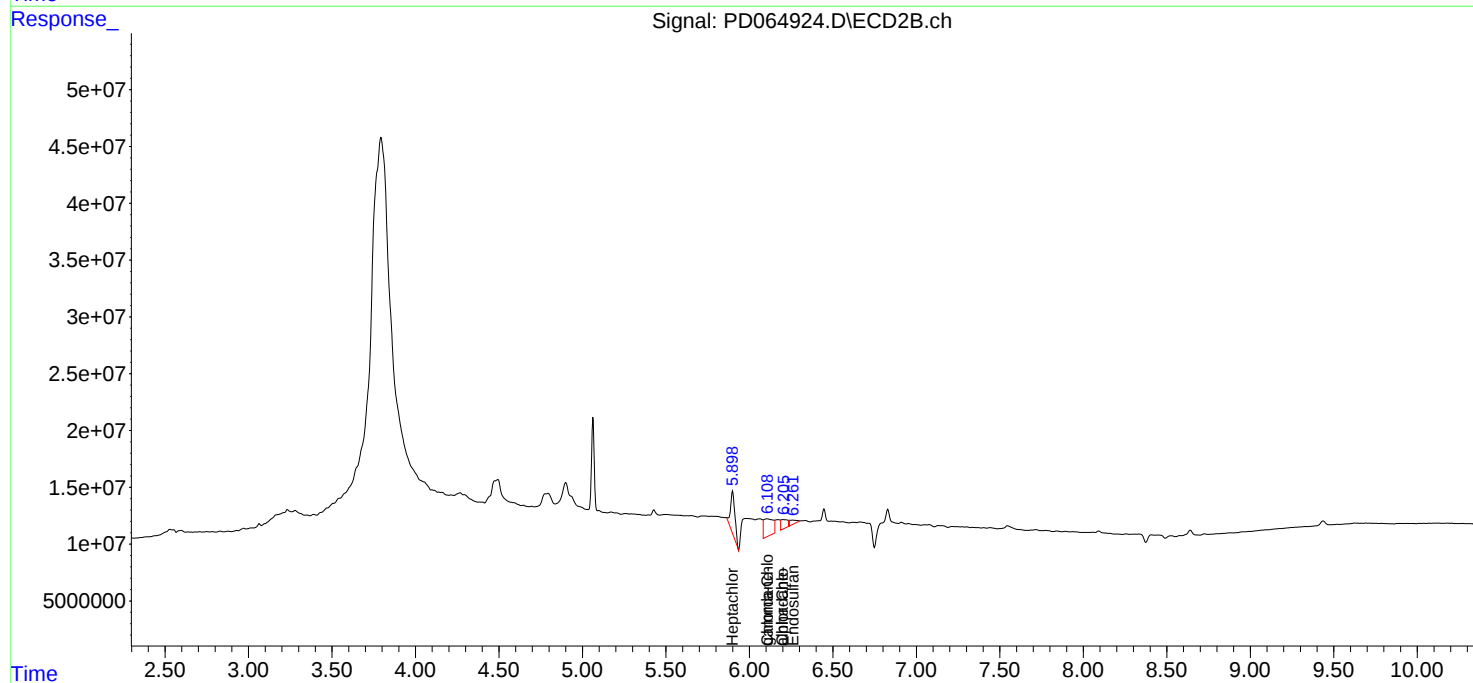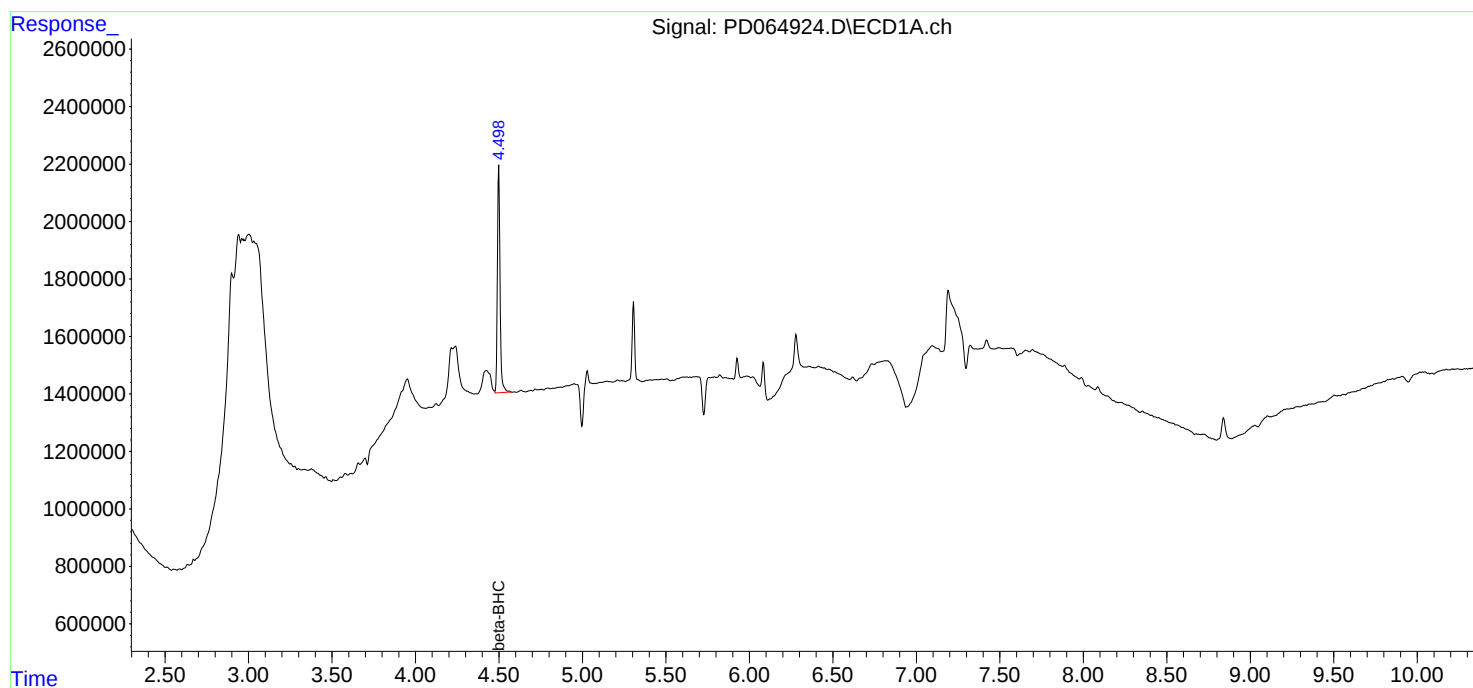

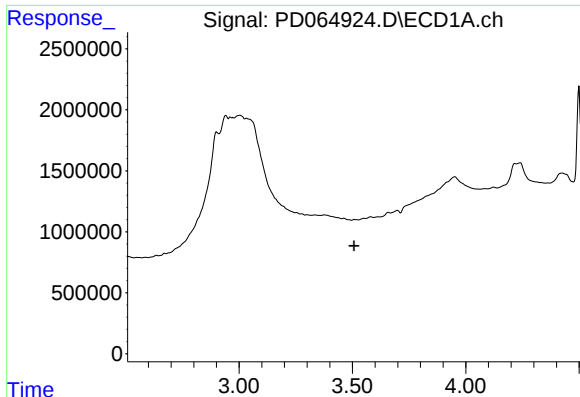


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.508 min
Response: 0
Conc: N.D.

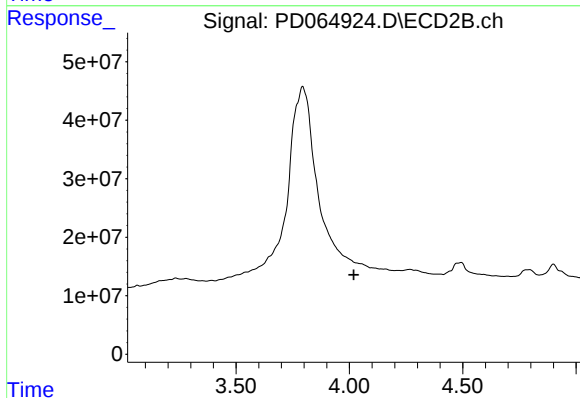


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.020 min
Response: 0
Conc: N.D.

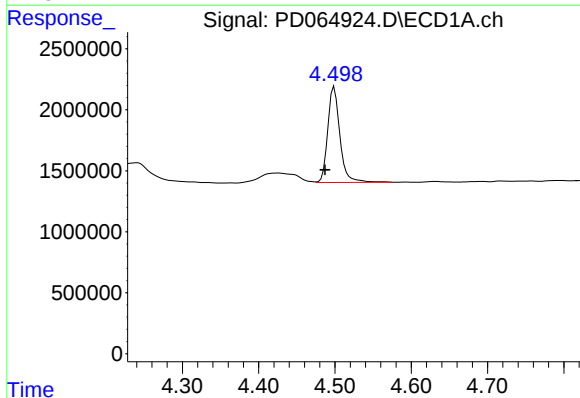


#6 beta-BHC

R.T.: 4.499 min
Delta R.T.: 0.012 min
Response: 8709319
Conc: 7.00 ng/ml

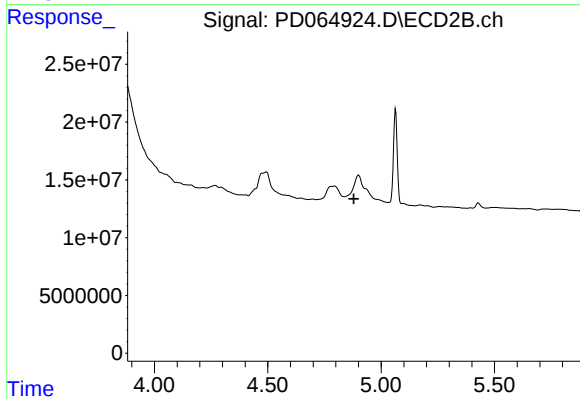


#6 beta-BHC

R.T.: 4.900 min
Delta R.T.: 0.021 min
Response: 22675676
Conc: N.D.

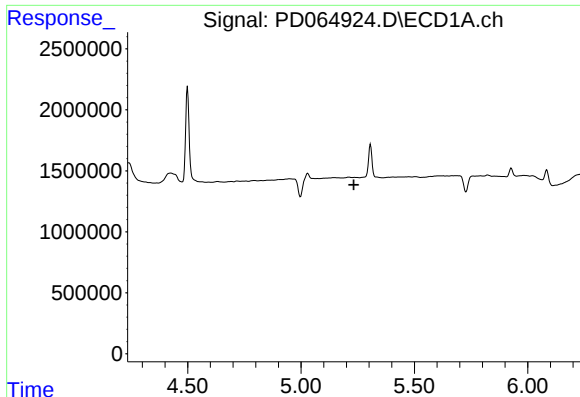


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

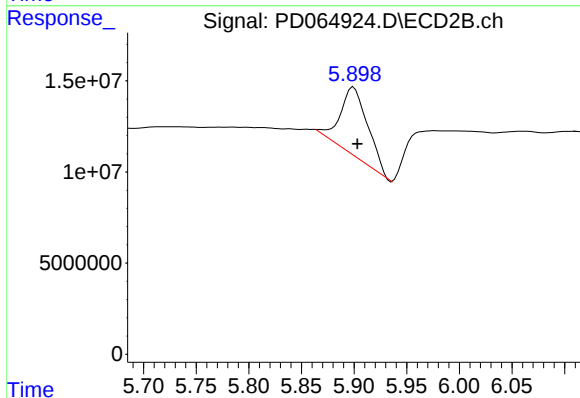


#8 Heptachlor epoxide

R.T.: 5.900 min
Delta R.T.: -0.003 min
Response: 68667268
Conc: 2.69 ng/ml

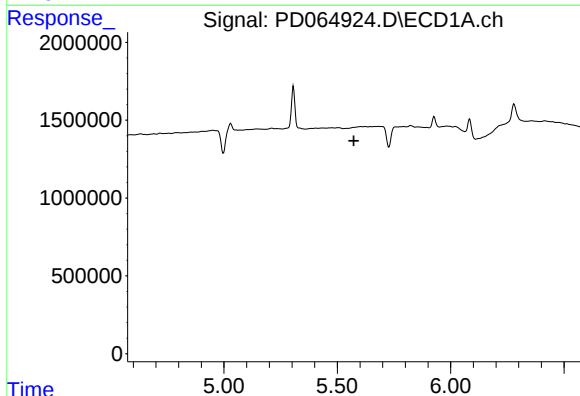


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.572 min
Response: 0
Conc: N.D.

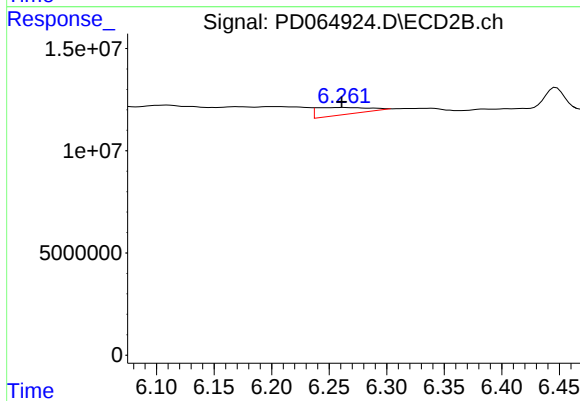


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 10681769
Conc: 0.45 ng/ml

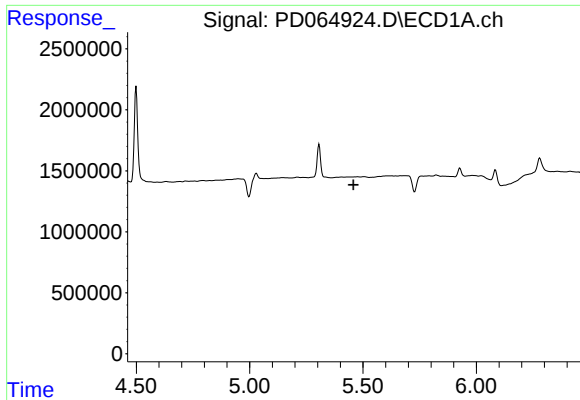


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

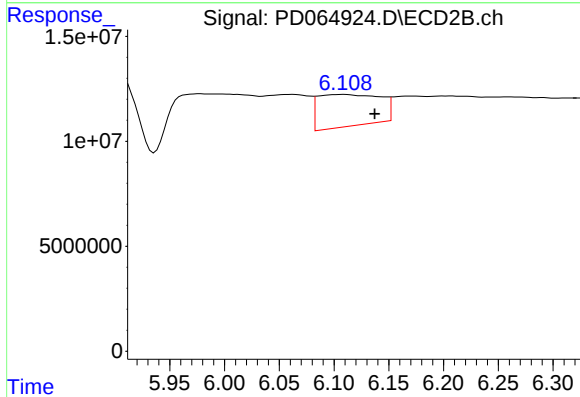


#10 gamma-Chlordane

R.T.: 6.109 min
Delta R.T.: -0.028 min
Response: 59633968
Conc: 2.28 ng/ml

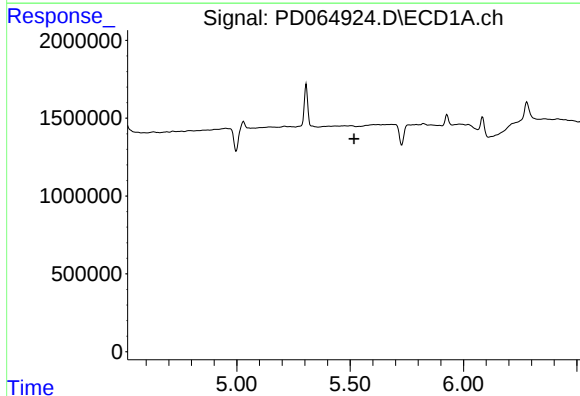


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.517 min
Response: 0
Conc: N.D.

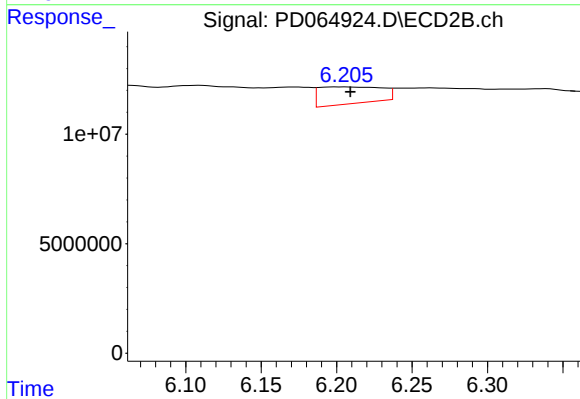


#11 alpha-Chlordane

R.T.: 6.206 min
Delta R.T.: -0.003 min
Response: 22216683
Conc: 0.88 ng/ml

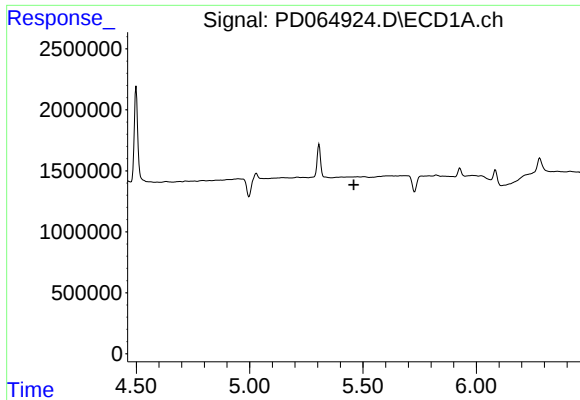


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

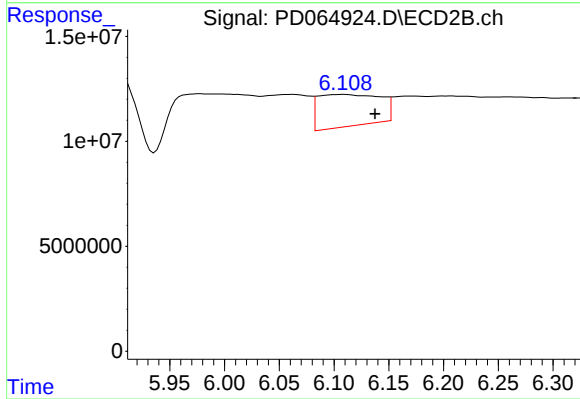


#25 Chlordane-3

R.T.: 6.109 min
Delta R.T.: -0.028 min
Response: 59633968
Conc: 17.11 ng/ml

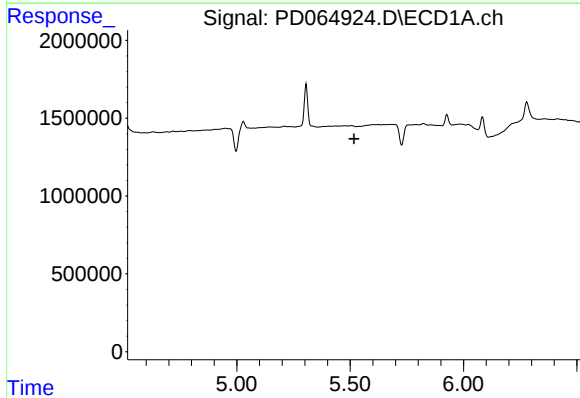


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.518 min
Response: 0
Conc: N.D.

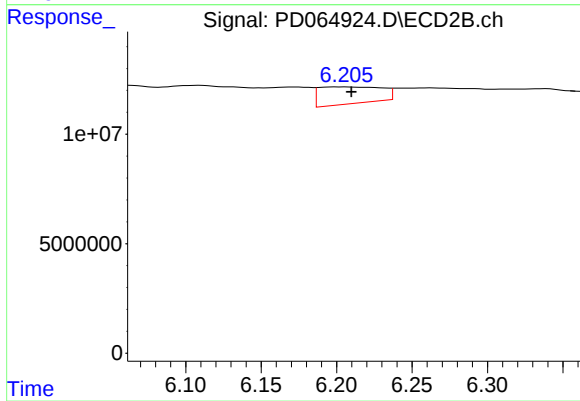


#26 Chlordane-4

R.T.: 6.206 min
Delta R.T.: -0.004 min
Response: 22216683
Conc: 5.46 ng/ml

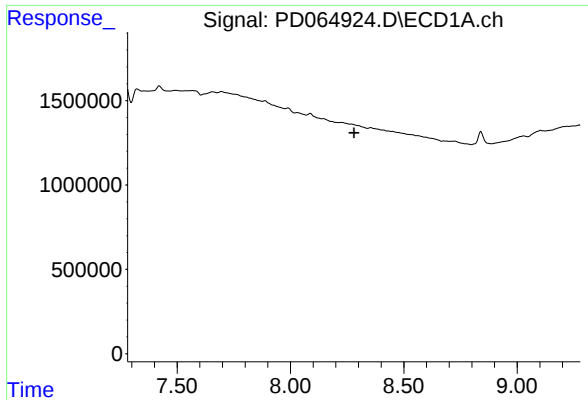

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.280 min
Response: 0
Conc: N.D.

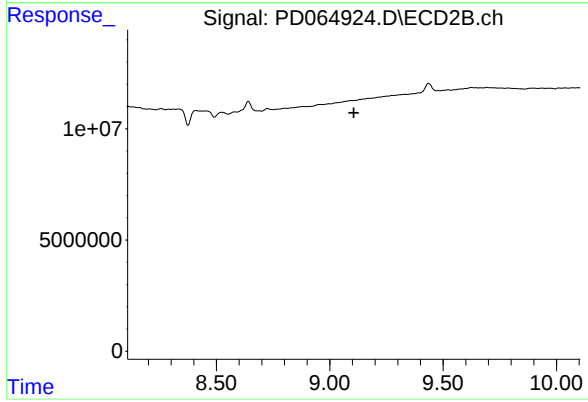

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.106 min
Response: 0
Conc: N.D.