

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 01:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:26:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 06:24:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.020	37704180	403.5E6	19.293	19.868
28)	SA Decachlor...	8.281	9.105	48283248	231.6E6	19.647	20.838
Target Compounds							
15)	B Endosulfa...	0.000	6.953	0	2558604	N.D.	0.133 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 01:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:26:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 06:24:32 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

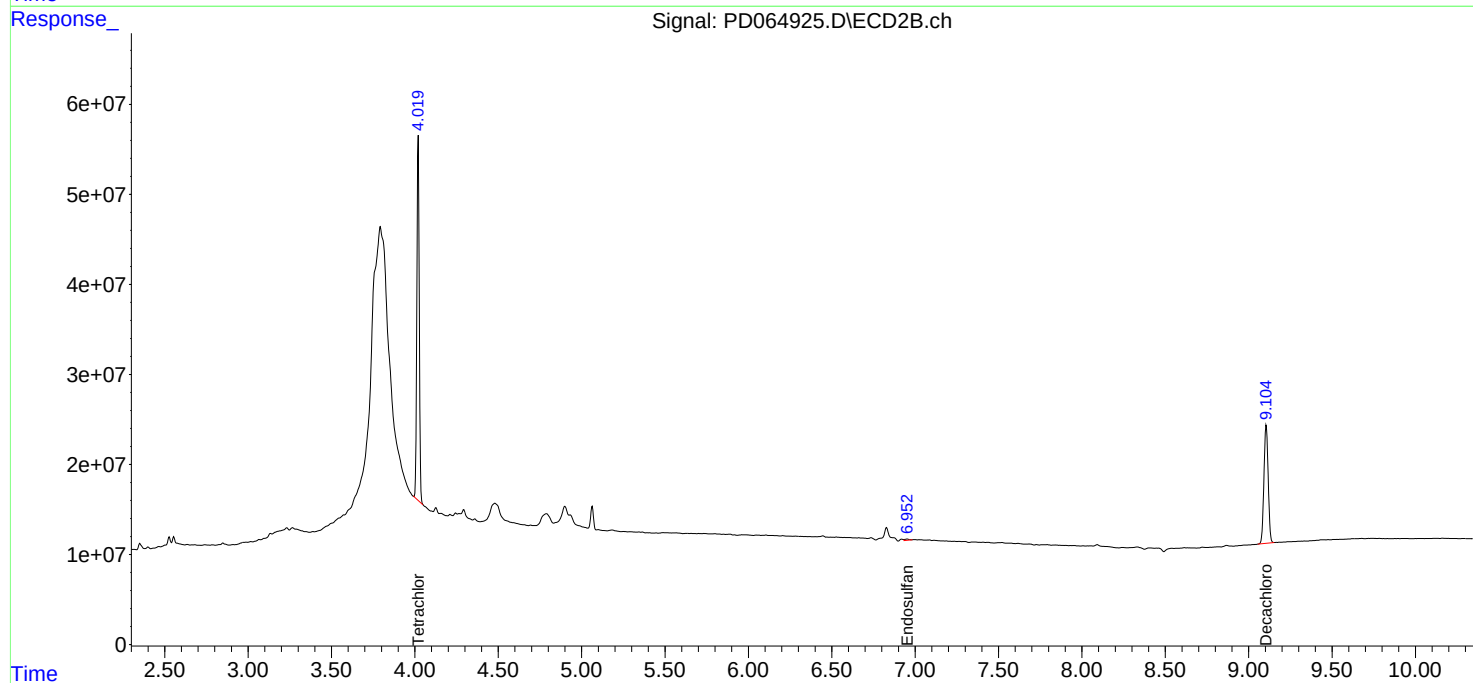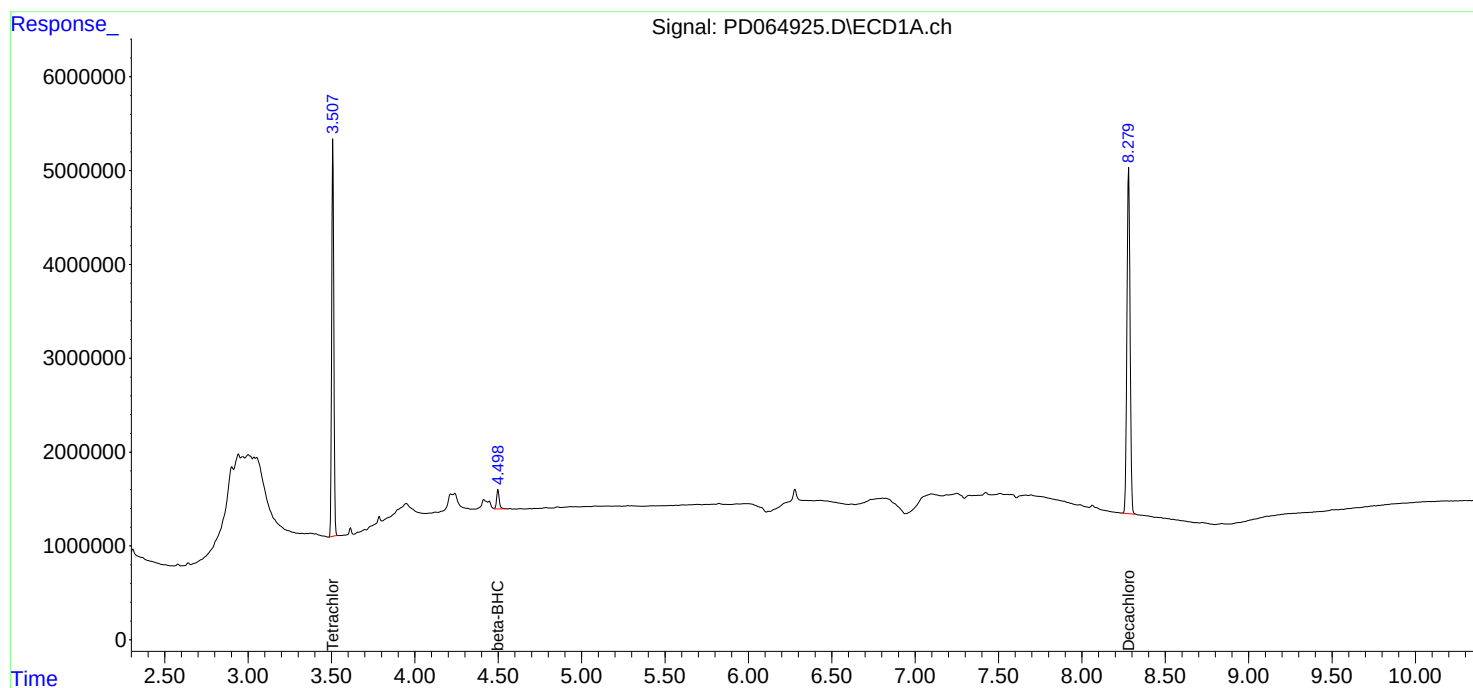

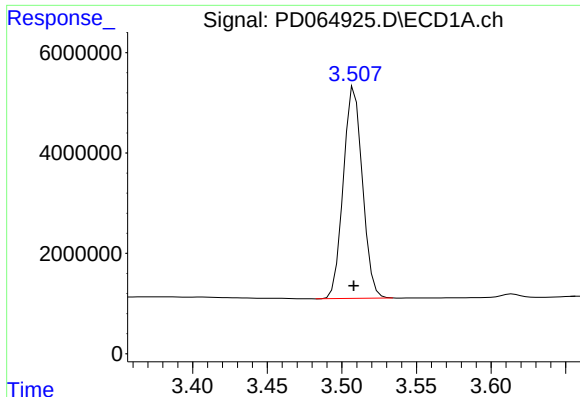


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 37704180
Conc: 19.29 ng/ml

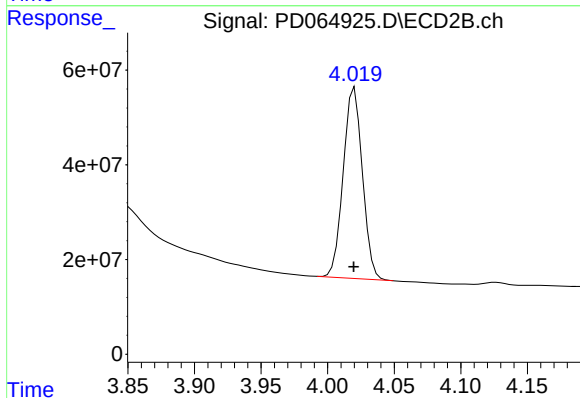


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 403469152
Conc: 19.87 ng/ml

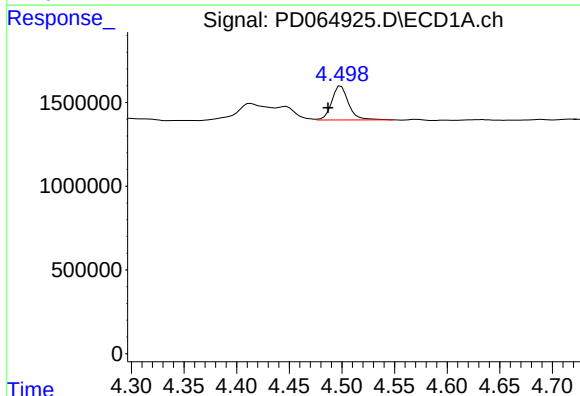


#6 beta-BHC

R.T.: 4.499 min
Delta R.T.: 0.012 min
Response: 2255987
Conc: 1.81 ng/ml

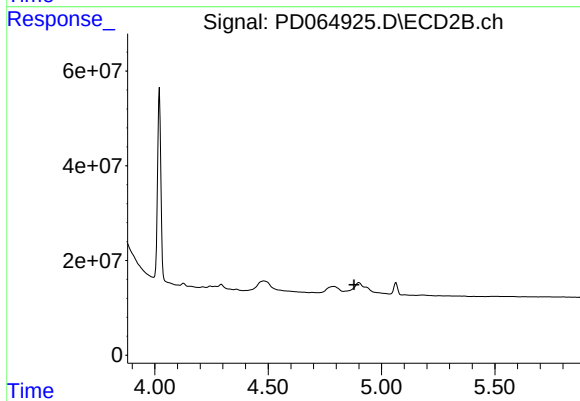


#6 beta-BHC

R.T.: 4.900 min
Delta R.T.: 0.021 min
Response: 20328743
Conc: N.D.

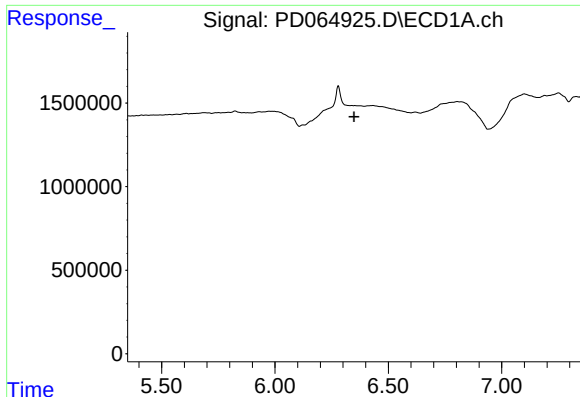


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

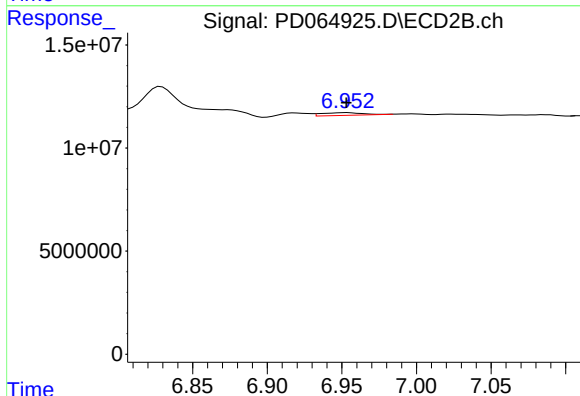


#15 Endosulfan II

R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 2558604
Conc: 0.13 ng/ml

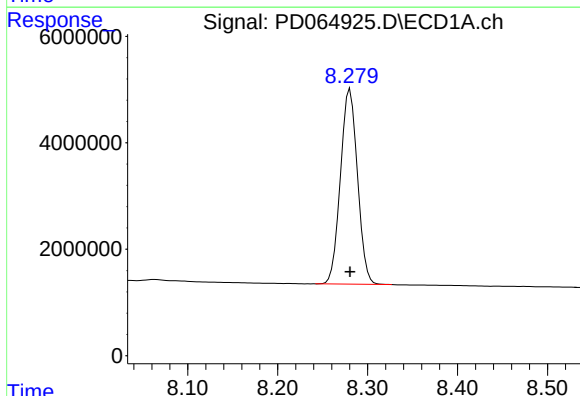

#28 Decachlorobiphenyl

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 48283248
Conc: 19.65 ng/ml

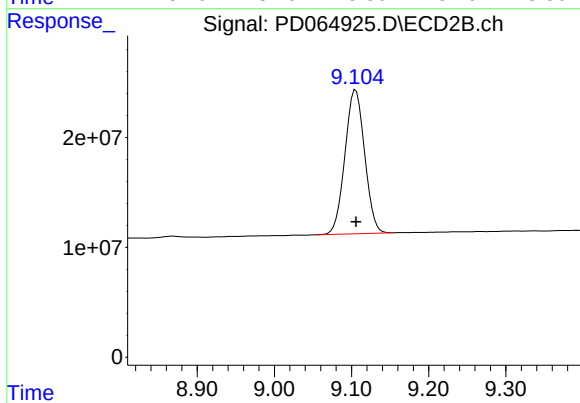

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 231596611
Conc: 20.84 ng/ml