

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 03:27
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:56:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 04:55:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	226.3E6	1894.0E6	98.636	93.954
28)	SA Decachlor...	8.280	9.106	225.7E6	997.3E6	94.757	91.948
Target Compounds							
23)	Chlordane-1	4.386	5.018	70430540	836.2E6	969.467	932.694
24)	Chlordane-2	4.889	5.488	80951065	755.1E6	931.413	908.746
25)	Chlordane-3	5.460	6.138	255.5E6	3182.8E6	989.255	949.005
26)	Chlordane-4	5.519	6.211	203.7E6	3668.2E6	979.058	943.254
27)	Chlordane-5	6.359	7.023	91712521	686.0E6	976.618	939.525


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 03:27
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:56:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 04:55:08 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

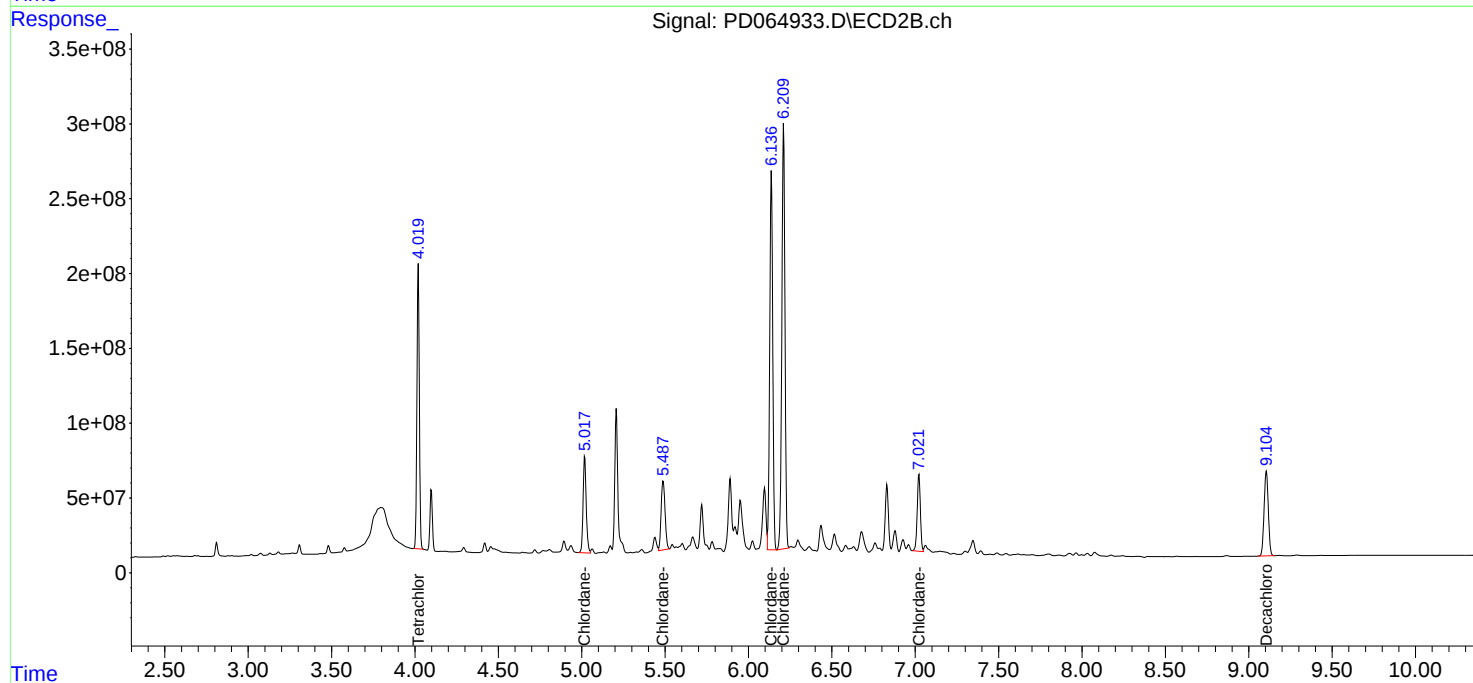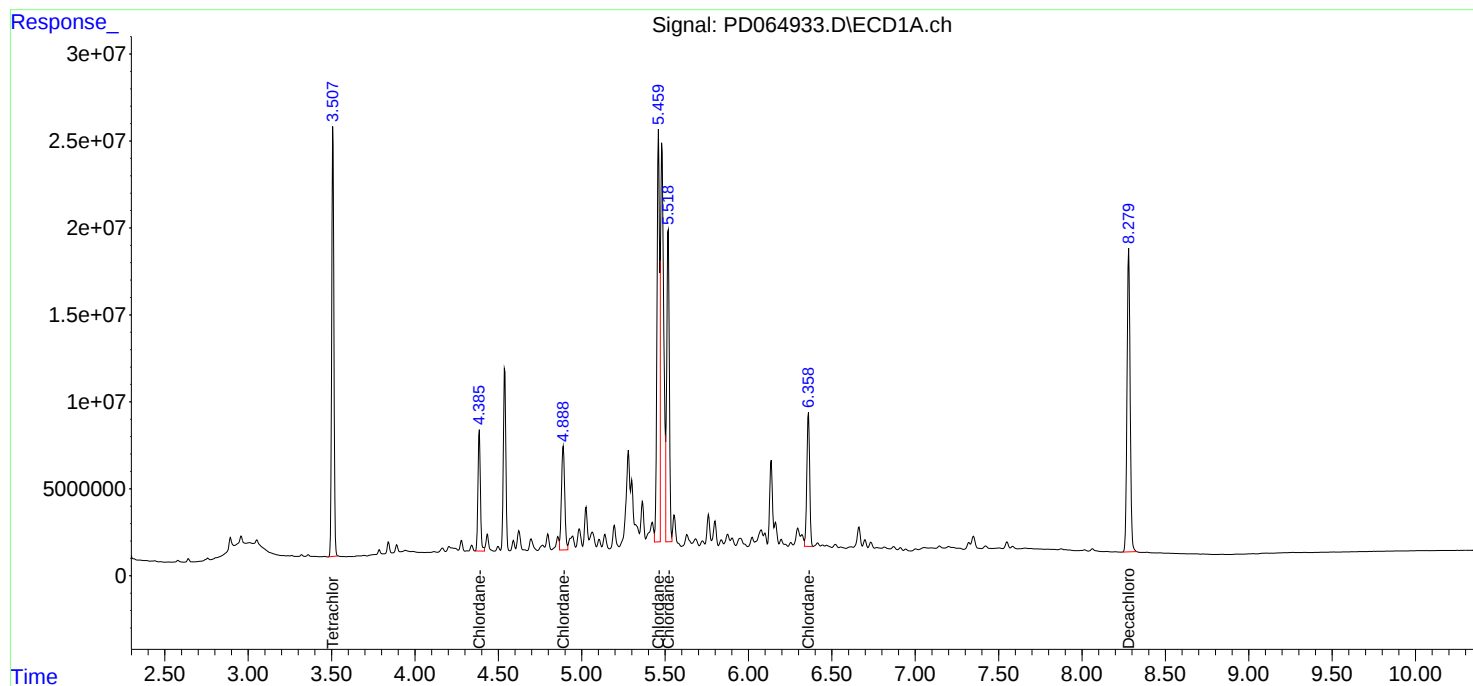

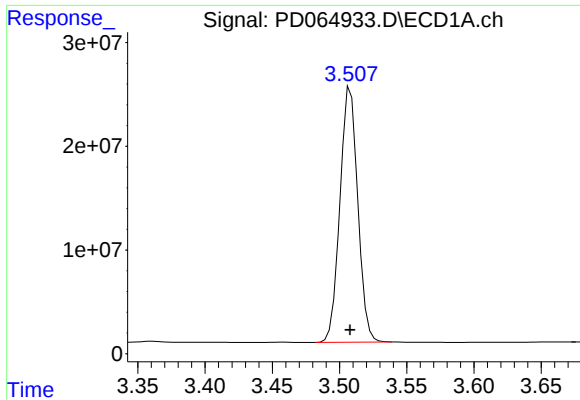


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 226277932
Conc: 98.64 ng/ml

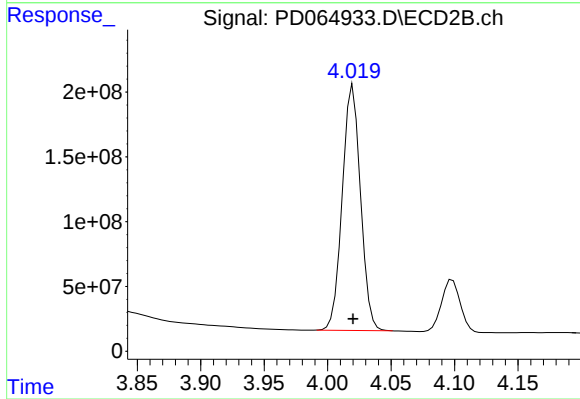


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 1894046385
Conc: 93.95 ng/ml

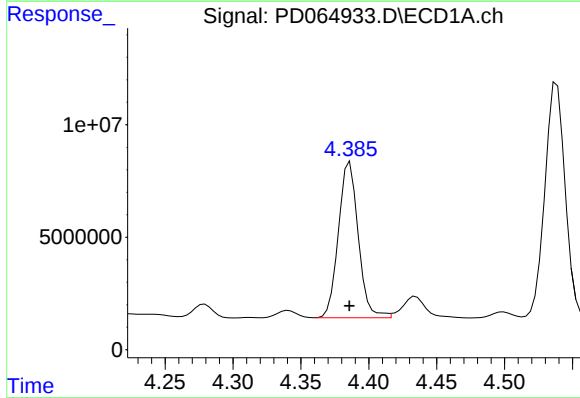


#23 Chlordane-1

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 70430540
Conc: 969.47 ng/ml

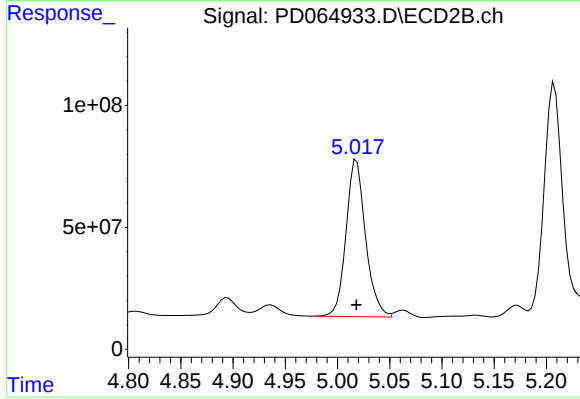


#23 Chlordane-1

R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 836171061
Conc: 932.69 ng/ml

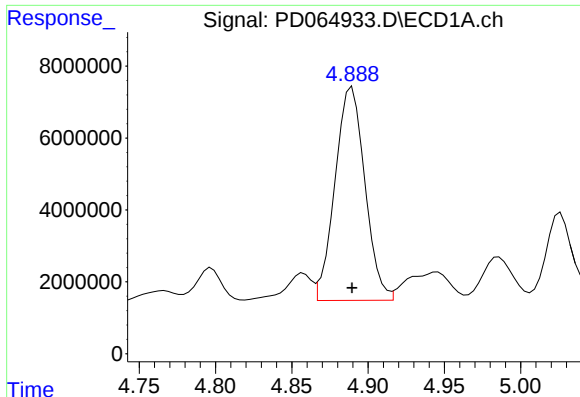


#24 Chlordane-2

R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 80951065
Conc: 931.41 ng/ml

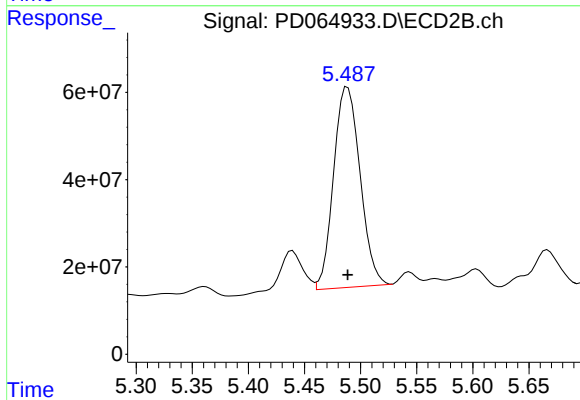


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 755107198
Conc: 908.75 ng/ml

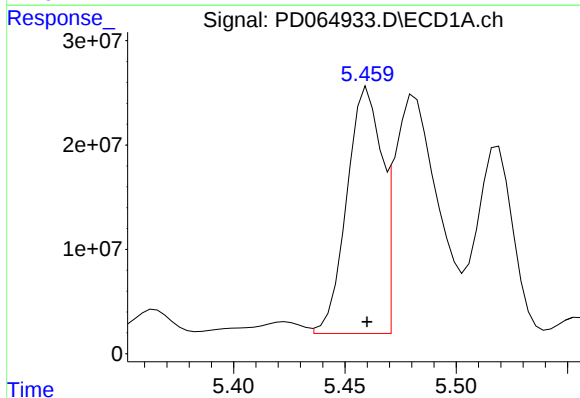


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 255532076
Conc: 989.25 ng/ml

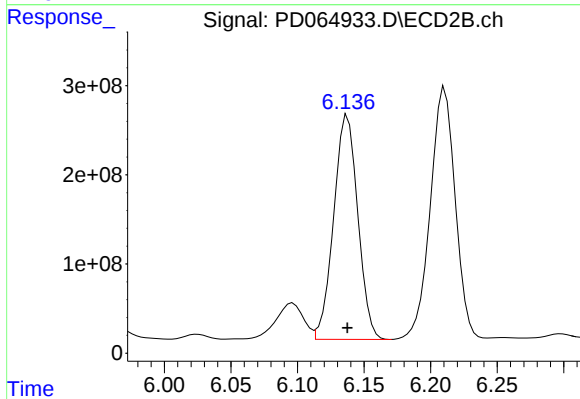


#25 Chlordane-3

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 3182752810
Conc: 949.00 ng/ml

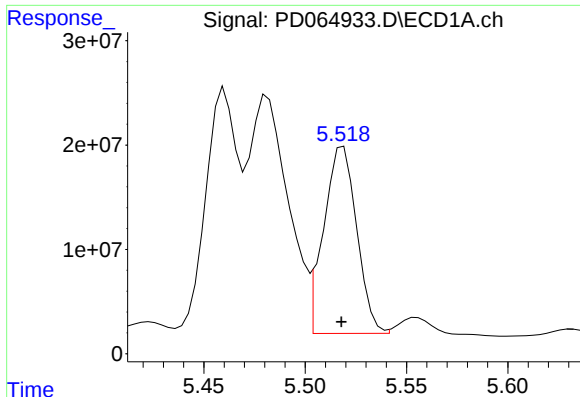


#26 Chlordane-4

R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 203686983
Conc: 979.06 ng/ml

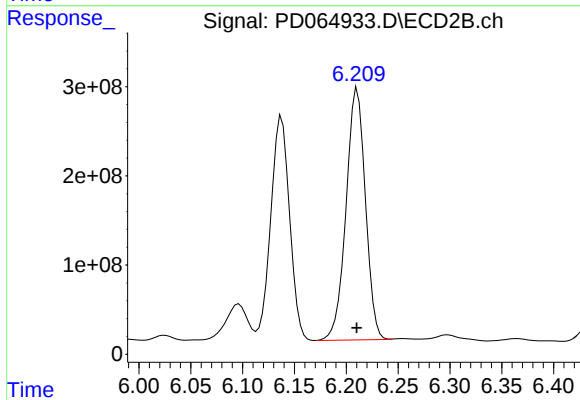


#26 Chlordane-4

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 3668157788
Conc: 943.25 ng/ml

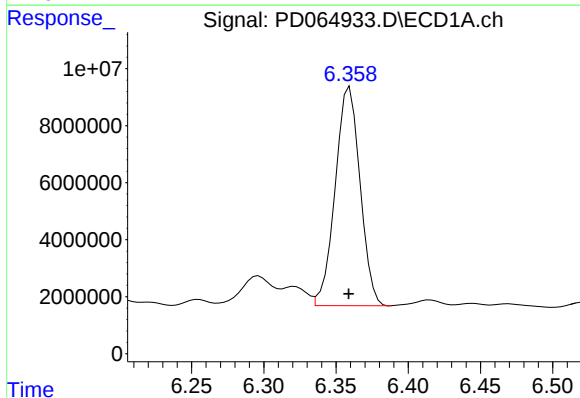


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 91712521
Conc: 976.62 ng/ml

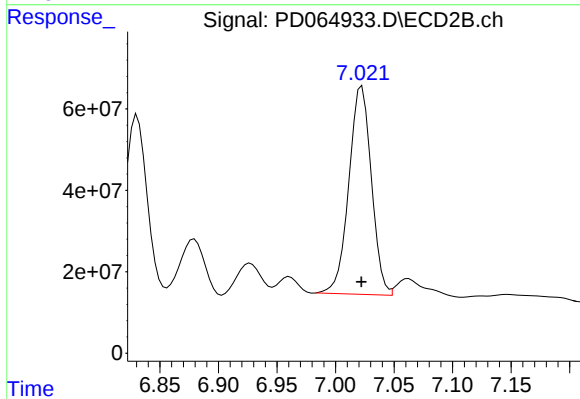


#27 Chlordane-5

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 686022014
Conc: 939.52 ng/ml

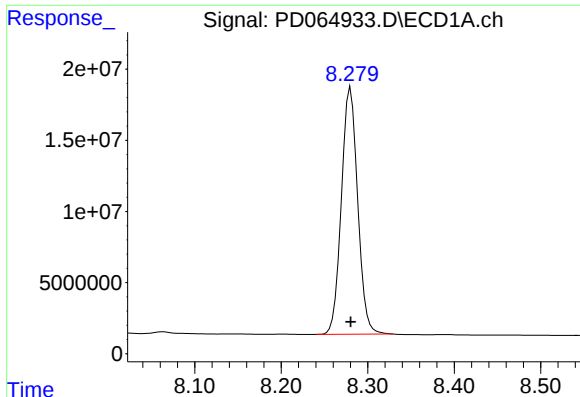

#28 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 225659170
Conc: 94.76 ng/ml

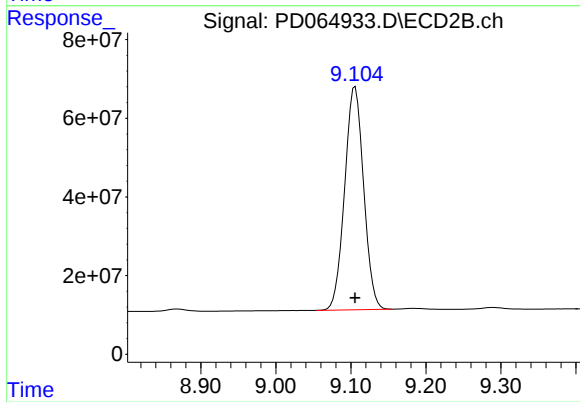

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 997294963
Conc: 91.95 ng/ml