

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 06:13
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD081421

Manual Integrations
 APPROVED

mohammad
 8/20/2021 5:41:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:32:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 05:39:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.509	4.020	99788092	1057.3E6	51.003	50.917
7) SA Decachlor...	8.281	9.106	124.8E6	583.2E6	50.389	50.050
Target Compounds						
2) Toxaphene-1	5.777	6.419	9164961	63601236	499.274	512.237
3) Toxaphene-2	6.262	6.611	10159795	104.4E6	513.018	509.758
4) Toxaphene-3	6.557	7.119	17988528	95310835	503.865m	502.101
5) Toxaphene-4	6.983	7.281	18207368	174.4E6	531.452	506.636
6) Toxaphene-5	7.118	7.700	27199928	126.0E6	509.973	506.505

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 06:13
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:32:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 05:39:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

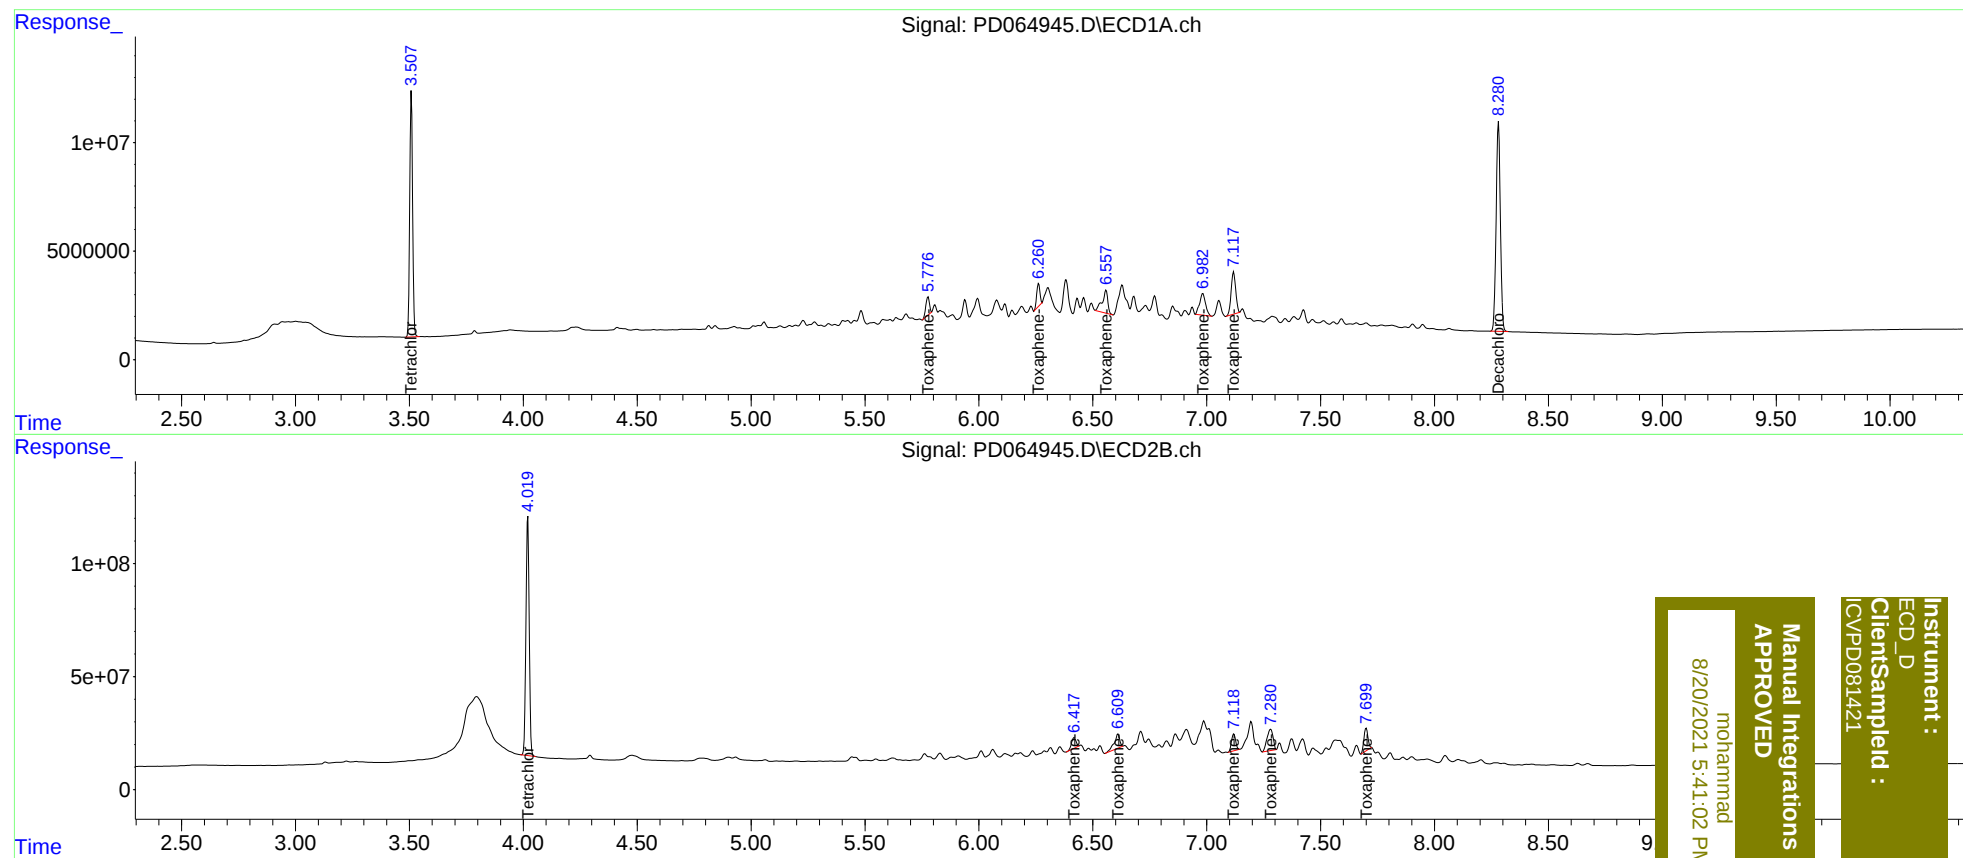

Manual Integrations
APPROVED

mohammad
8/20/2021 5:41:02 PM

Instrument :
ECD_D
ClientSampled :
ICV/PD081421