

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 09:55
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:37:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 05:39:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.509	4.020	97153117	1027.5E6	49.656	49.483
7) SA Decachlor...	8.281	9.104	105.7E6	579.7E6	42.688	49.753
Target Compounds						
2) Toxaphene-1	5.778	6.417	8249607	63114445	449.409	508.316
3) Toxaphene-2	6.263	6.610	9384926	103.5E6	473.891	505.395
4) Toxaphene-3	6.559	7.119	16427715	94966187	460.147	500.285
5) Toxaphene-4	6.983	7.281	16051946	174.0E6	468.538	505.536
6) Toxaphene-5	7.118	7.700	23611691	126.4E6	442.697	508.005

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 09:55
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:37:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 05:39:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

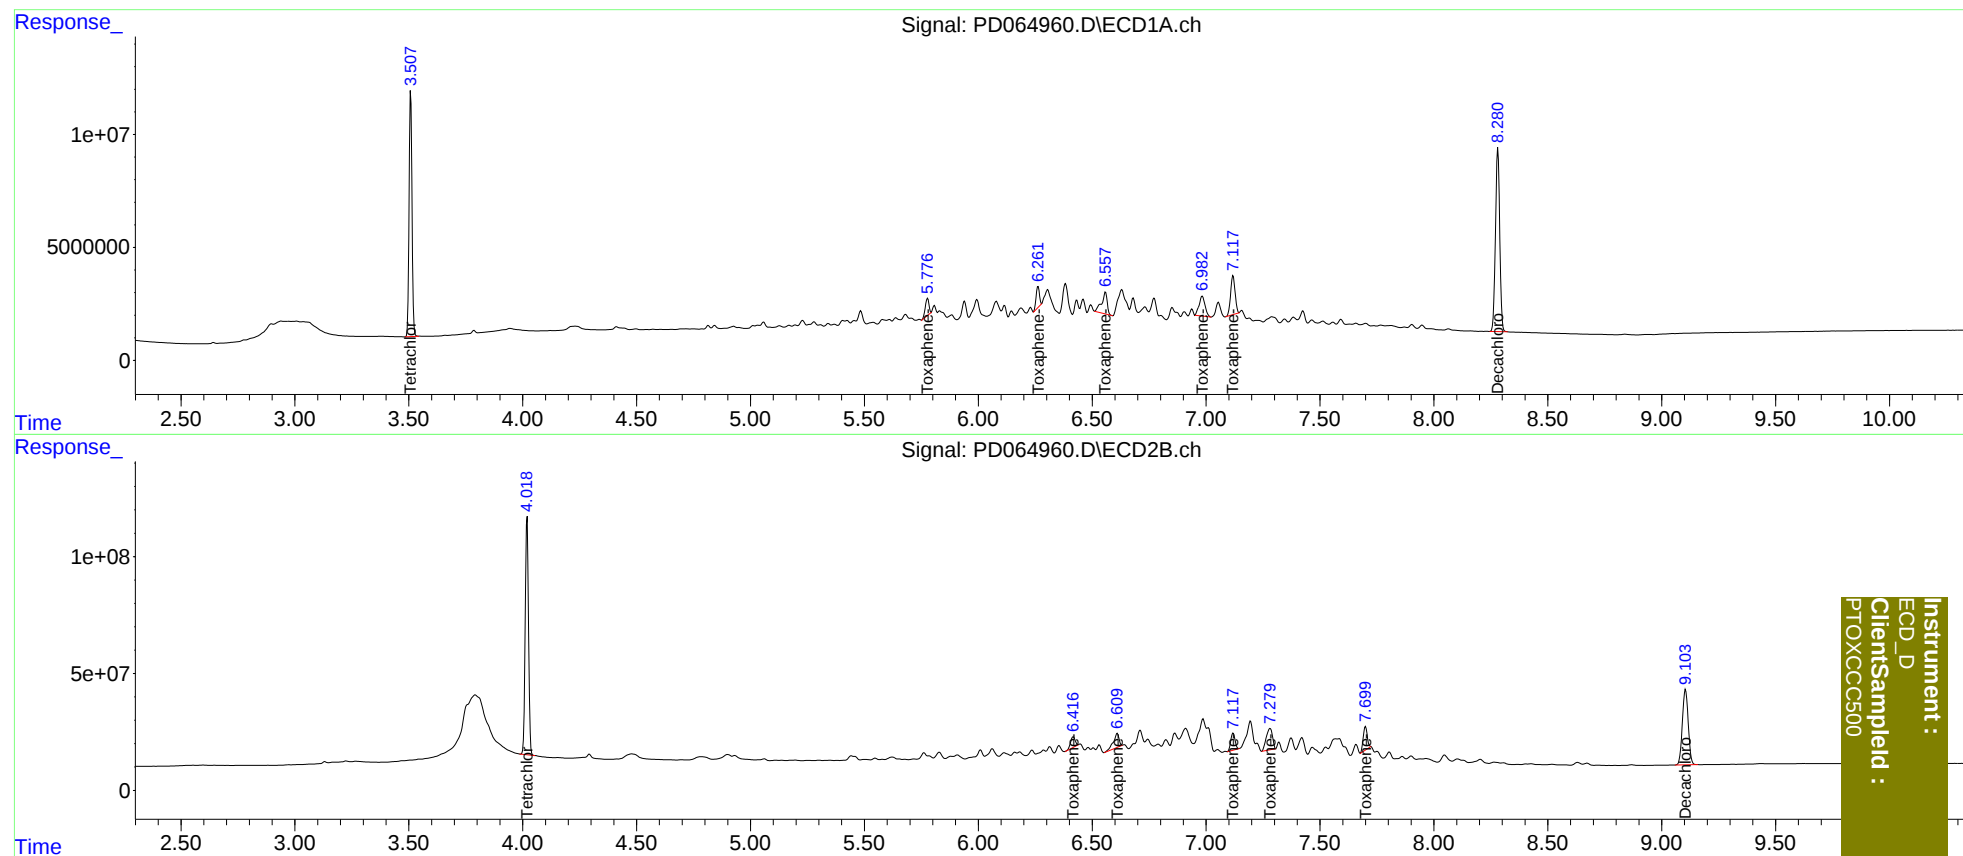

Instrument :
ECD_D
ClientSample :
PTOXCCC500