

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 12:40
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:38:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 05:39:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.509	4.020	95675247	1030.8E6	48.901	49.639
7) SA Decachlor...	8.280	9.105	72568138	587.8E6	29.301	50.448 #
Target Compounds						
2) Toxaphene-1	5.777	6.418	6363198	58633402	346.644	472.226 #
3) Toxaphene-2	6.262	6.610	6830455	102.6E6	344.903	501.110 #
4) Toxaphene-3	6.558	7.118	12186587	92043851	341.351	484.891 #
5) Toxaphene-4	6.983	7.280	12190151	171.9E6	355.817	499.406 #
6) Toxaphene-5	7.118	7.699	17539506	125.9E6	328.849	506.290 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 12:40
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:38:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 05:39:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

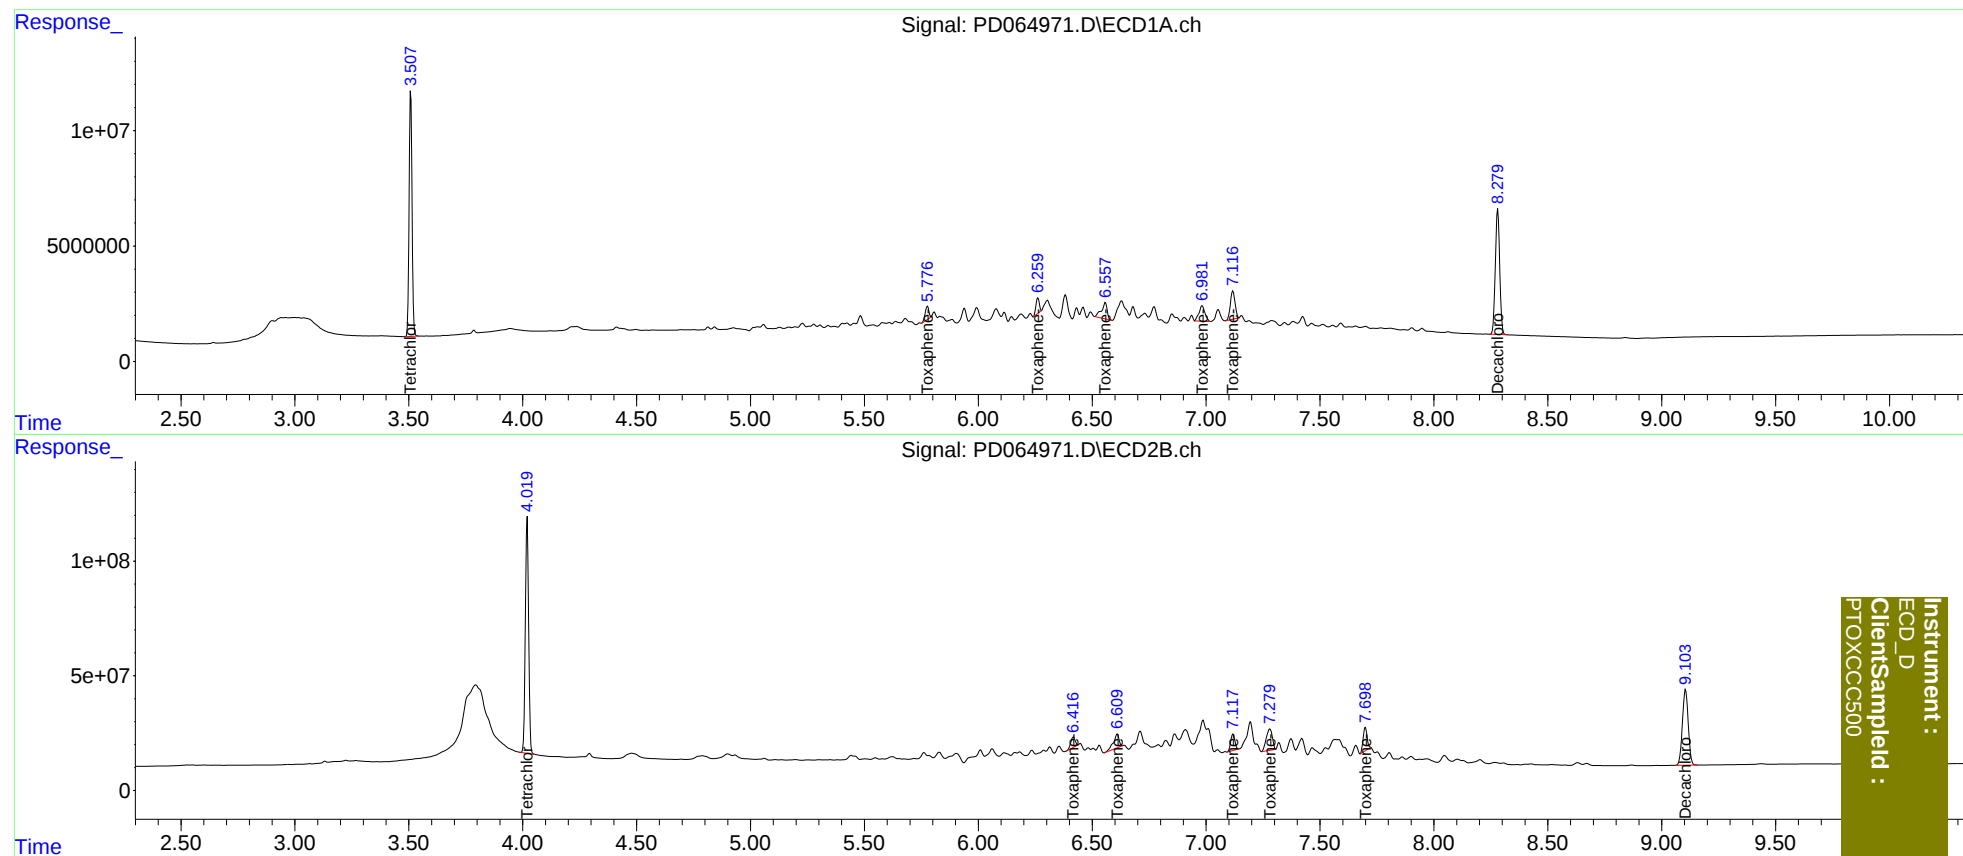

Instrument :
ECD_D
ClientSampled :
PTOXC500