

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 02:04
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:27:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 06:24:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	38988505	412.0E6	19.950	20.290
28)	SA Decachlor...	8.281	9.105	47321956	221.4E6	19.255	19.925
Target Compounds							
9)	A Endosulfan I	5.573	6.261	24954894	247.8E6	9.848	10.501
10)	B gamma-Chl...	5.459	6.137	26761836	271.8E6	9.684	10.405
12)	B 4,4'-DDE	5.682	6.368	52007401	497.7E6	19.782	20.481
13)	MA Dieldrin	5.818	6.521	54452305	511.7E6	19.874	20.746
19)	B Endosulfa...	6.733	7.301	46838388	378.6E6	20.275	19.628
20)	A Methoxychlor	6.991	7.622	119.8E6	799.1E6	85.459	84.123
21)	B Endrin ke...	7.229	7.776	54636680	376.3E6	18.986	19.723



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 02:04
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:27:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 06:24:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

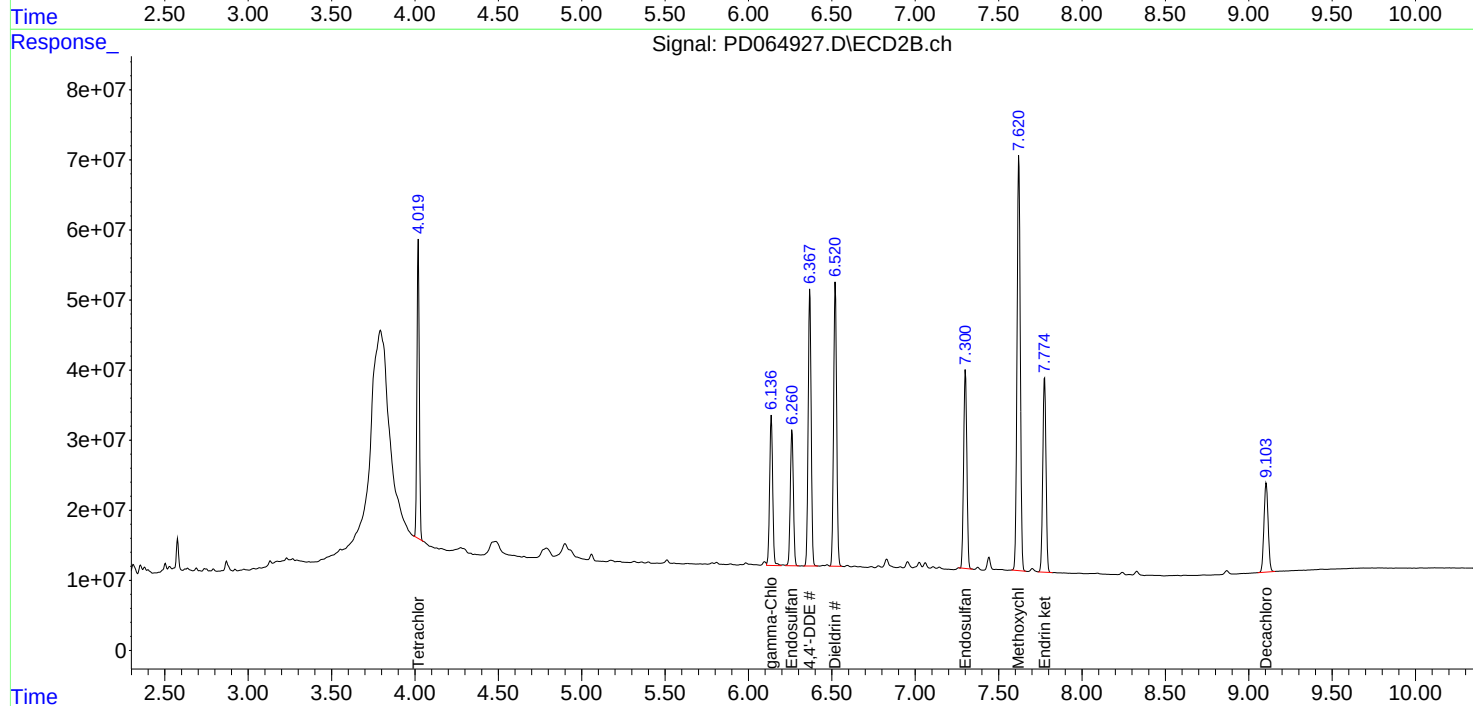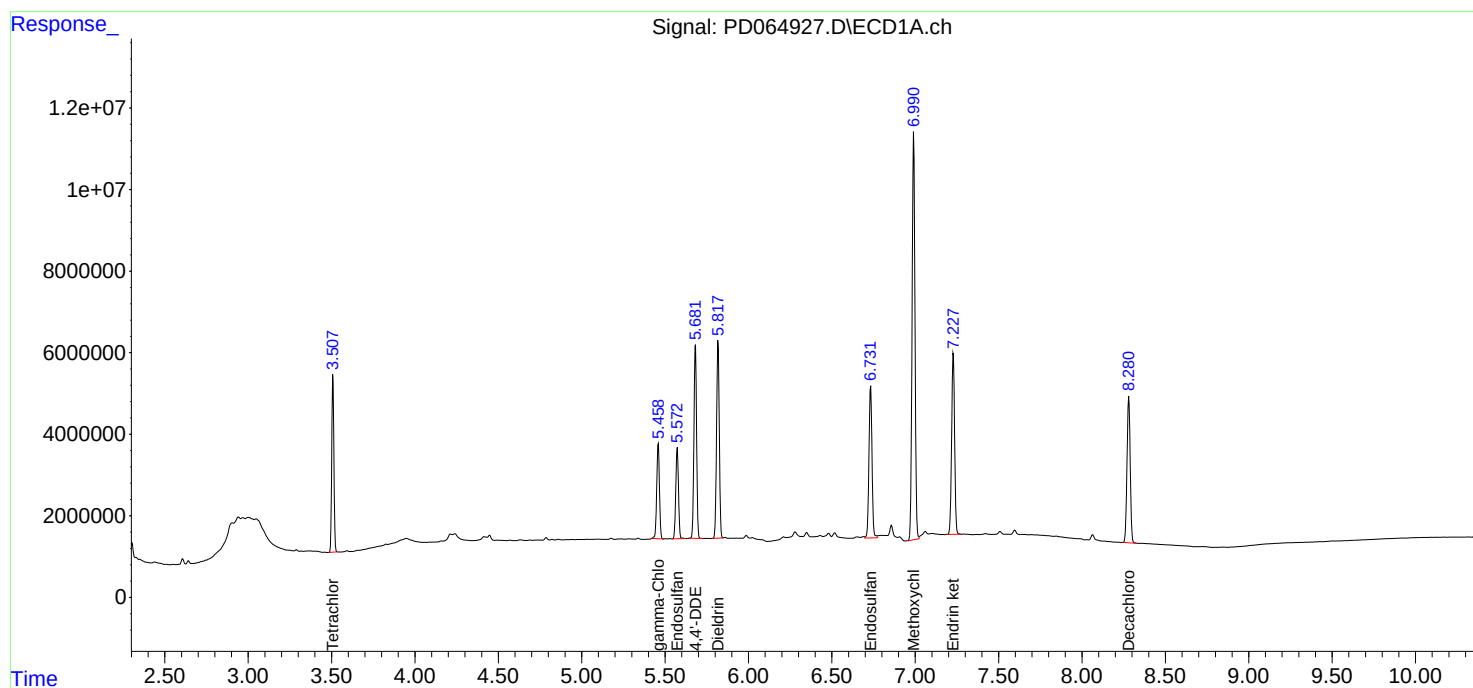


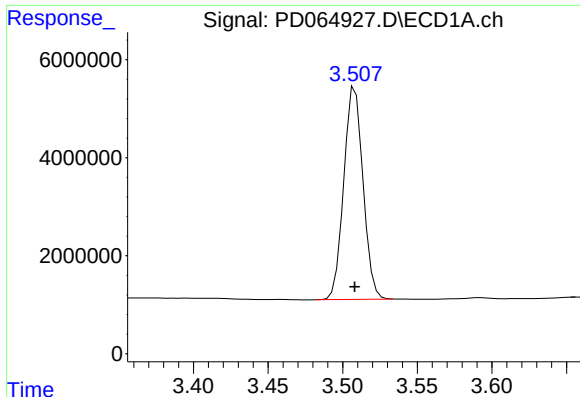

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 38988505
Conc: 19.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

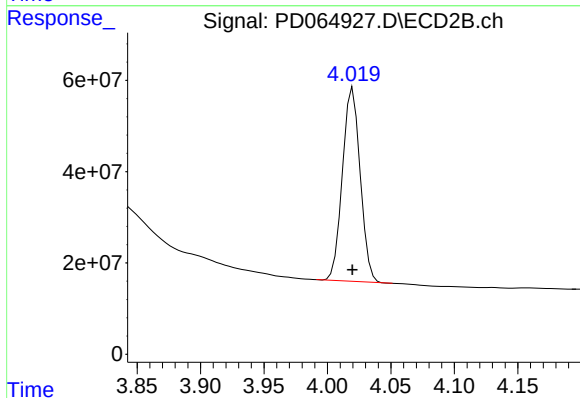


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 412022498
Conc: 20.29 ng/ml

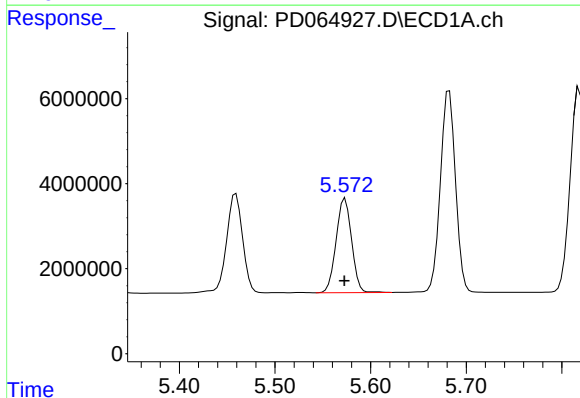


#9 Endosulfan I

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 24954894
Conc: 9.85 ng/ml

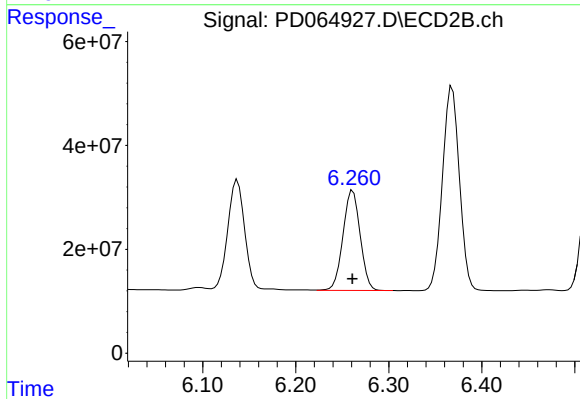

#9 Endosulfan I


R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 247759700
Conc: 10.50 ng/ml

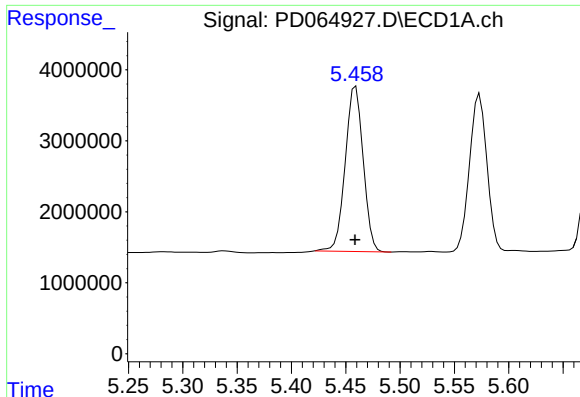

#10 gamma-Chlordane


R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 26761836
Conc: 9.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

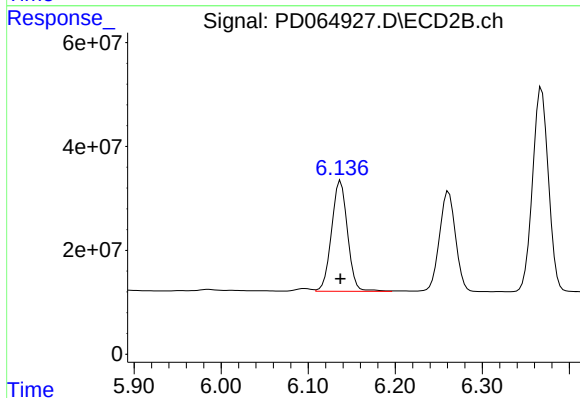


#10 gamma-Chlordane

R.T.: 6.137 min
Delta R.T.: 0.000 min
Response: 271782456
Conc: 10.41 ng/ml

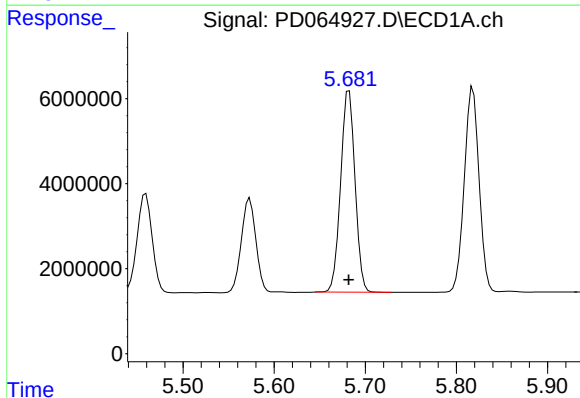


#12 4,4'-DDE

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 52007401
Conc: 19.78 ng/ml

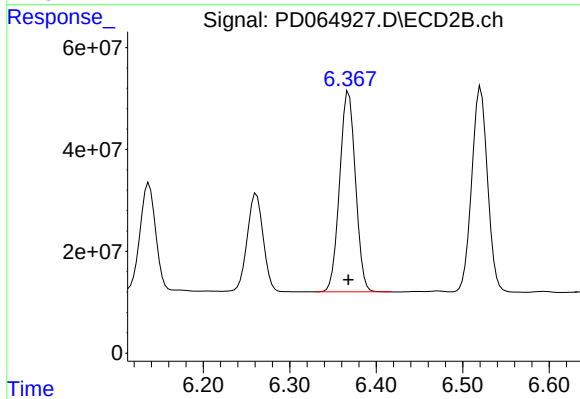

#12 4,4'-DDE


R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 497741491
Conc: 20.48 ng/ml

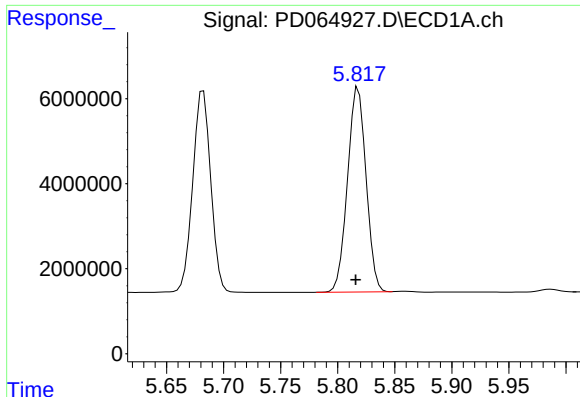

#13 Dieldrin


R.T.: 5.818 min
Delta R.T.: 0.002 min
Response: 54452305
Conc: 19.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

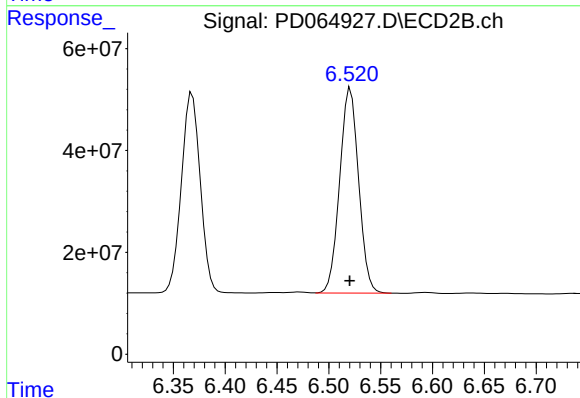


#13 Dieldrin

R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 511659347
Conc: 20.75 ng/ml

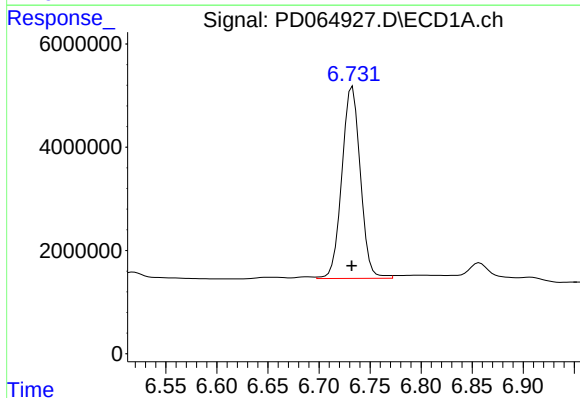


#19 Endosulfan Sulfate

R.T.: 6.733 min
Delta R.T.: 0.000 min
Response: 46838388
Conc: 20.28 ng/ml

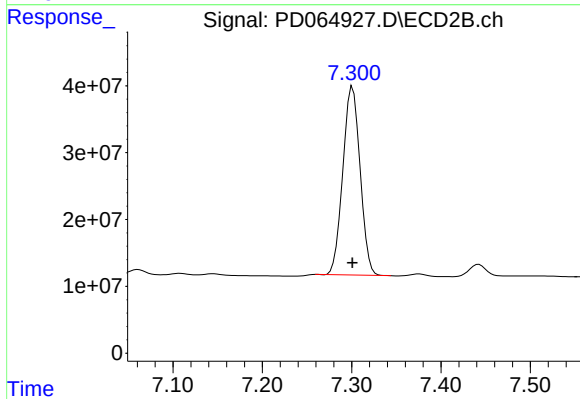

#19 Endosulfan Sulfate


R.T.: 7.301 min
Delta R.T.: 0.000 min
Response: 378633045
Conc: 19.63 ng/ml

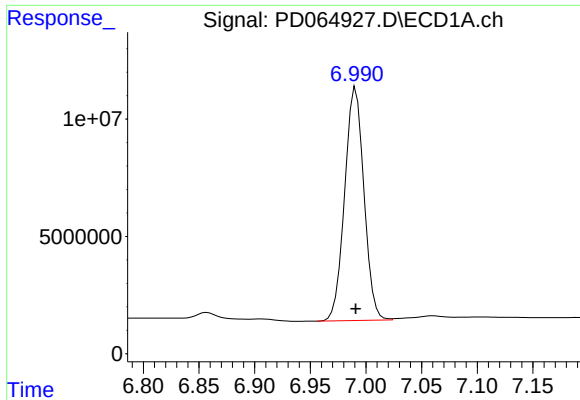

#20 Methoxychlor


R.T.: 6.991 min
Delta R.T.: 0.000 min
Response: 119834777
Conc: 85.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

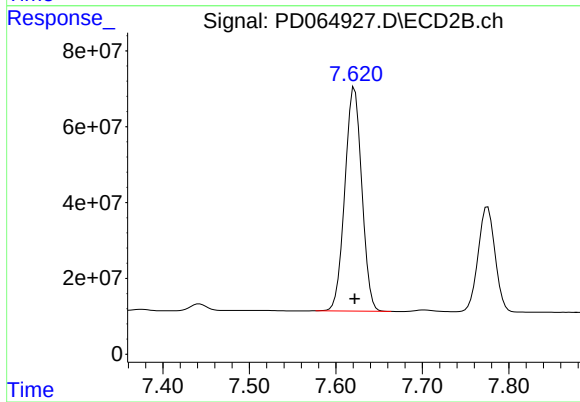


#20 Methoxychlor

R.T.: 7.622 min
Delta R.T.: 0.000 min
Response: 799140320
Conc: 84.12 ng/ml

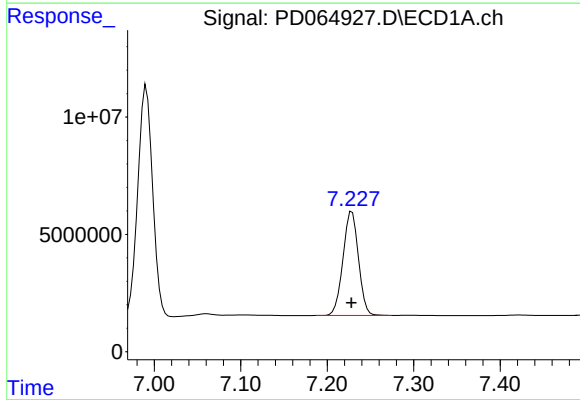


#21 Endrin ketone

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 54636680
Conc: 18.99 ng/ml

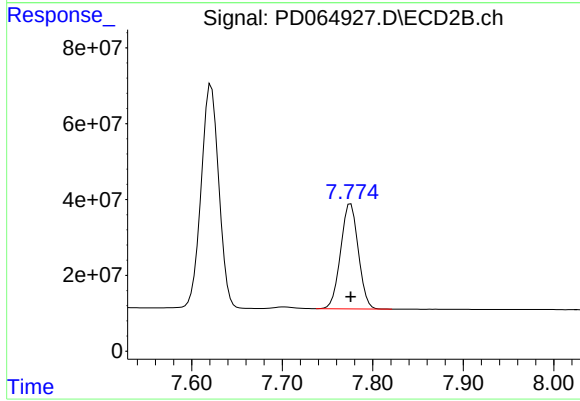

#21 Endrin ketone

R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 376252467
Conc: 19.72 ng/ml

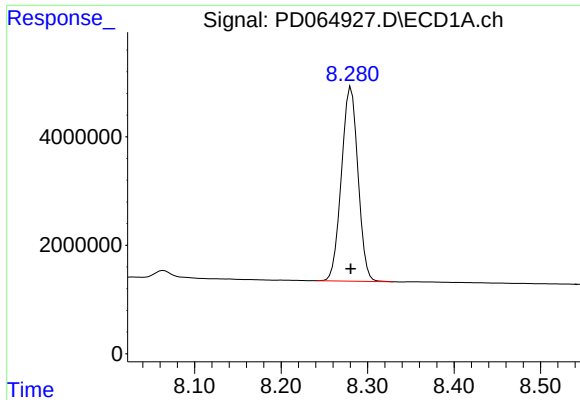

#28 Decachlorobiphenyl


R.T.: 8.281 min

Delta R.T.: 0.000 min

Response: 47321956

Conc: 19.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

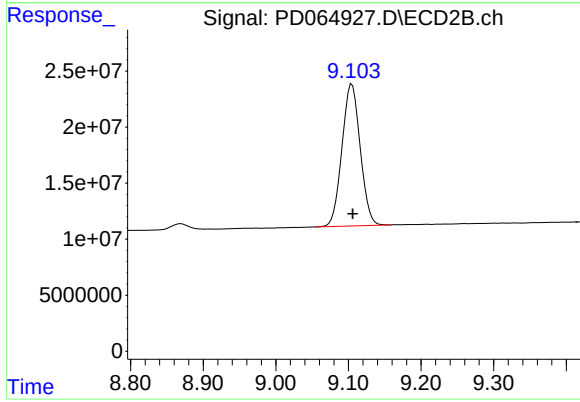

#28 Decachlorobiphenyl

R.T.: 9.105 min

Delta R.T.: 0.000 min

Response: 221449698

Conc: 19.93 ng/ml