

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 03:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:56:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 04:55:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	174.0E6	1488.8E6	75.848	73.854
28)	SA Decachlor...	8.281	9.106	176.5E6	787.1E6	74.108	72.567
Target Compounds							
23)	Chlordane-1	4.386	5.018	54332561	659.1E6	747.881	735.198
24)	Chlordane-2	4.890	5.488	63614587	602.1E6	731.941	724.572
25)	Chlordane-3	5.460	6.138	193.5E6	2495.1E6	749.183	743.962
26)	Chlordane-4	5.518	6.210	157.3E6	2880.9E6	756.170	740.814
27)	Chlordane-5	6.359	7.022	70590654	538.4E6	751.698	737.408



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 03:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:56:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 04:55:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

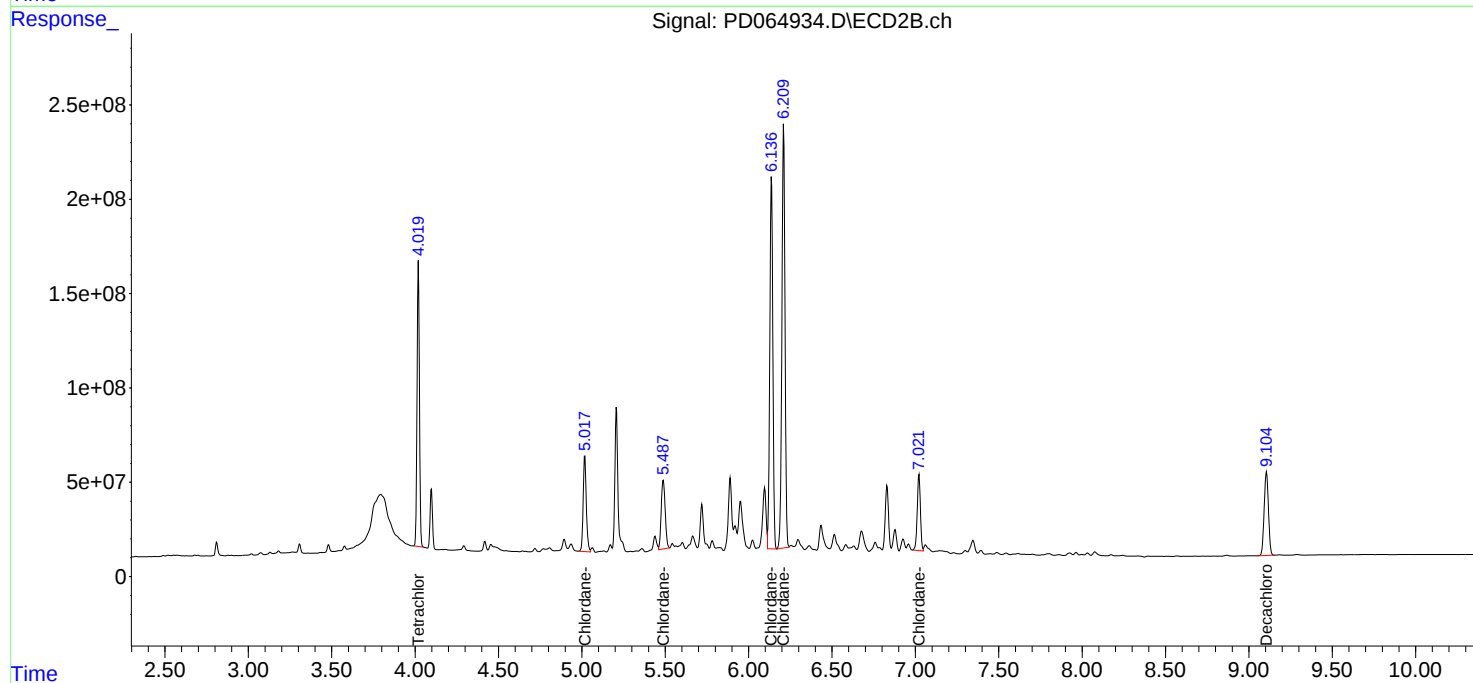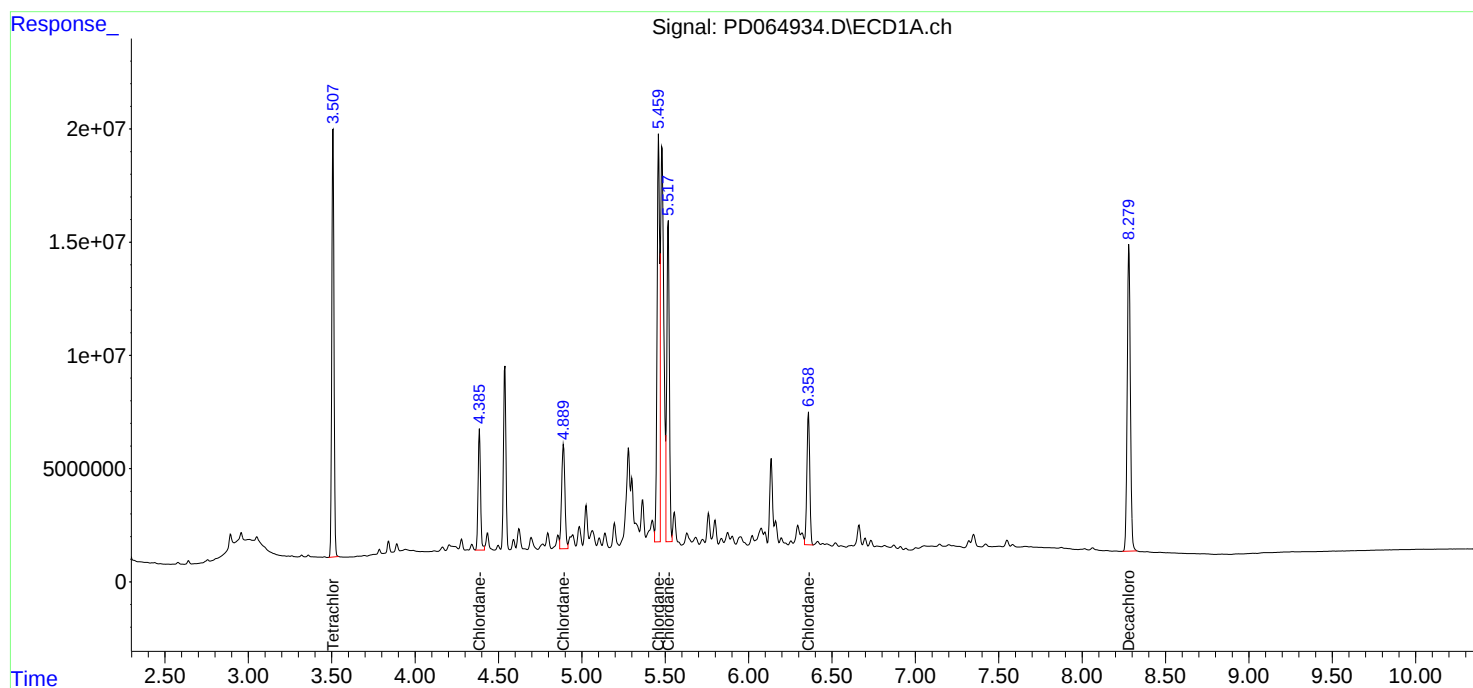


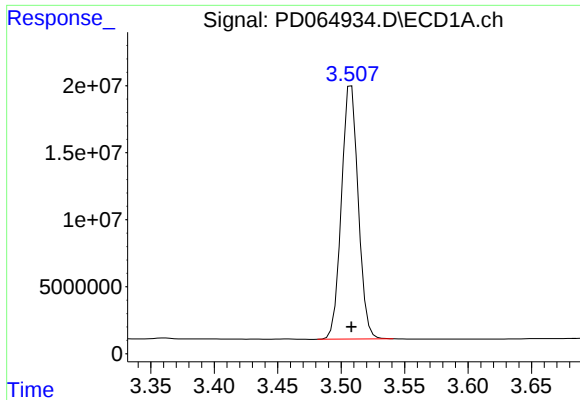

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 174002259
Conc: 75.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

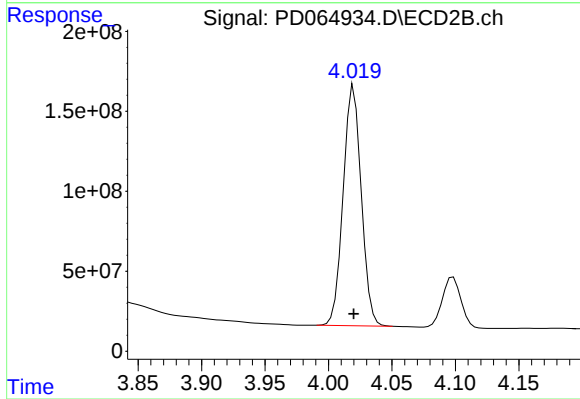


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 1488847366
Conc: 73.85 ng/ml

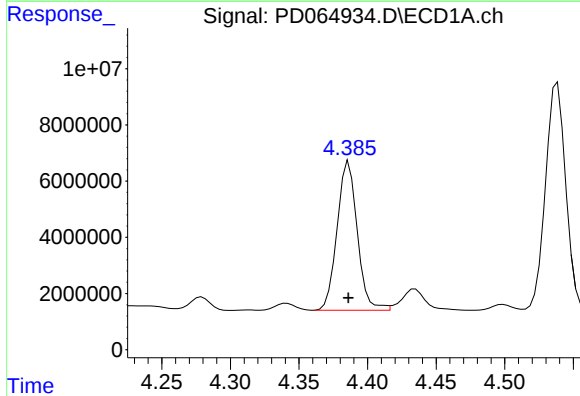


#23 Chlordane-1

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 54332561
Conc: 747.88 ng/ml

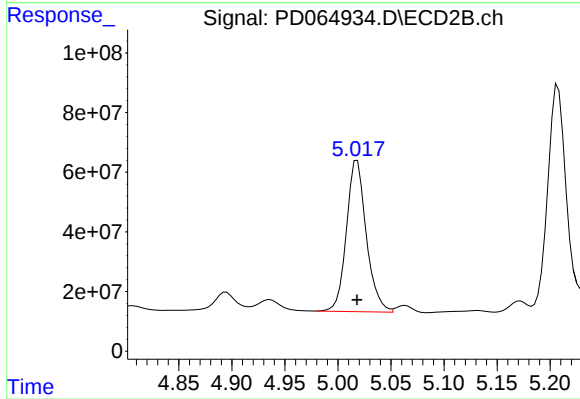

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 659114012
Conc: 735.20 ng/ml

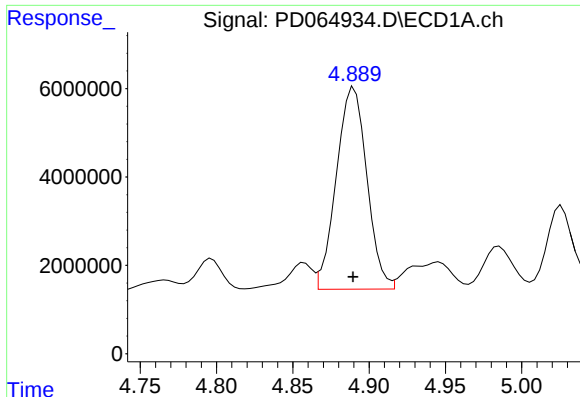

#24 Chlordane-2


R.T.: 4.890 min
Delta R.T.: 0.000 min
Response: 63614587
Conc: 731.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

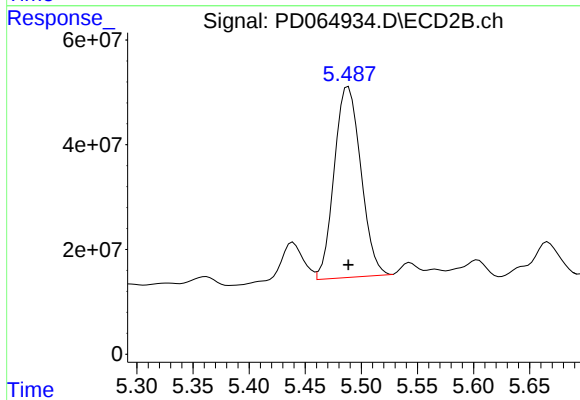


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 602071117
Conc: 724.57 ng/ml

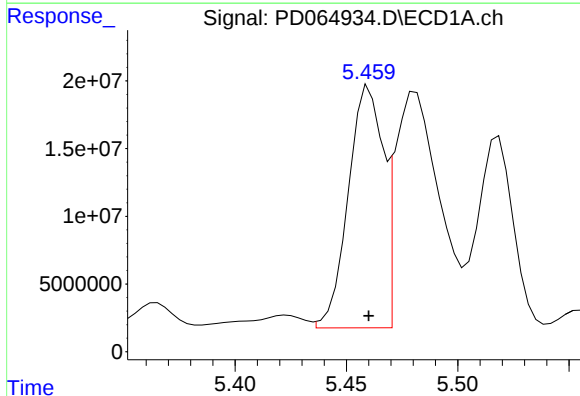


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 193519743
Conc: 749.18 ng/ml

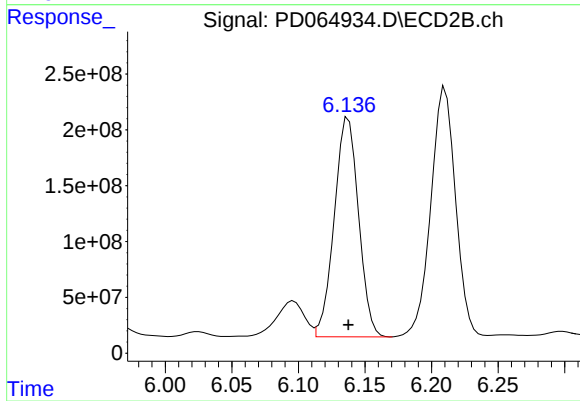

#25 Chlordane-3


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 2495085853
Conc: 743.96 ng/ml

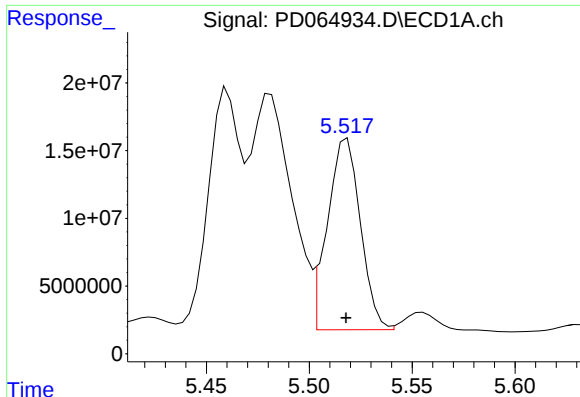

#26 Chlordane-4


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 157316467
Conc: 756.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

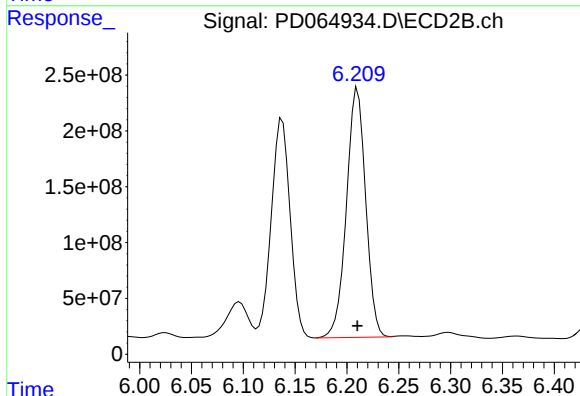


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 2880902056
Conc: 740.81 ng/ml

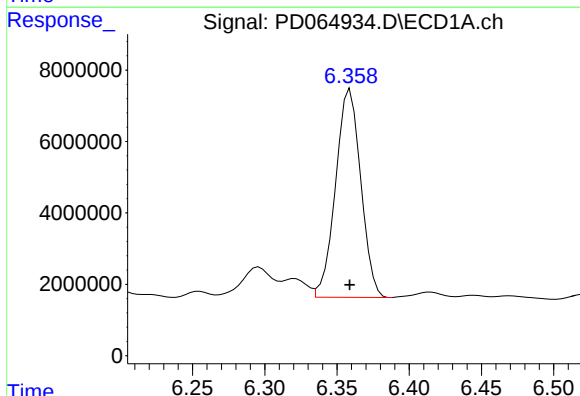


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 70590654
Conc: 751.70 ng/ml

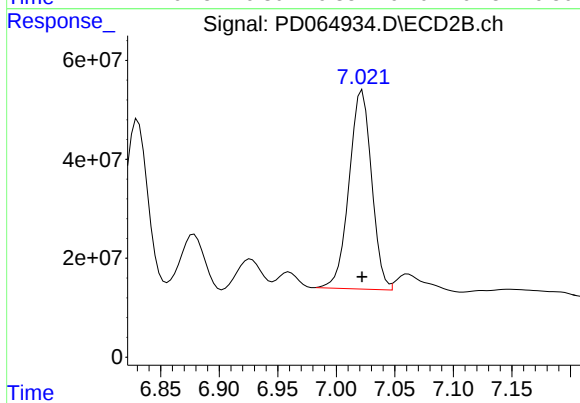

#27 Chlordane-5


R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 538440010
Conc: 737.41 ng/ml

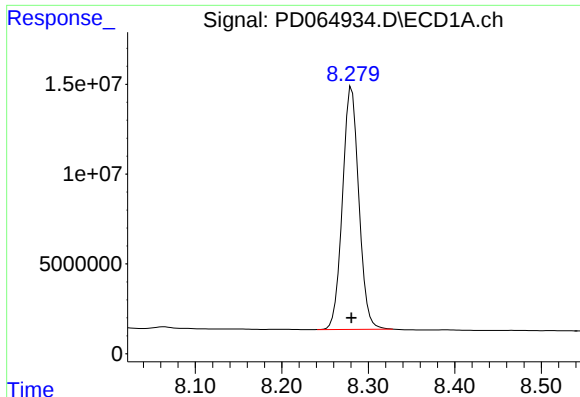

#28 Decachlorobiphenyl

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 176483395
Conc: 74.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

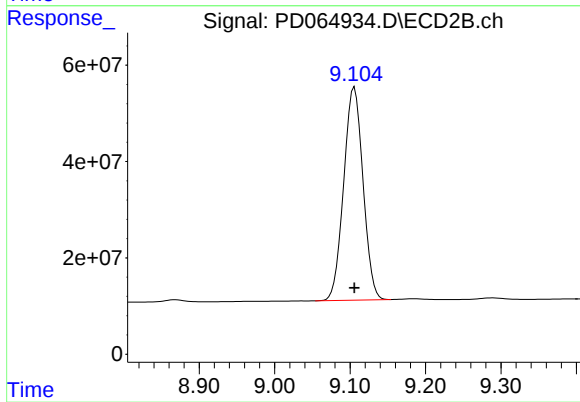

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 787087344
Conc: 72.57 ng/ml