

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 03:55
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:56:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 04:55:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	114.7E6	1008.0E6	50.000	50.000
28)	SA Decachlor...	8.281	9.106	119.1E6	542.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.386	5.018	36324352	448.3E6	500.000	500.000
24)	Chlordane-2	4.890	5.489	43456069	415.5E6	500.000	500.000
25)	Chlordane-3	5.460	6.138	129.2E6	1676.9E6	500.000	500.000
26)	Chlordane-4	5.518	6.210	104.0E6	1944.4E6	500.000	500.000
27)	Chlordane-5	6.359	7.022	46954162	365.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 03:55
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:56:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 04:55:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

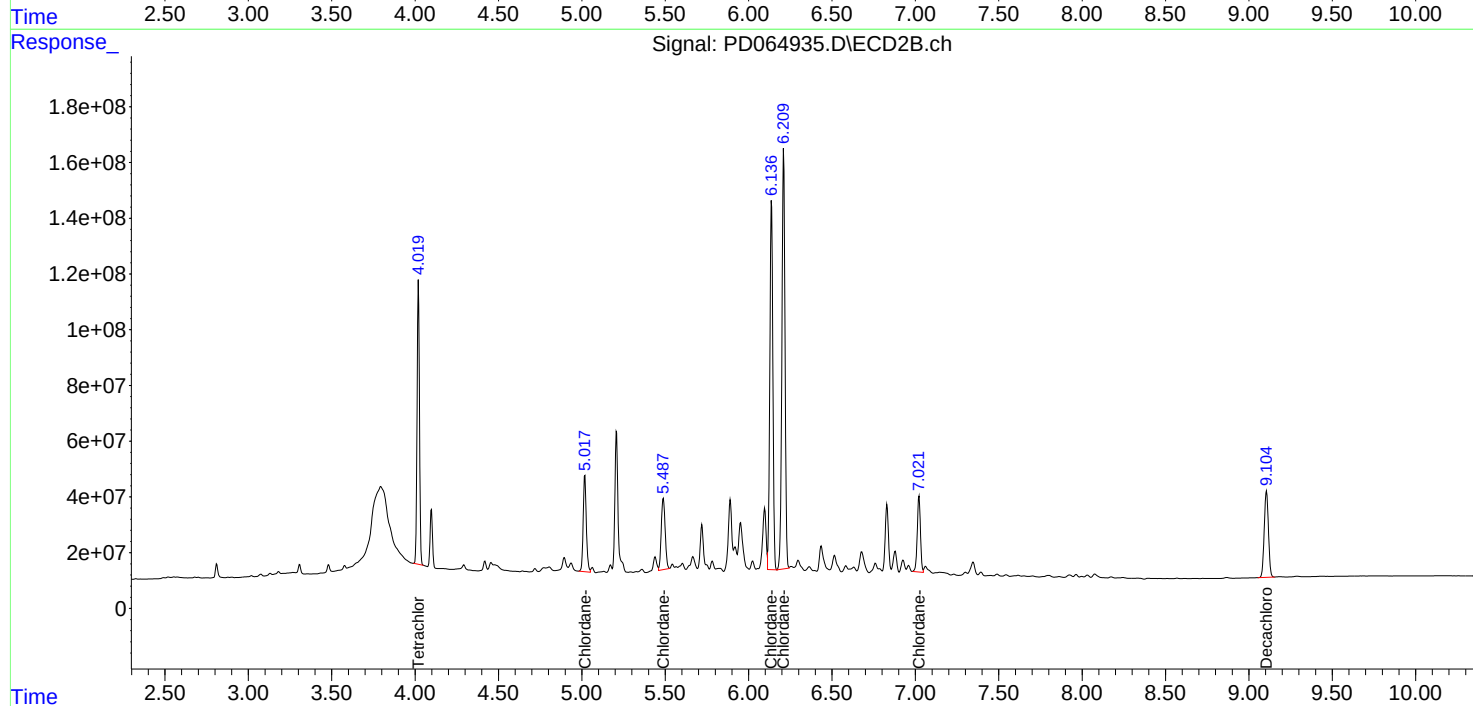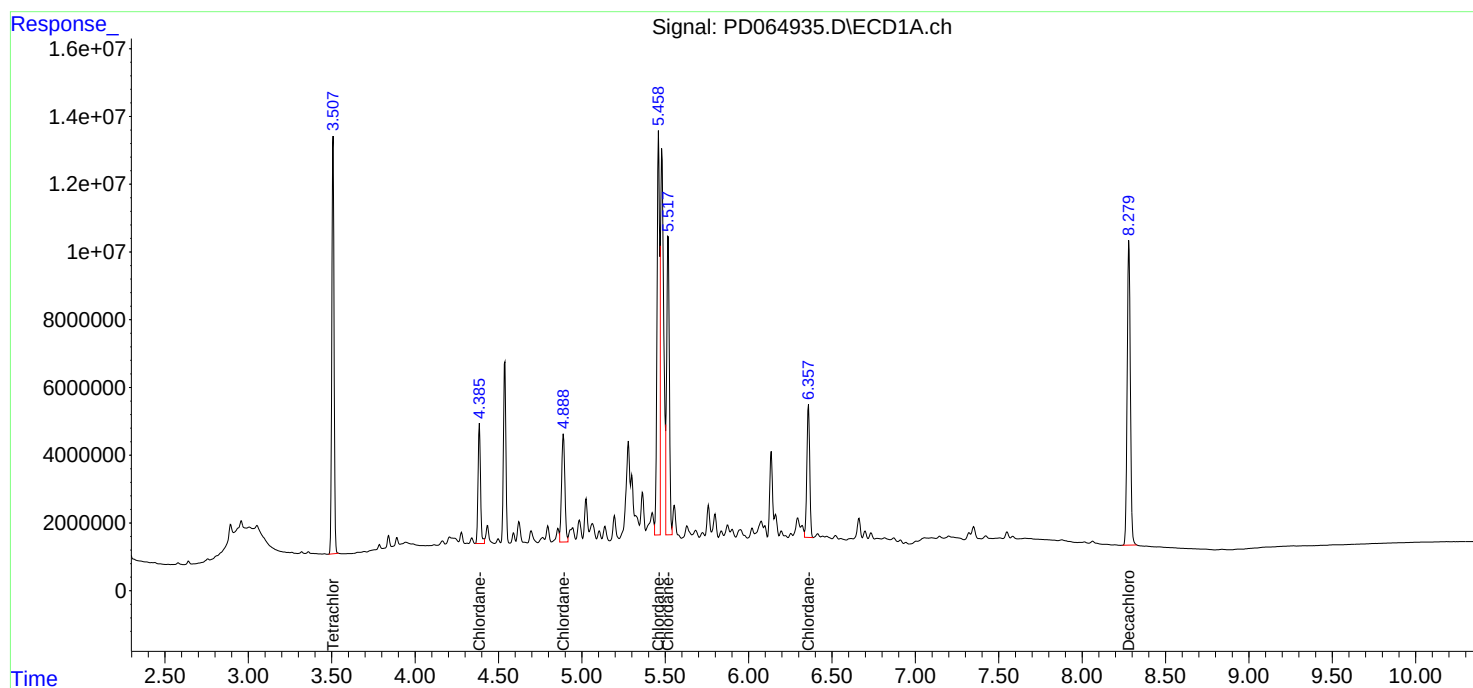


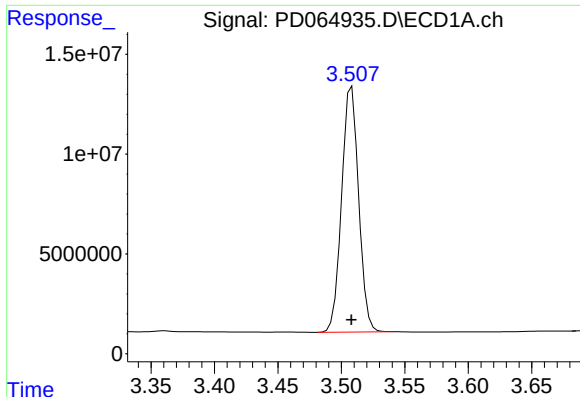

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 114703841
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

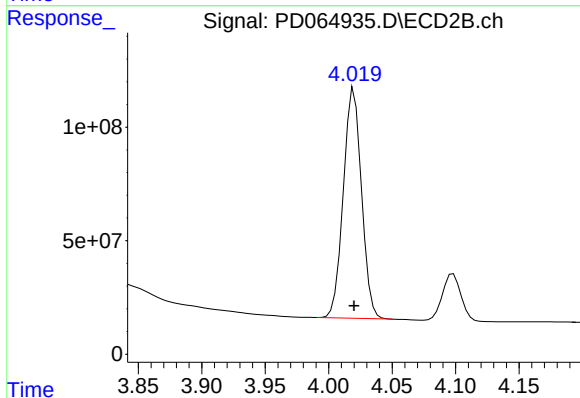


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 1007963105
Conc: 50.00 ng/ml

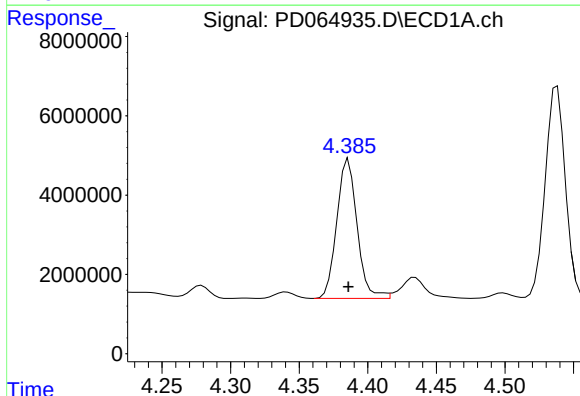


#23 Chlordane-1

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 36324352
Conc: 500.00 ng/ml

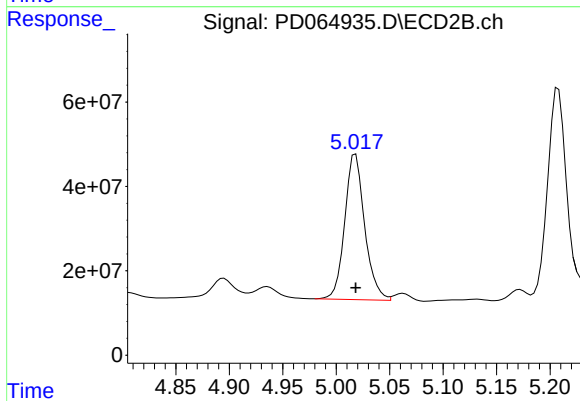

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 448256008
Conc: 500.00 ng/ml

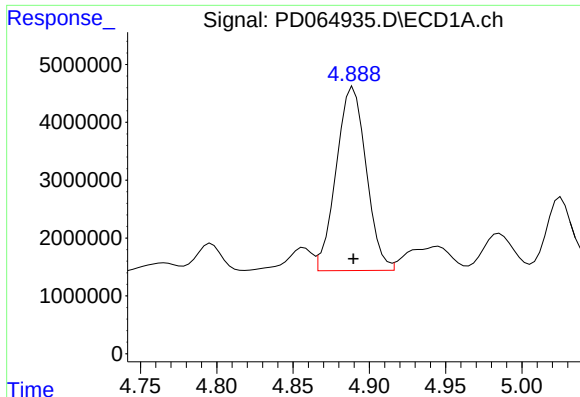

#24 Chlordane-2


R.T.: 4.890 min
Delta R.T.: 0.000 min
Response: 43456069
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

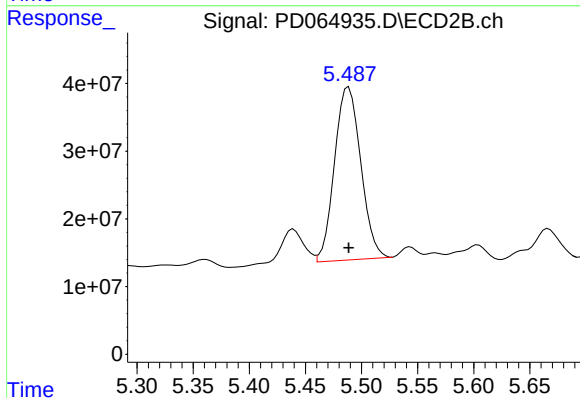


#24 Chlordane-2

R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 415466555
Conc: 500.00 ng/ml

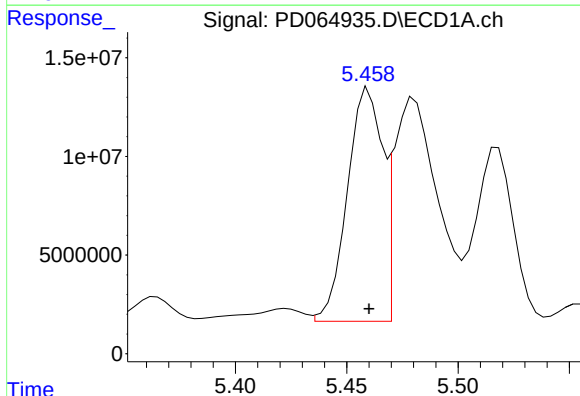


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 129153798
Conc: 500.00 ng/ml

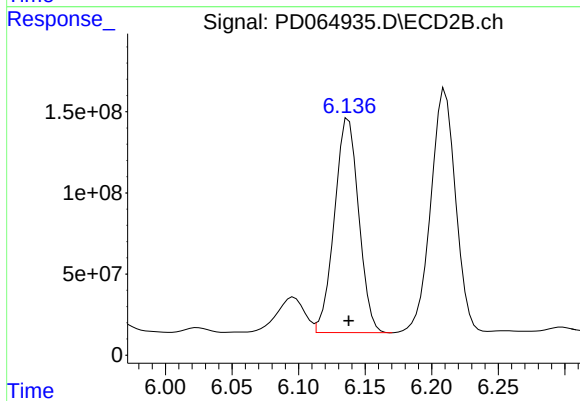

#25 Chlordane-3


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 1676889580
Conc: 500.00 ng/ml

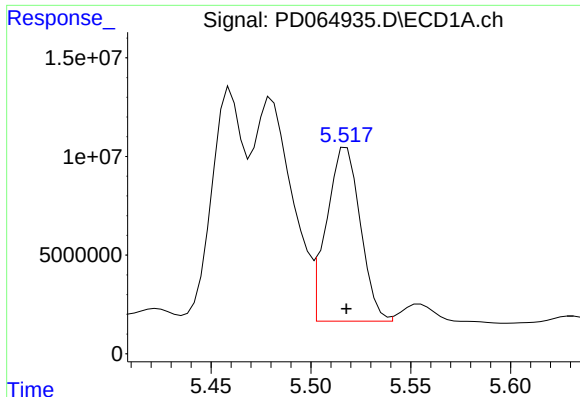

#26 Chlordane-4


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 104021940
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

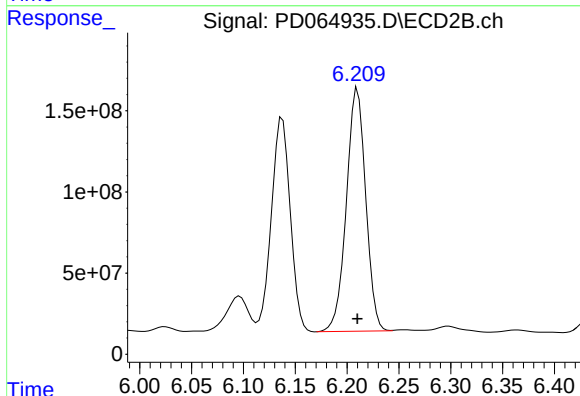


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 1944417181
Conc: 500.00 ng/ml

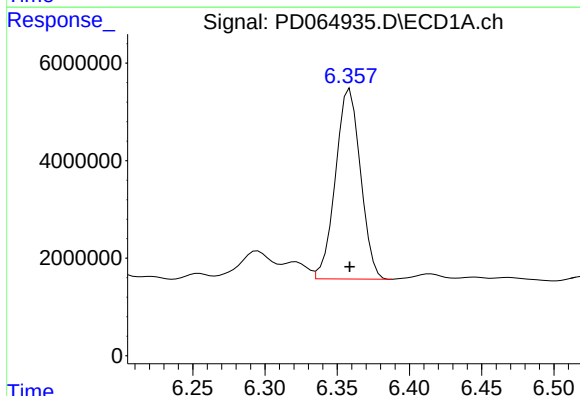


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 46954162
Conc: 500.00 ng/ml

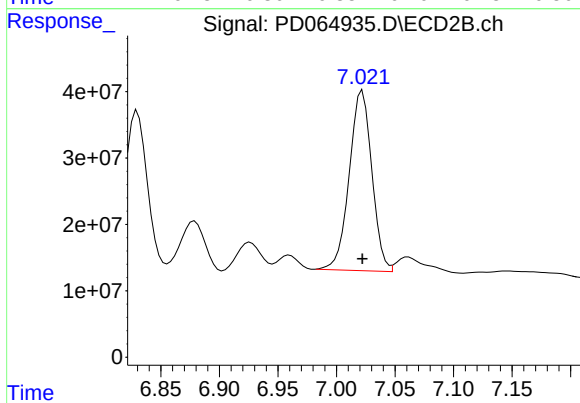

#27 Chlordane-5


R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 365089826
Conc: 500.00 ng/ml

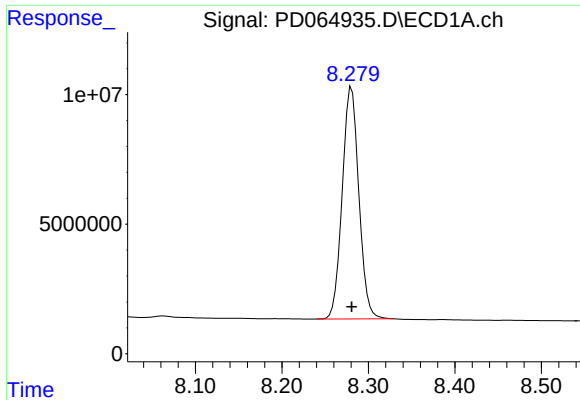

#28 Decachlorobiphenyl

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 119071942
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

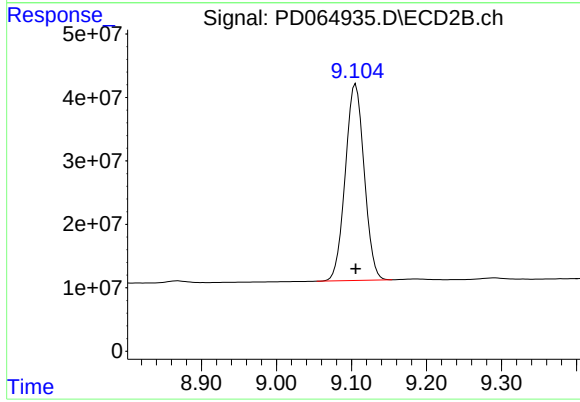

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 542314813
Conc: 50.00 ng/ml