

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 04:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:56:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 14 04:55:08 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	57423186	530.4E6	25.031	26.308
28)	SA Decachlor...	8.280	9.106	63528519	294.2E6	26.677	27.125
Target Compounds							
23)	Chlordane-1	4.386	5.018	18409802	236.6E6	253.409	263.961
24)	Chlordane-2	4.890	5.488	23285942	226.7E6	267.925	272.844
25)	Chlordane-3	5.460	6.137	63768813	876.7E6	246.872	261.410
26)	Chlordane-4	5.518	6.211	52812964	1024.0E6	253.855	263.323
27)	Chlordane-5	6.359	7.022	24253293	192.4E6	258.266	263.496



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 04:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:56:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Sat Aug 14 04:55:08 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

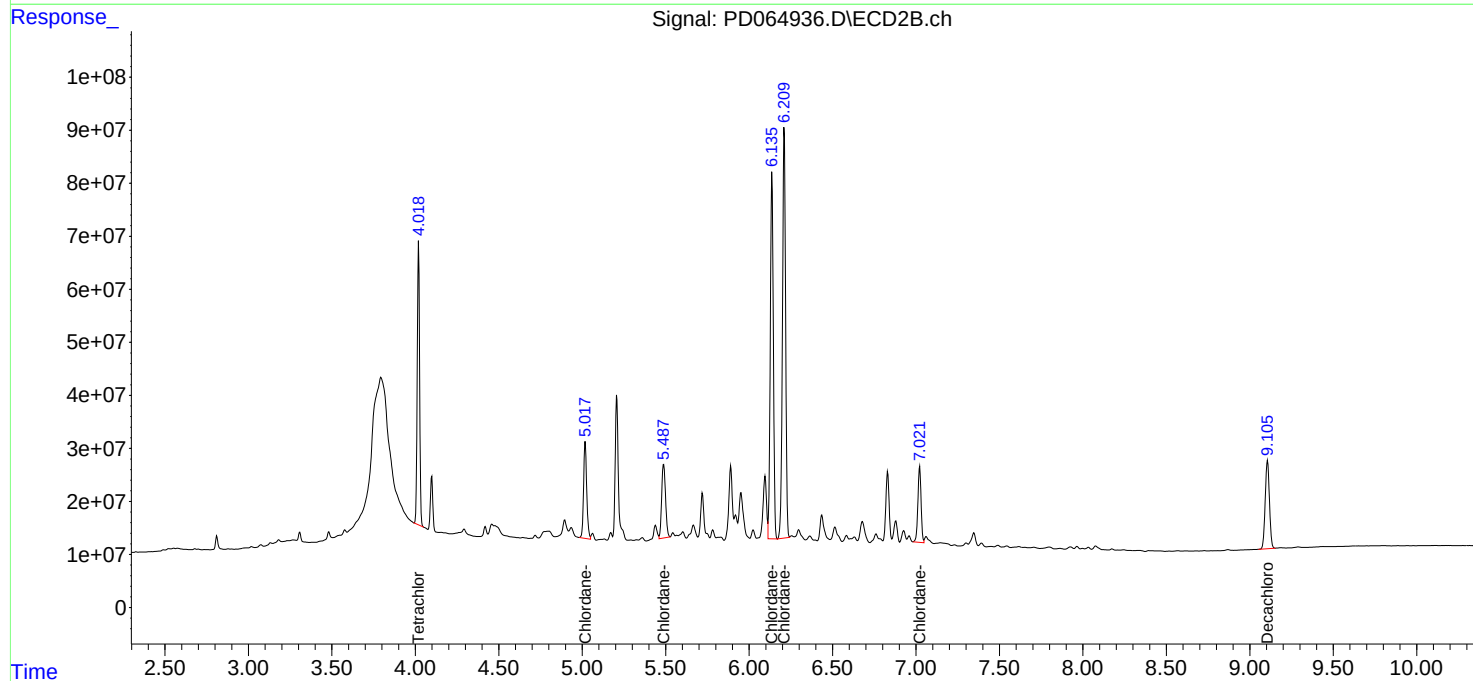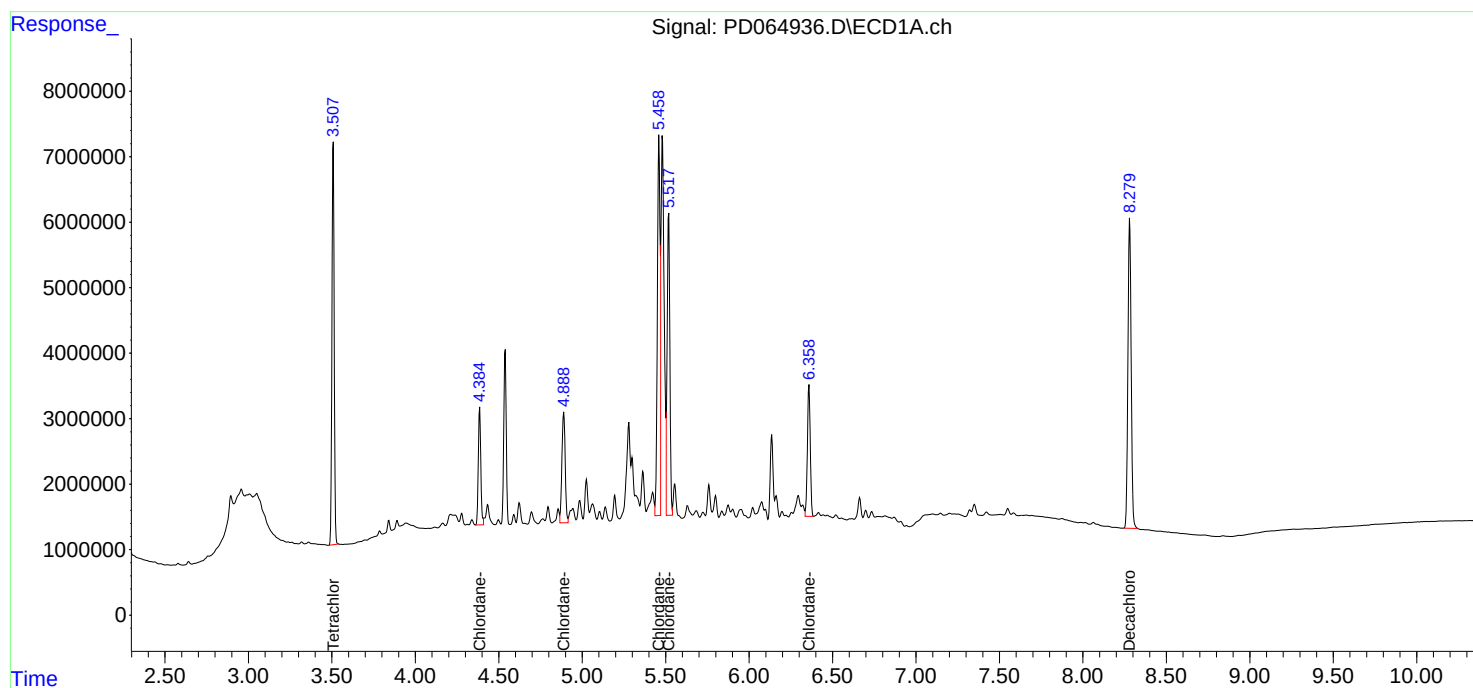


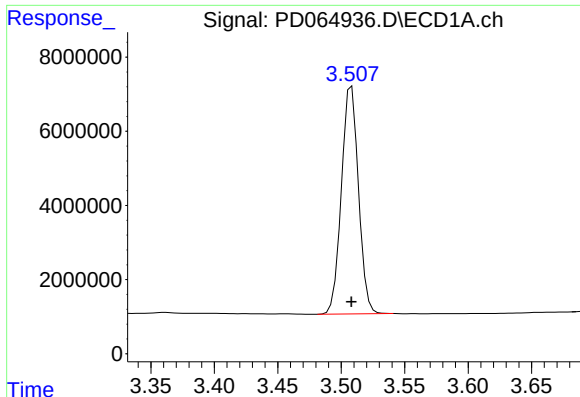

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 57423186
Conc: 25.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

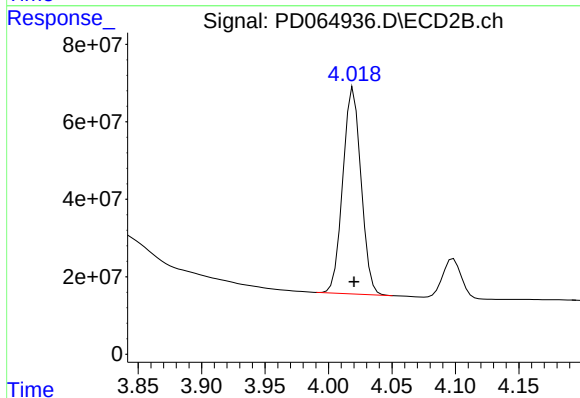


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 530356918
Conc: 26.31 ng/ml

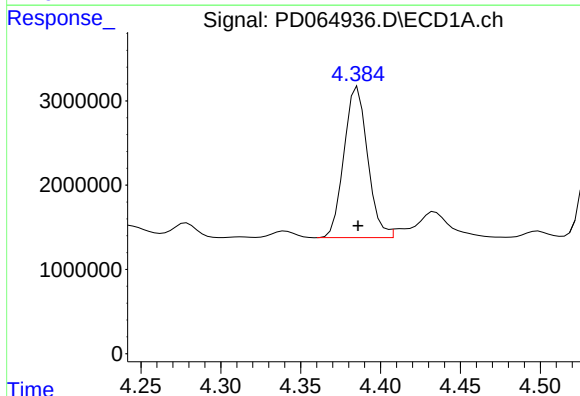


#23 Chlordane-1

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 18409802
Conc: 253.41 ng/ml

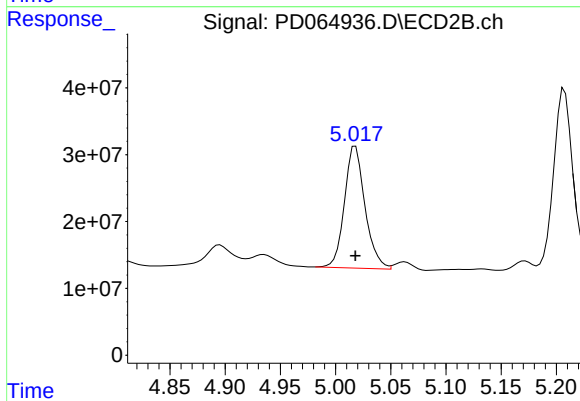

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 236644643
Conc: 263.96 ng/ml

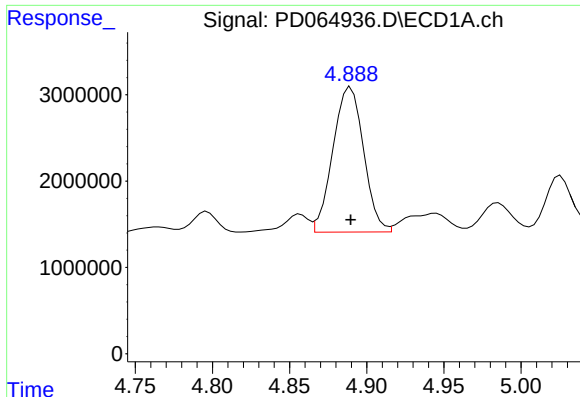

#24 Chlordane-2


R.T.: 4.890 min
Delta R.T.: 0.000 min
Response: 23285942
Conc: 267.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

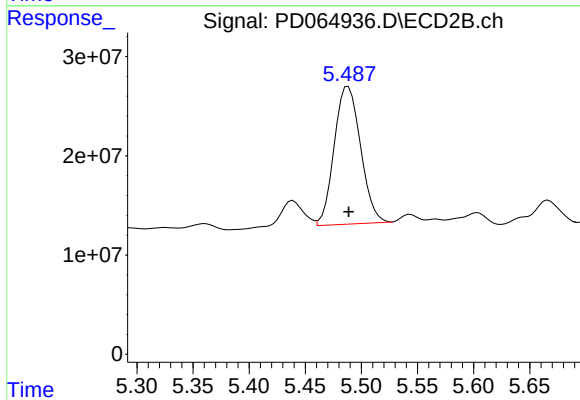


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 226715103
Conc: 272.84 ng/ml

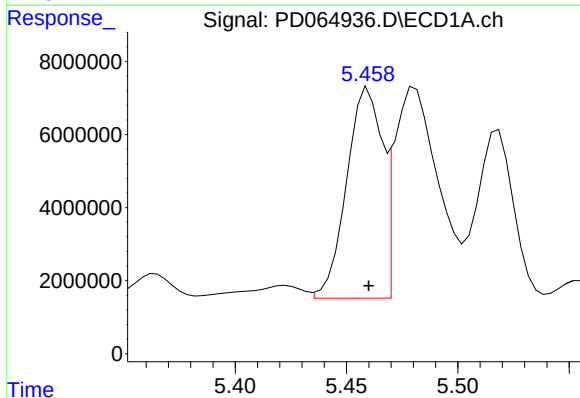


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 63768813
Conc: 246.87 ng/ml

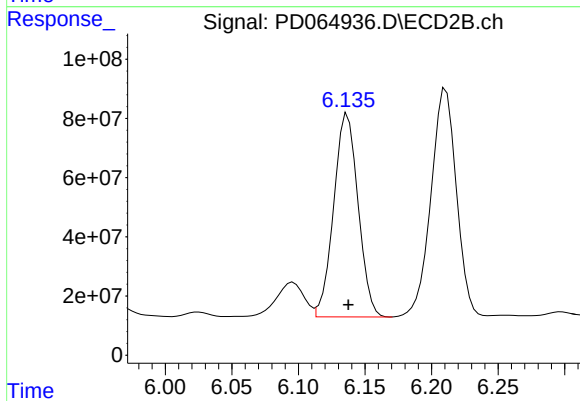

#25 Chlordane-3


R.T.: 6.137 min
Delta R.T.: 0.000 min
Response: 876709843
Conc: 261.41 ng/ml

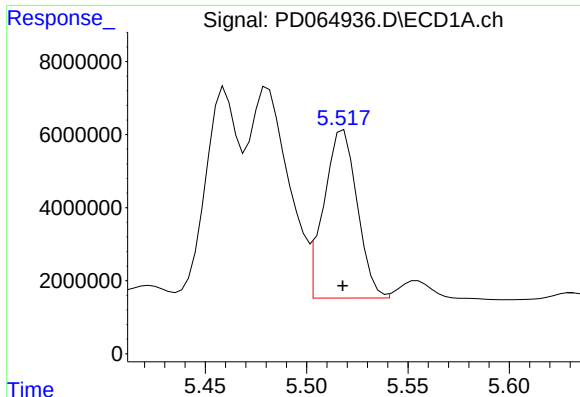

#26 Chlordane-4


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 52812964
Conc: 253.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

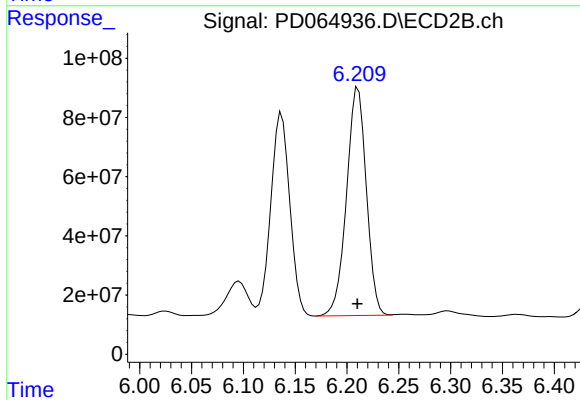


#26 Chlordane-4

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 1024020013
Conc: 263.32 ng/ml

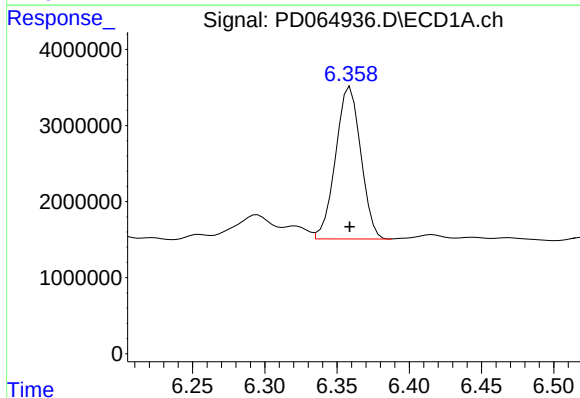


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 24253293
Conc: 258.27 ng/ml

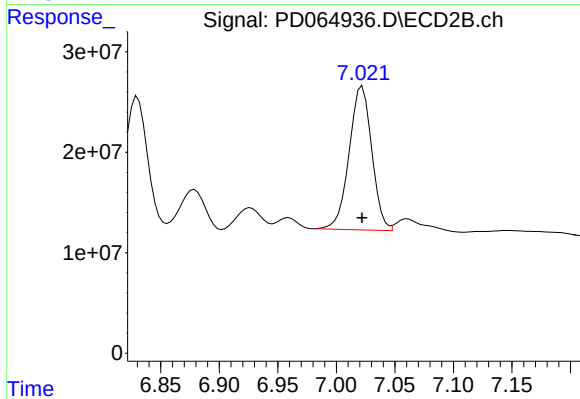

#27 Chlordane-5


R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 192399311
Conc: 263.50 ng/ml

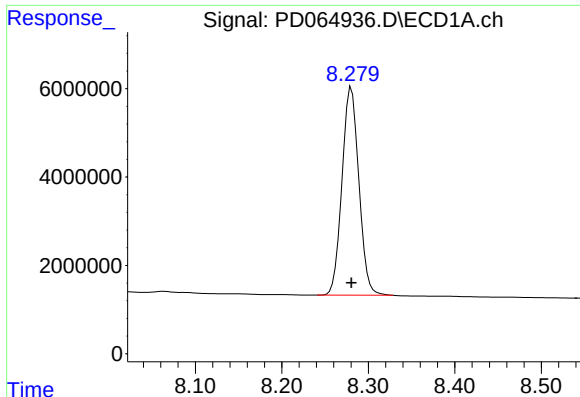

#28 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 63528519
Conc: 26.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

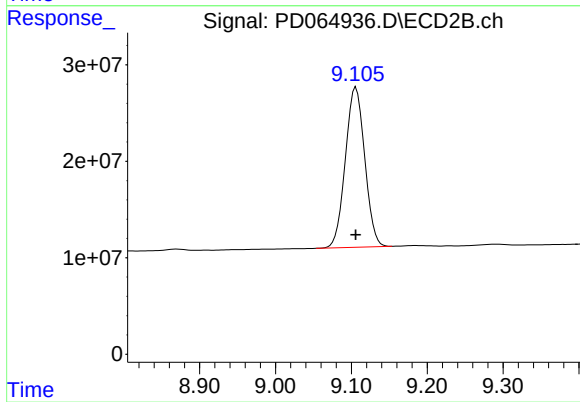

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 294206952
Conc: 27.13 ng/ml