

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 09:41
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 05:01:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	112.6E6	1006.7E6	57.616	49.571
28)	SA Decachlor...	8.279	9.105	109.4E6	559.8E6	44.528	50.369
Target Compounds							
23)	Chlordane-1	4.385	5.017	35254719	449.6E6	485.277	501.493
24)	Chlordane-2	4.889	5.488	41684900	419.4E6	479.621	504.697
25)	Chlordane-3	5.460	6.136	121.1E6	1683.4E6	468.902	501.947
26)	Chlordane-4	5.517	6.209	100.0E6	1951.3E6	480.868	501.779
27)	Chlordane-5	6.359	7.021	44423192	367.8E6	473.048	503.713



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 09:41
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 05:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

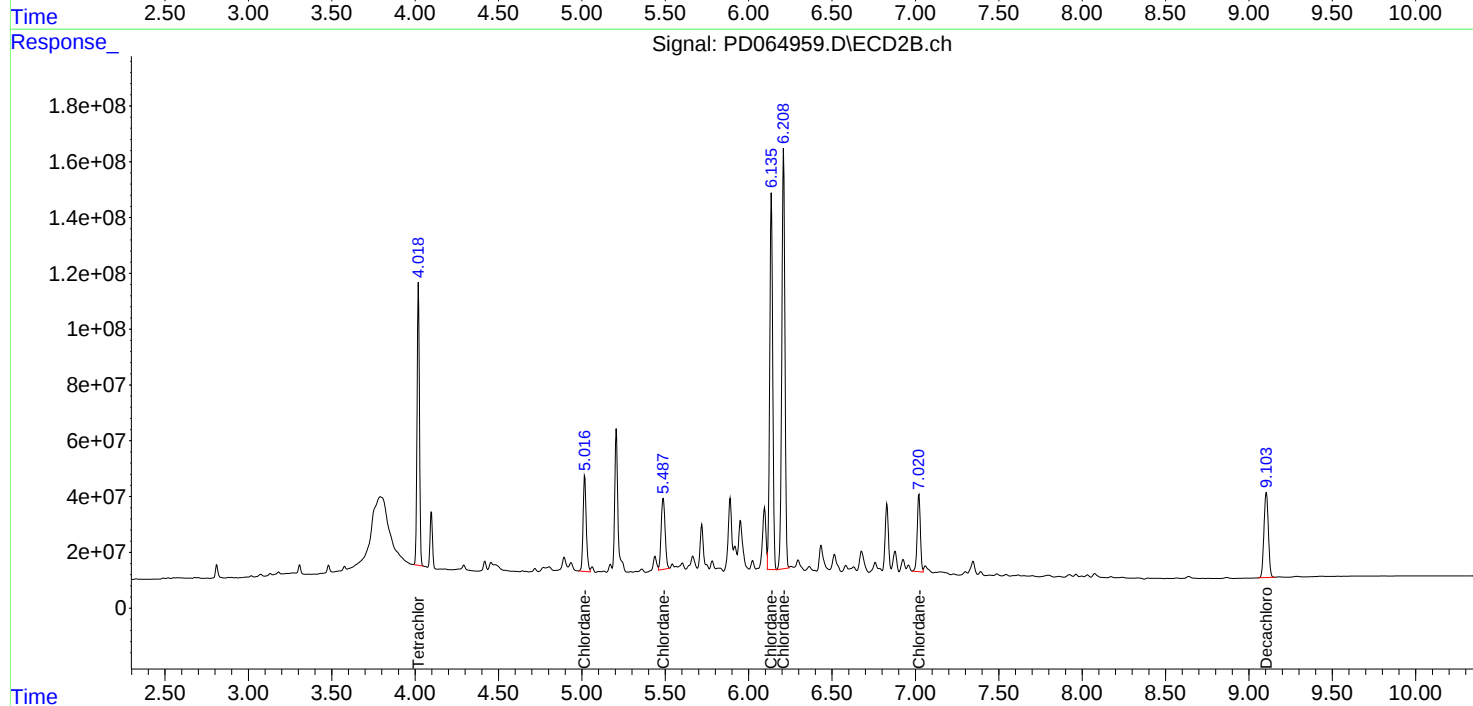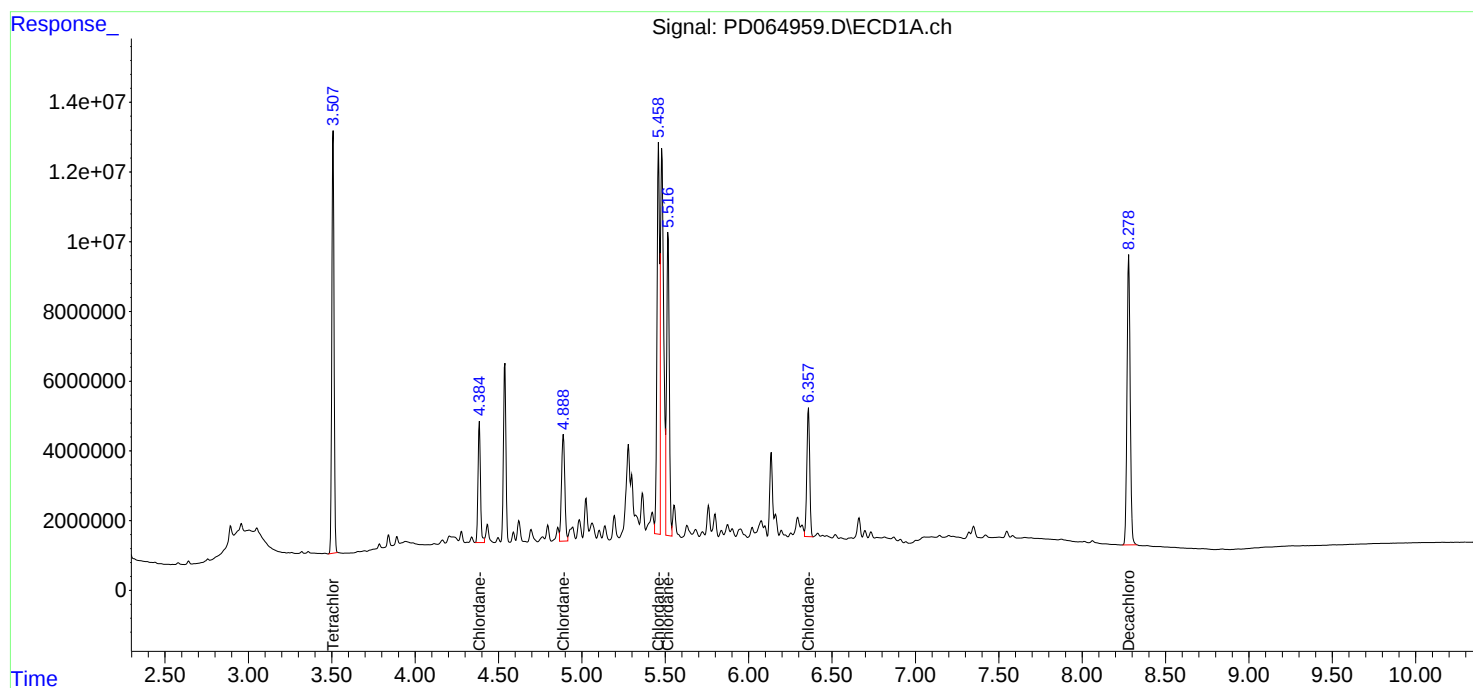


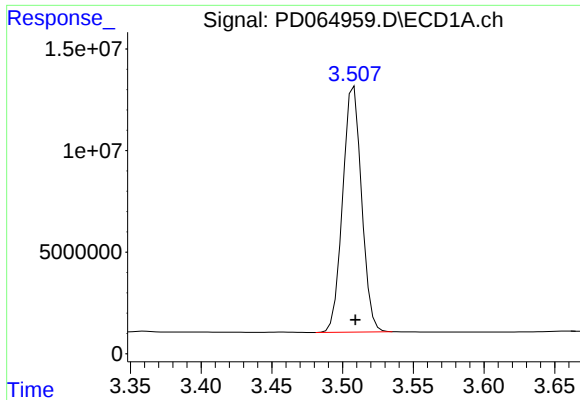

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 112600912
Conc: 57.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

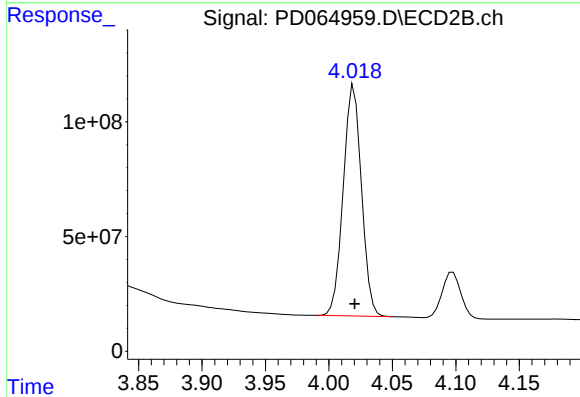


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 1006650364
Conc: 49.57 ng/ml

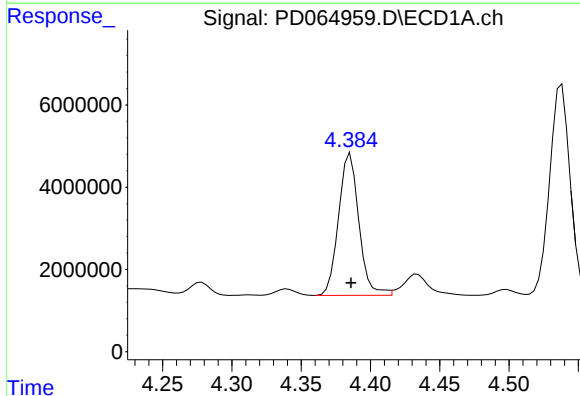


#23 Chlordane-1

R.T.: 4.385 min
Delta R.T.: 0.000 min
Response: 35254719
Conc: 485.28 ng/ml

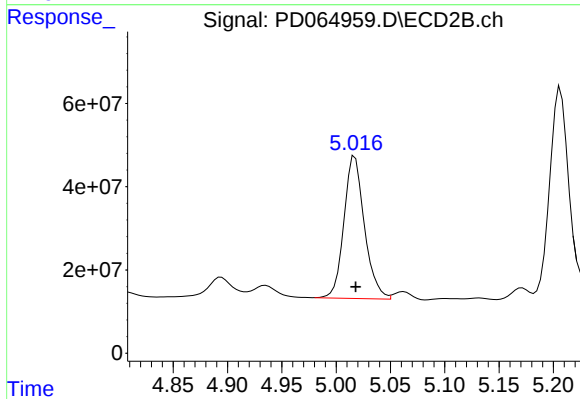

#23 Chlordane-1


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 449594638
Conc: 501.49 ng/ml

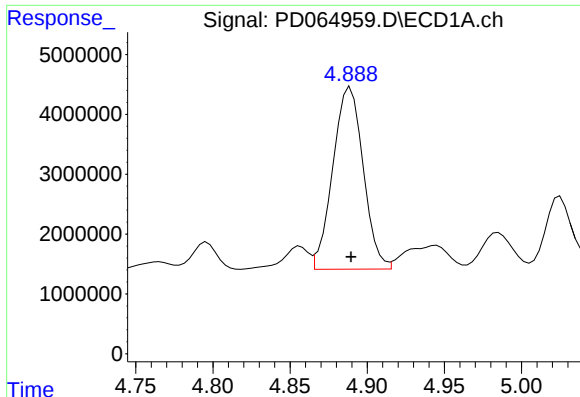

#24 Chlordane-2


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 41684900
Conc: 479.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

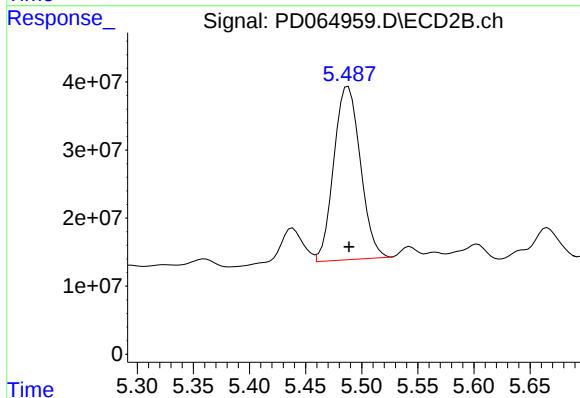


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 419369484
Conc: 504.70 ng/ml

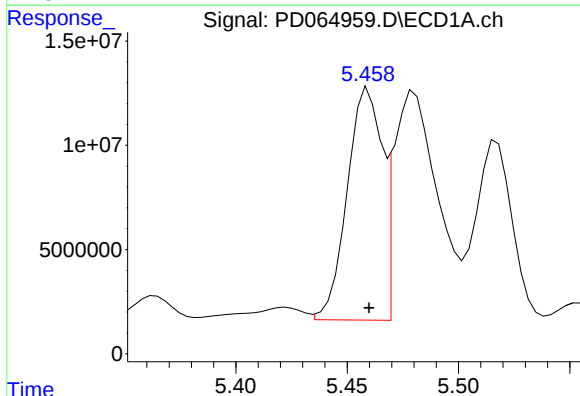


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 121120954
Conc: 468.90 ng/ml

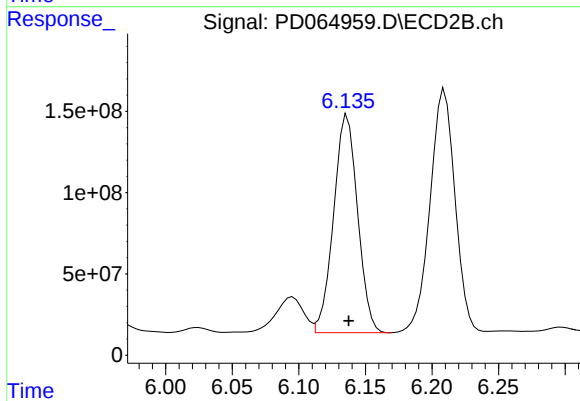

#25 Chlordane-3


R.T.: 6.136 min
Delta R.T.: -0.001 min
Response: 1683419198
Conc: 501.95 ng/ml

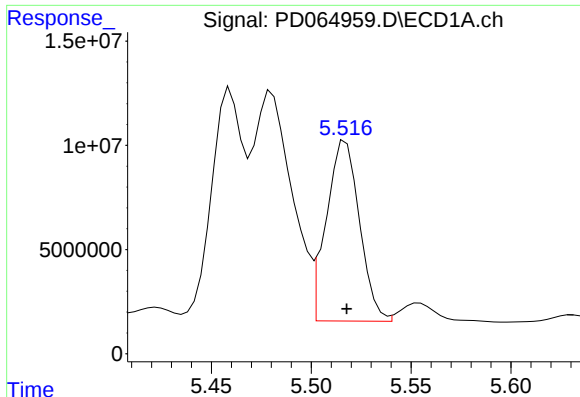

#26 Chlordane-4


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 100041745
Conc: 480.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

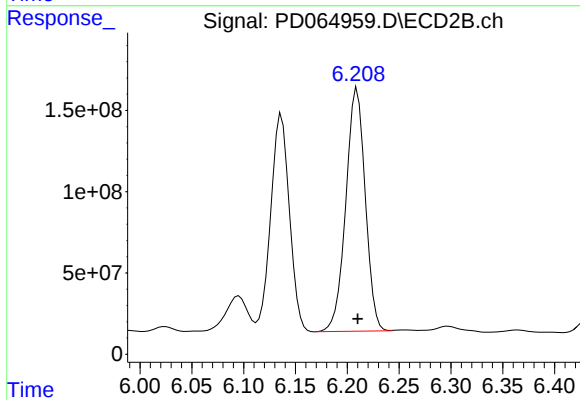


#26 Chlordane-4

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 1951333790
Conc: 501.78 ng/ml

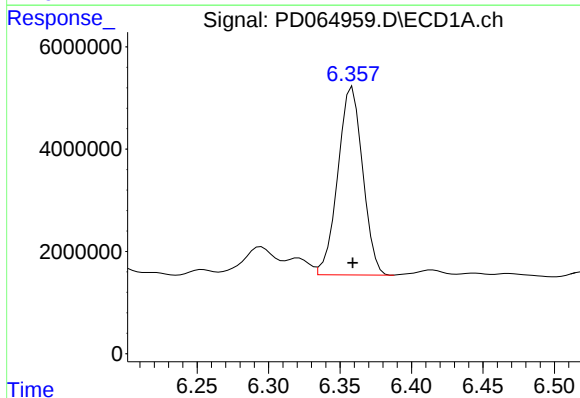


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 44423192
Conc: 473.05 ng/ml

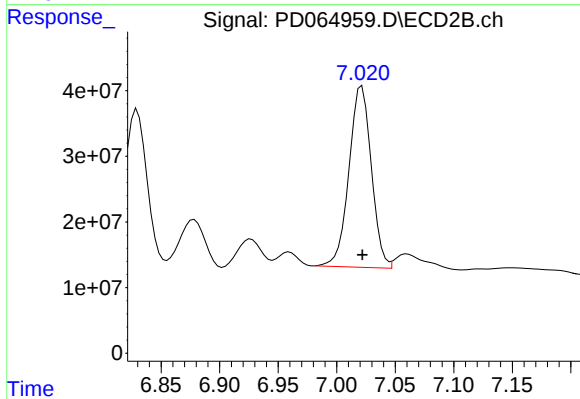

#27 Chlordane-5


R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 367800829
Conc: 503.71 ng/ml

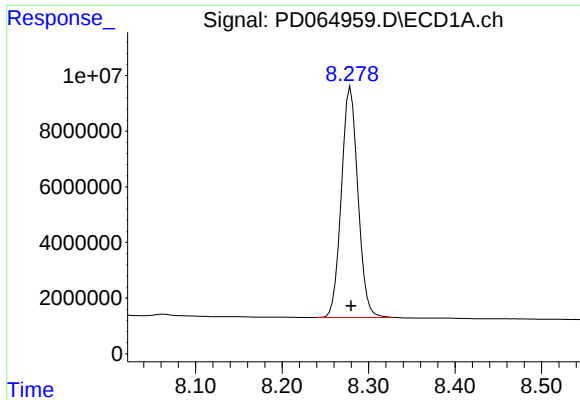

#28 Decachlorobiphenyl

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 109432534
Conc: 44.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

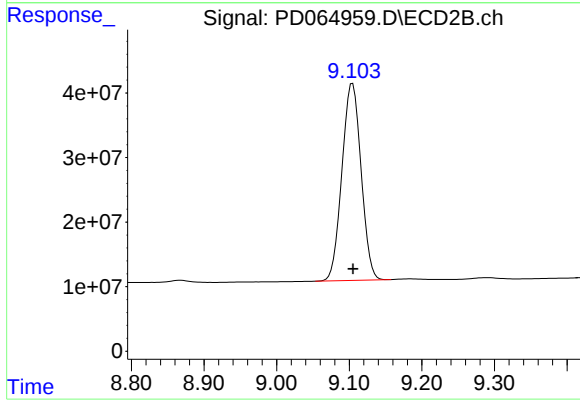

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 559793227
Conc: 50.37 ng/ml