

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
 Data File : PD064970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2021 12:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 05:03:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 16 03:35:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.020	110.8E6	1000.9E6	56.688	49.287
28)	SA Decachlor...	8.280	9.106	71102820	563.1E6	28.932	50.662 #
Target Compounds							
23)	Chlordane-1	4.386	5.018	31120494	448.4E6	428.370	500.140
24)	Chlordane-2	4.889	5.488	31928771	417.3E6	367.368	502.260 #
25)	Chlordane-3	5.460	6.137	84630964	1673.2E6	327.636	498.909 #
26)	Chlordane-4	5.518	6.210	70040421	1942.0E6	336.662	499.389 #
27)	Chlordane-5	6.359	7.022	31722511	364.4E6	337.803	499.015 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081421\
Data File : PD064970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2021 12:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 05:03:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081421.M
Quant Title : GC Extractables
QLast Update : Mon Aug 16 03:35:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

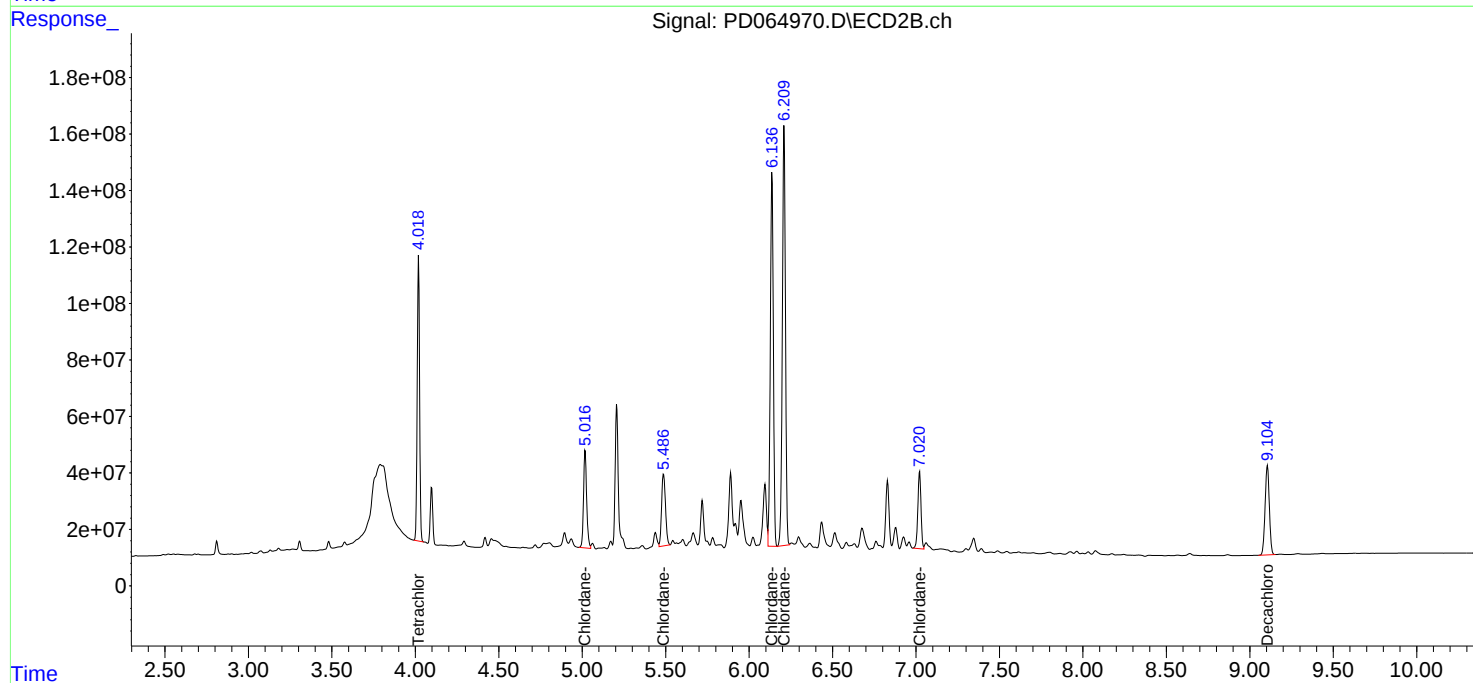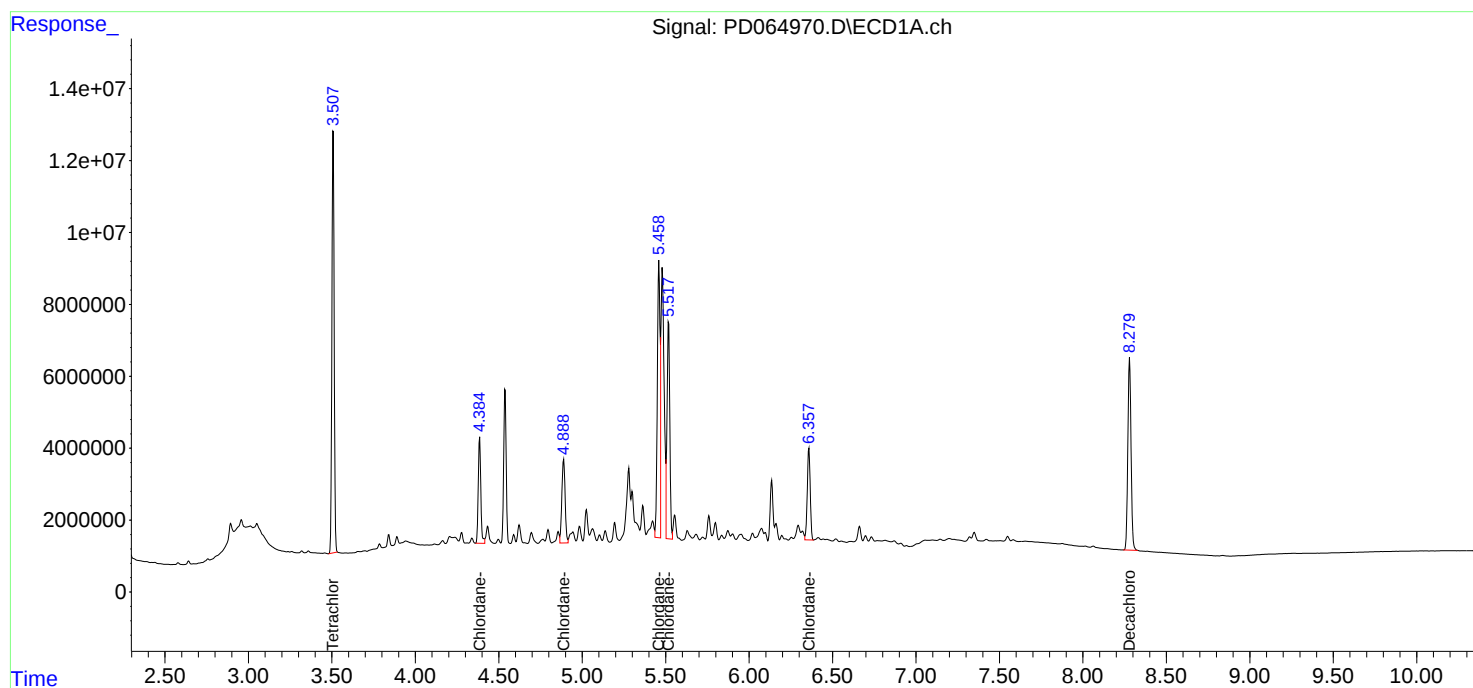


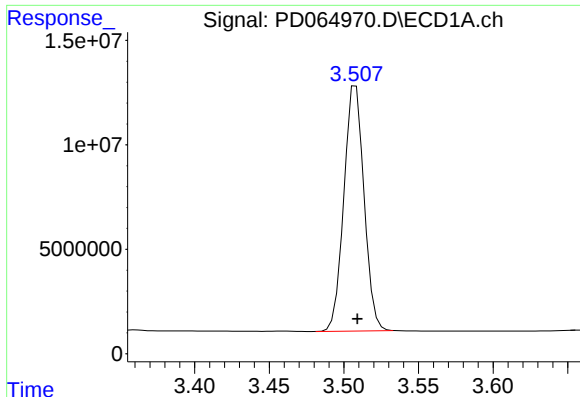

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 110786969
Conc: 56.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

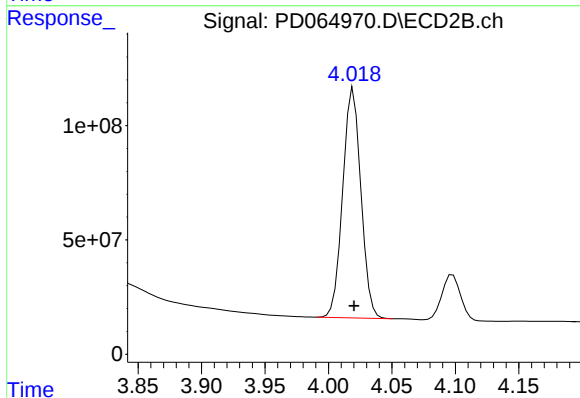


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 1000875727
Conc: 49.29 ng/ml

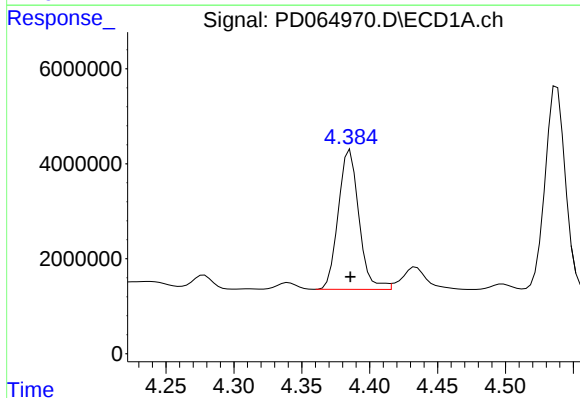


#23 Chlordane-1

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 31120494
Conc: 428.37 ng/ml

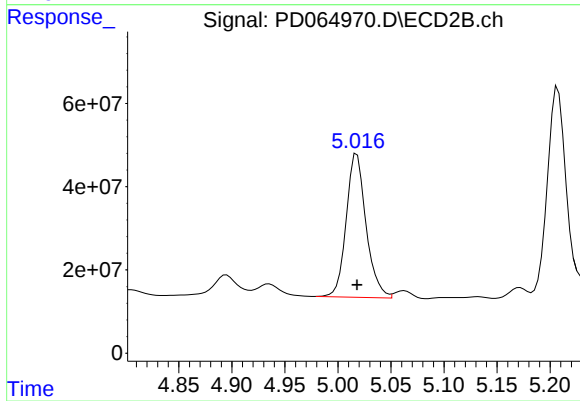

#23 Chlordane-1


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 448381967
Conc: 500.14 ng/ml

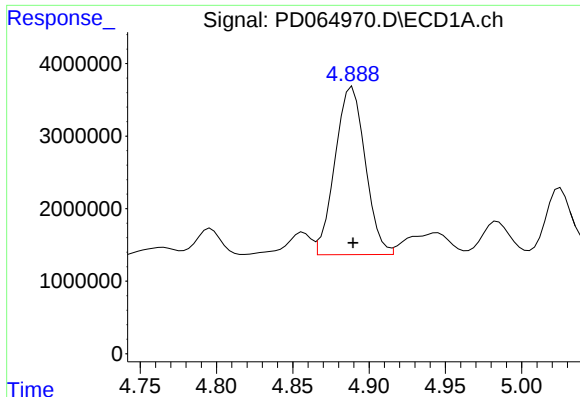

#24 Chlordane-2


R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 31928771
Conc: 367.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

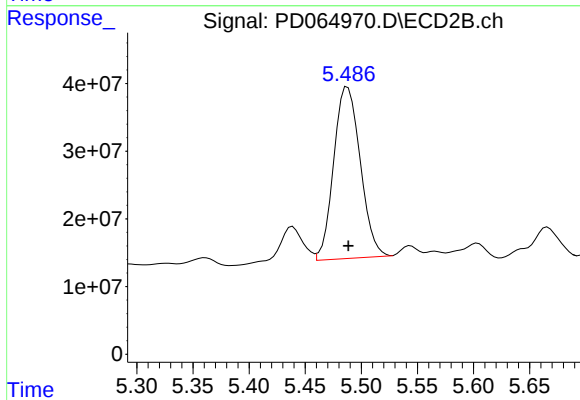


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 417344768
Conc: 502.26 ng/ml

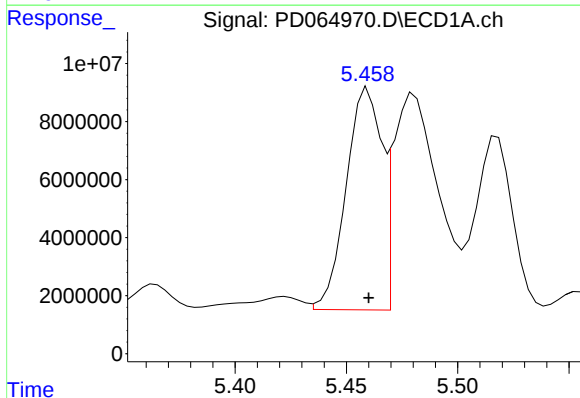


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 84630964
Conc: 327.64 ng/ml

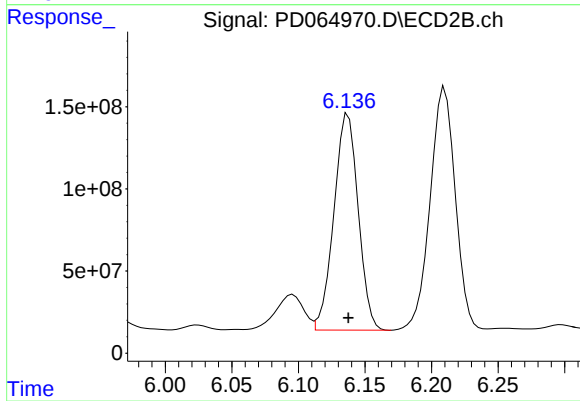

#25 Chlordane-3


R.T.: 6.137 min
Delta R.T.: 0.000 min
Response: 1673231801
Conc: 498.91 ng/ml

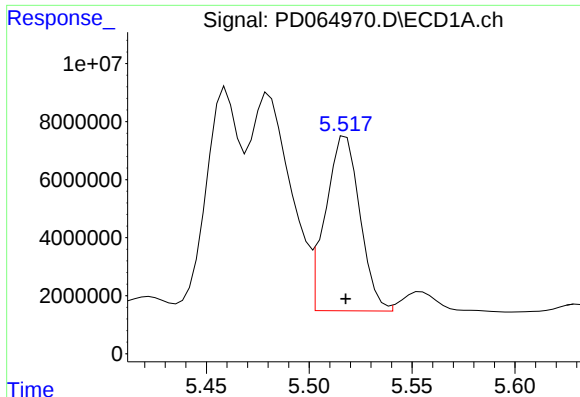

#26 Chlordane-4


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 70040421
Conc: 336.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

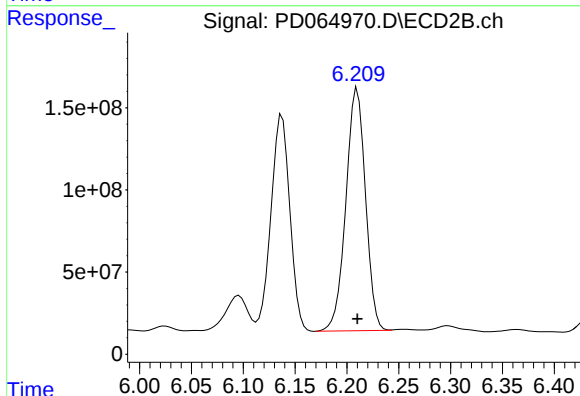


#26 Chlordane-4

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 1942039319
Conc: 499.39 ng/ml

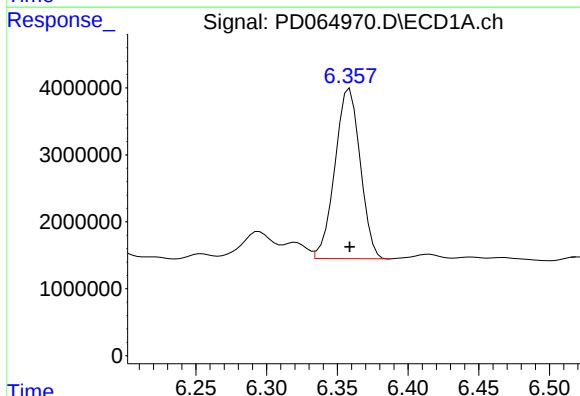


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 31722511
Conc: 337.80 ng/ml

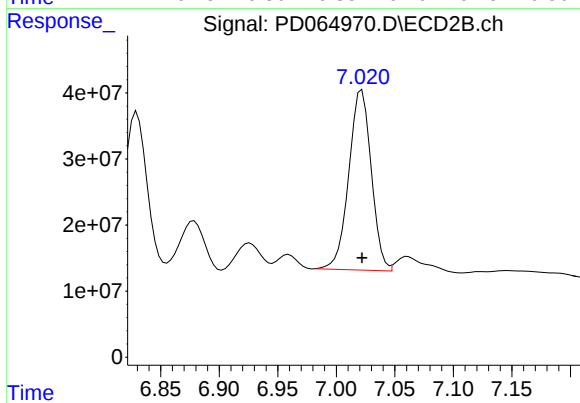

#27 Chlordane-5


R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 364370938
Conc: 499.02 ng/ml

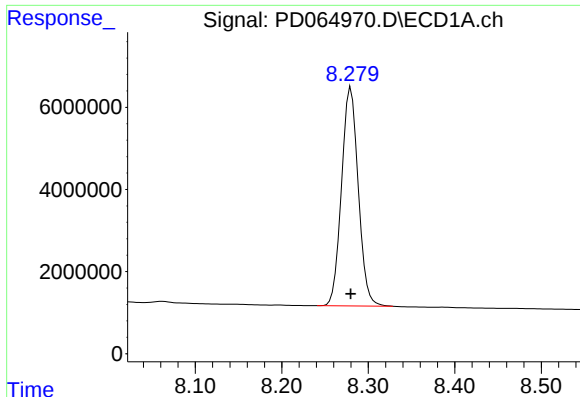

#28 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 71102820
Conc: 28.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

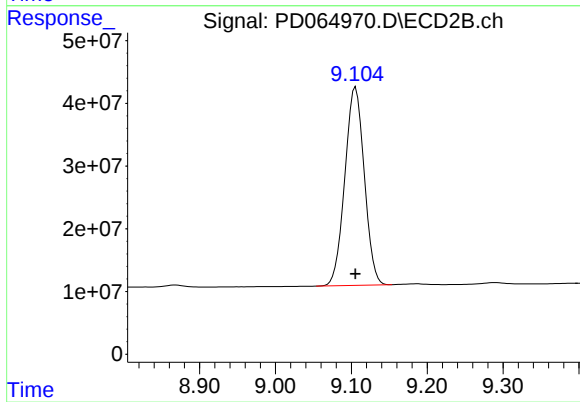

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 563054427
Conc: 50.66 ng/ml