

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 09:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:57:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
15) B	Endosulfa...	6.780	5.876f	5539117	393401	1.960 0.294 #
16) A	4,4'-DDD	6.780f	0.000	5539117	0	2.549 N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 09:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:57:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

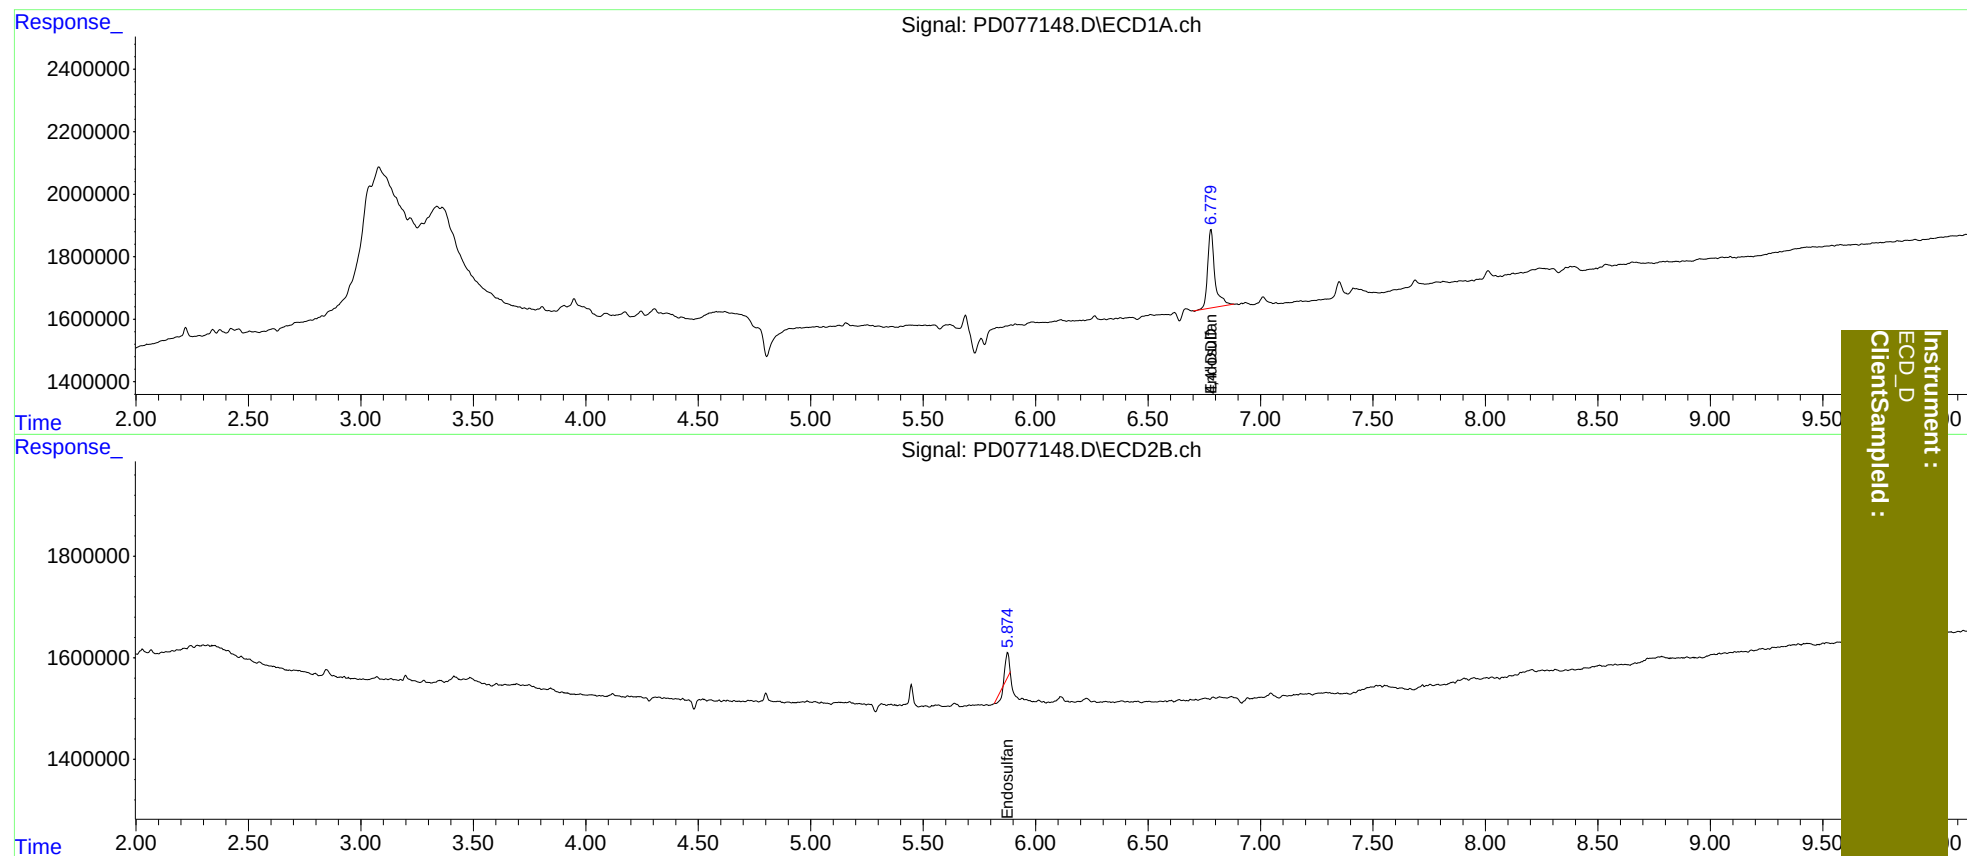


Instrument :
ECD_D
ClientSampled :
0

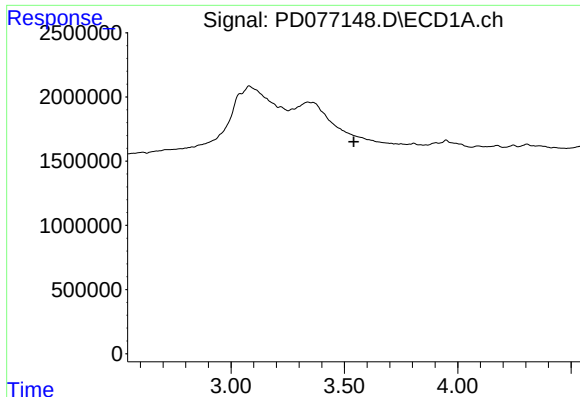

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

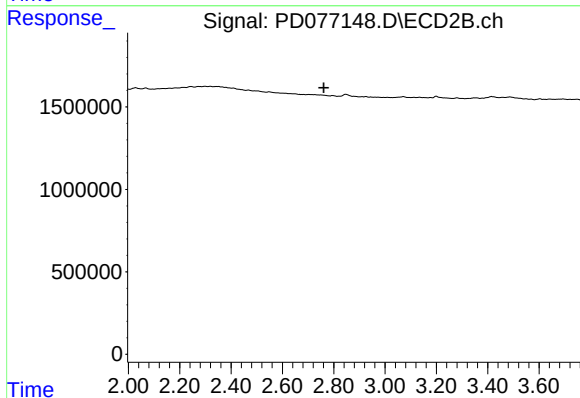


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.761 min
Response: 0
Conc: N.D.

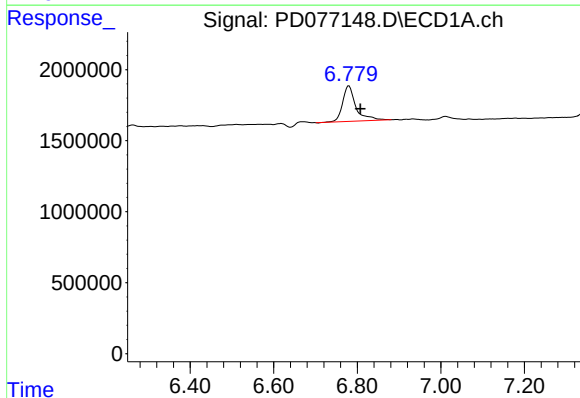


#15 Endosulfan II

R.T.: 6.780 min
Delta R.T.: -0.027 min
Response: 5539117
Conc: 1.96 ng/ml

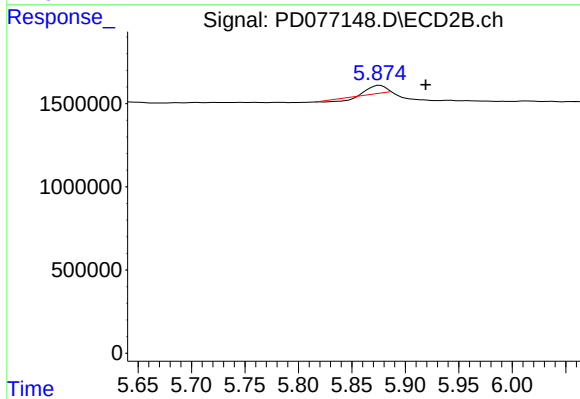

#15 Endosulfan II


R.T.: 5.876 min
Delta R.T.: -0.043 min
Response: 393401
Conc: 0.29 ng/ml

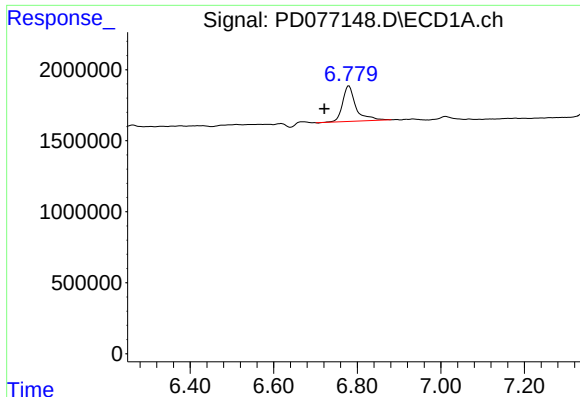

#16 4,4'-DDD


R.T.: 6.780 min
Delta R.T.: 0.059 min
Response: 5539117
Conc: 2.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

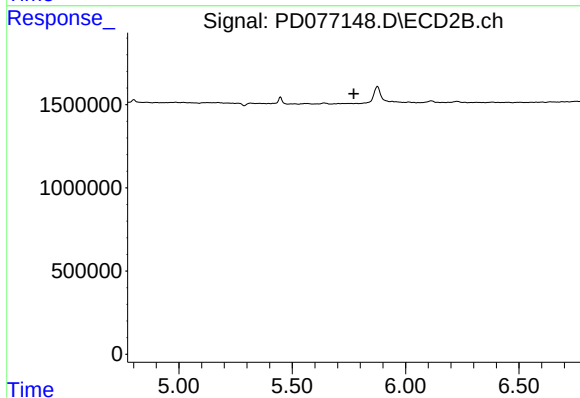


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.772 min
Response: 0
Conc: N.D.

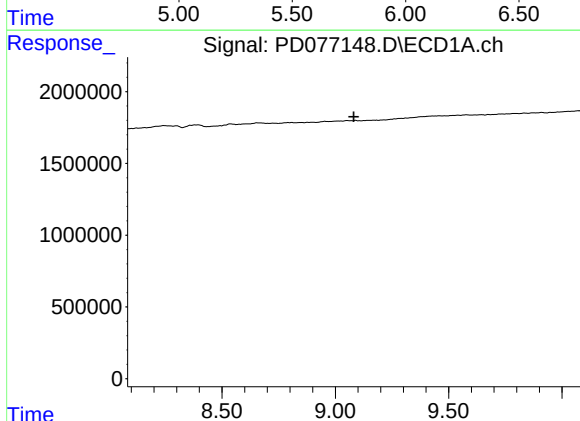

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.082 min
Response: 0
Conc: N.D.

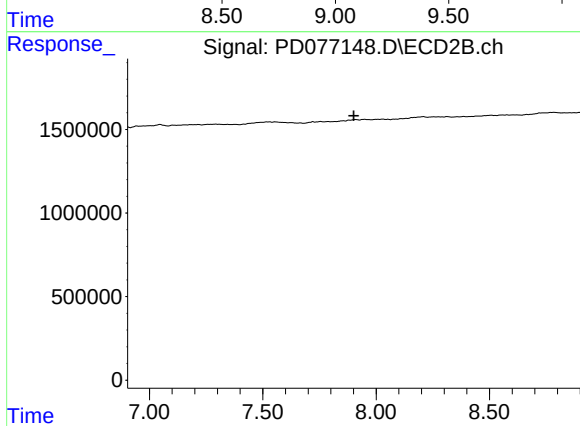

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.901 min
Response: 0
Conc: N.D.