

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 11:28
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:31:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:29:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	11283197	6475439	5.138	5.189
27)	SA Decachlor...	9.084	7.903	28493937	13416791	11.324	10.838
Target Compounds							
2)	A alpha-BHC	3.999	3.263	16589041	8848779	4.610	4.872
3)	MA gamma-BHC...	4.332	3.593	16350143	8413427	4.823	4.913
4)	MA Heptachlor	4.923	3.932	17174582	8678965	4.967	5.076
9)	A Endosulfan I	6.081	5.084	14540838	7065030	5.194	4.979
13)	MA Dieldrin	6.357	5.349	30030953	15167200	9.688	9.578
14)	MA Endrin	6.587	5.625	24642056	13524390	9.738	9.766
16)	A 4,4'-DDD	6.721	5.772	20885840	9441584	9.763	9.516
17)	MA 4,4'-DDT	7.036	6.024	20039827	8928654	9.156	8.652
20)	A Methoxychlor	7.513	6.599	65173477	28169215	50.762	49.112


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 11:28
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:31:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:29:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

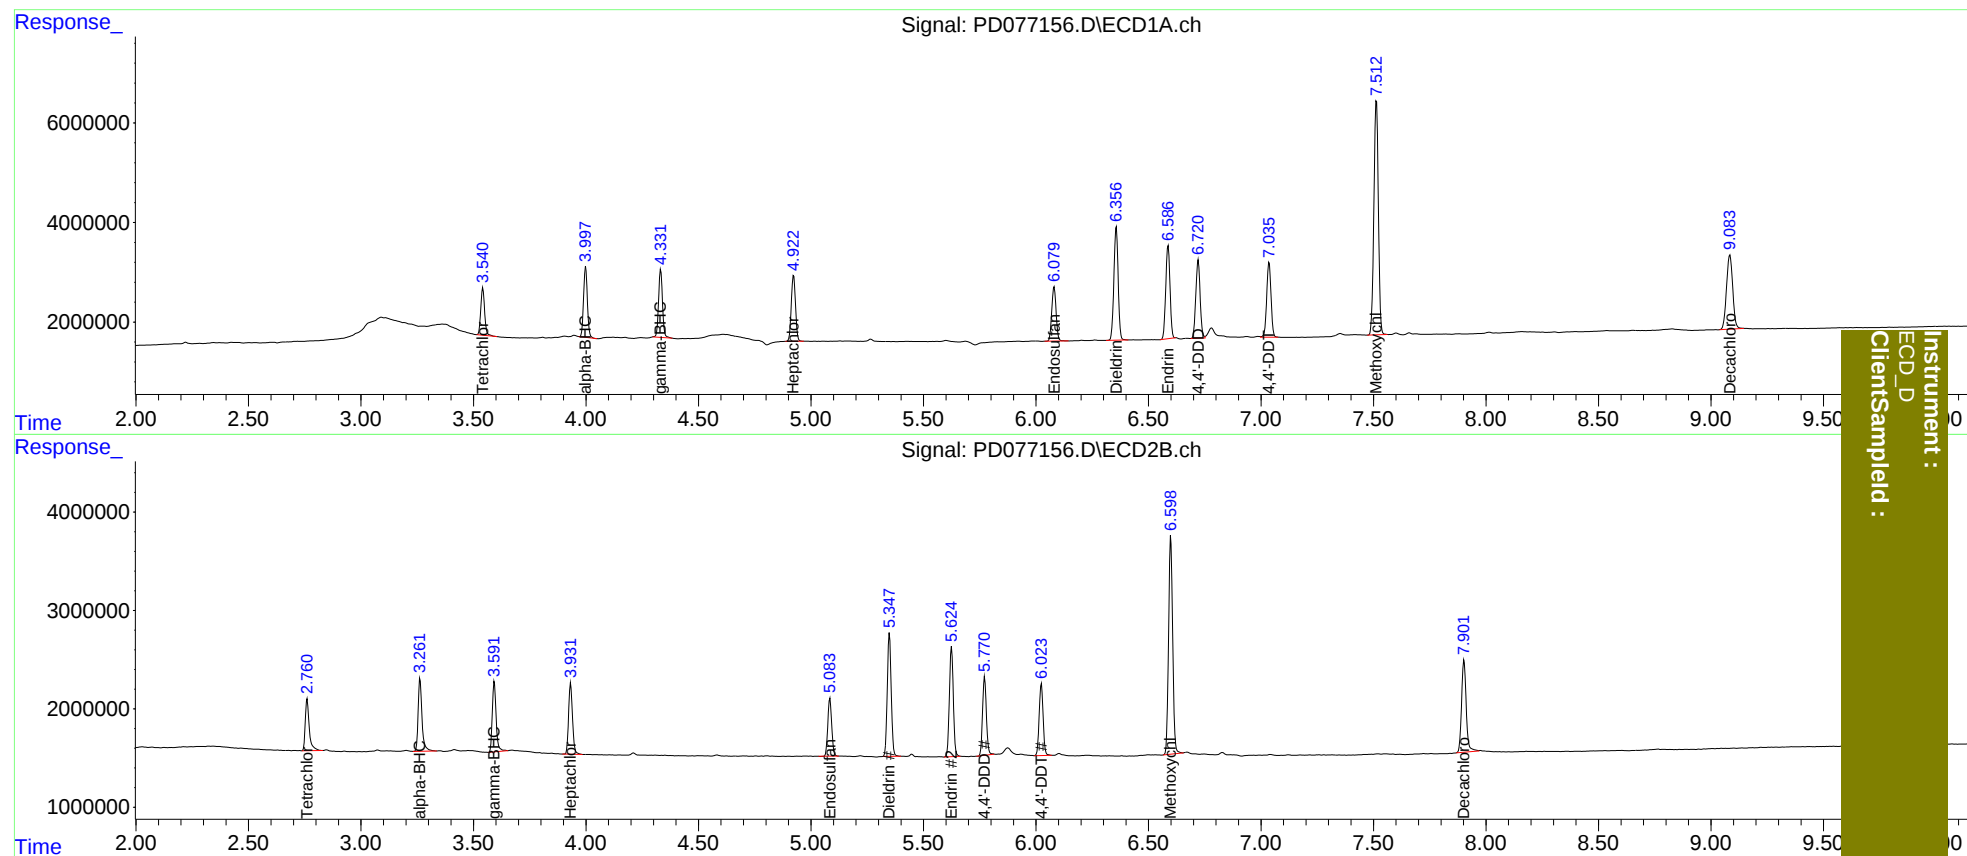


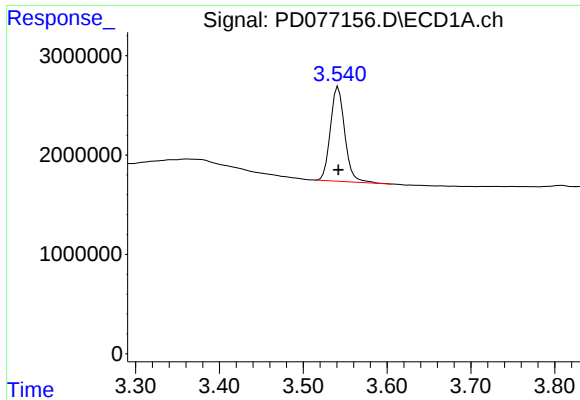

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 11283197
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

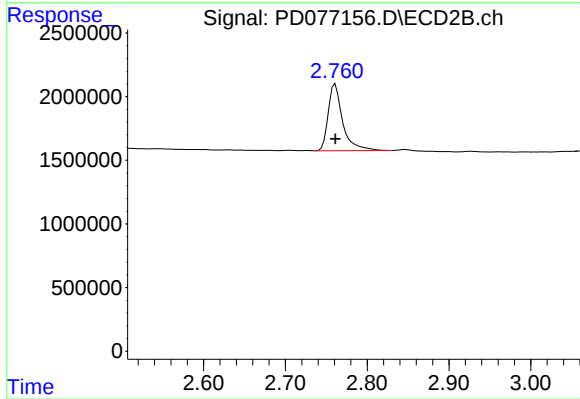


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 6475439
Conc: 5.19 ng/ml

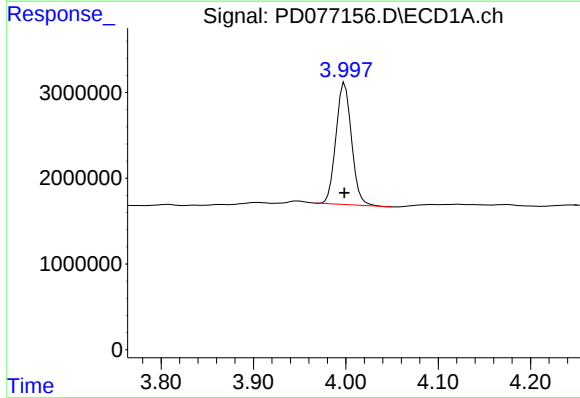


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 16589041
Conc: 4.61 ng/ml

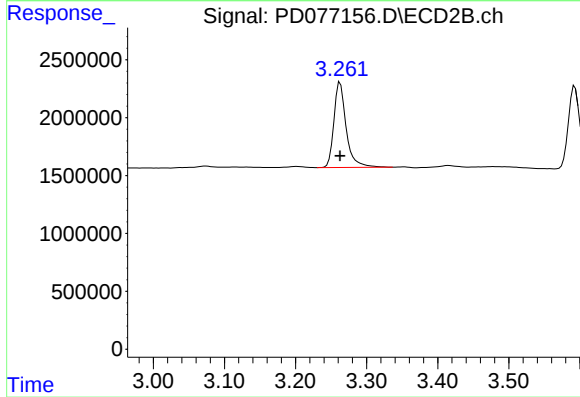

#2 alpha-BHC


R.T.: 3.263 min
Delta R.T.: 0.000 min
Response: 8848779
Conc: 4.87 ng/ml

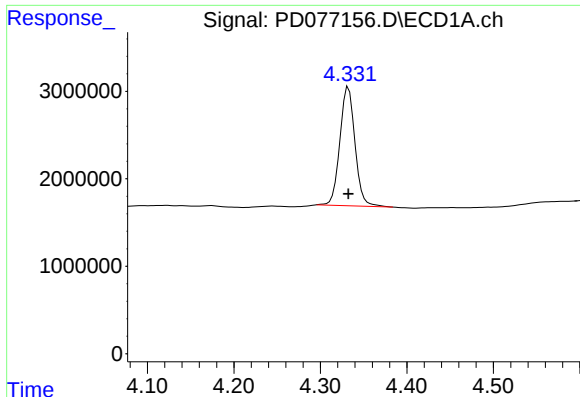

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 16350143
Conc: 4.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

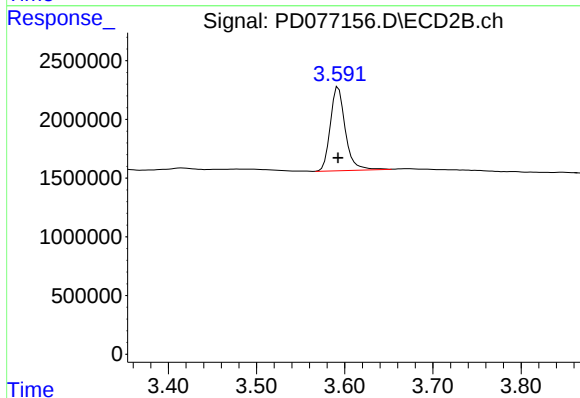


#3 gamma-BHC (Lindane)

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 8413427
Conc: 4.91 ng/ml

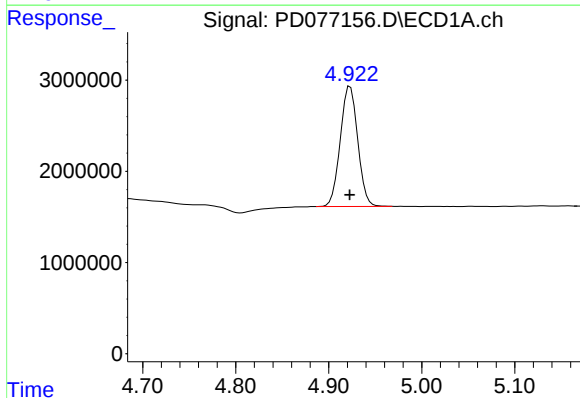


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 17174582
Conc: 4.97 ng/ml

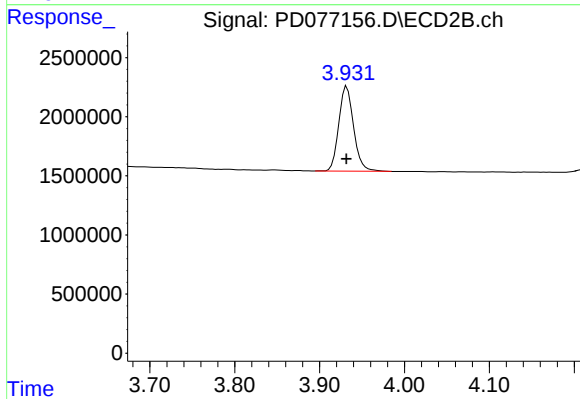

#4 Heptachlor


R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 8678965
Conc: 5.08 ng/ml

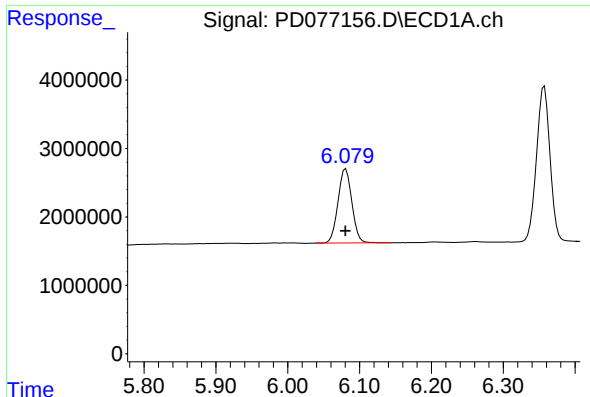

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 14540838
Conc: 5.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

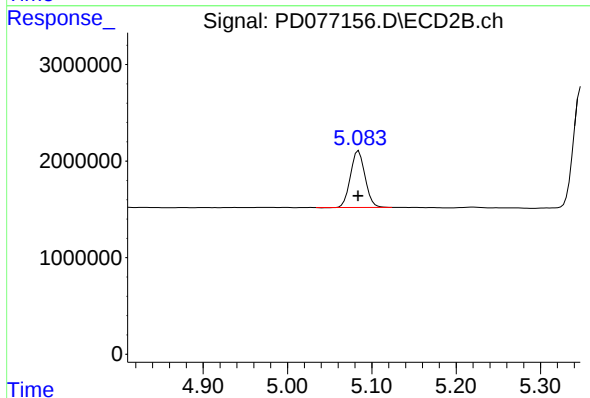


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 7065030
Conc: 4.98 ng/ml

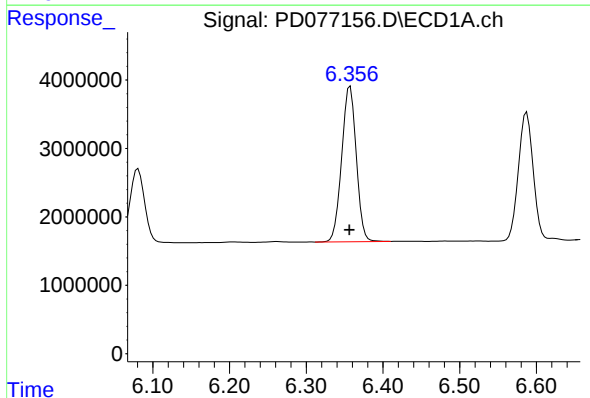


#13 Dieldrin

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 30030953
Conc: 9.69 ng/ml

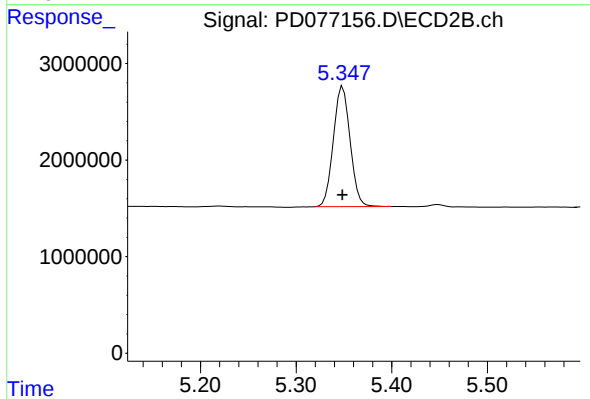

#13 Dieldrin


R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 15167200
Conc: 9.58 ng/ml

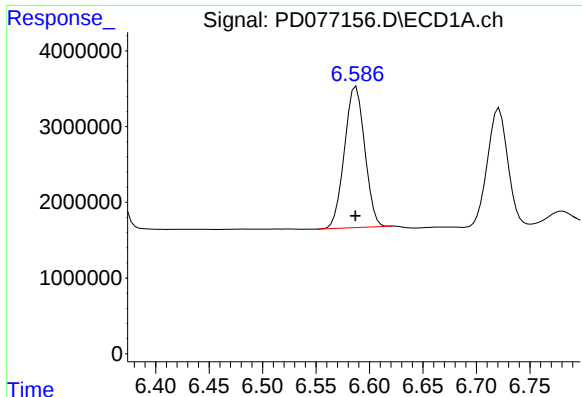

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 24642056
Conc: 9.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

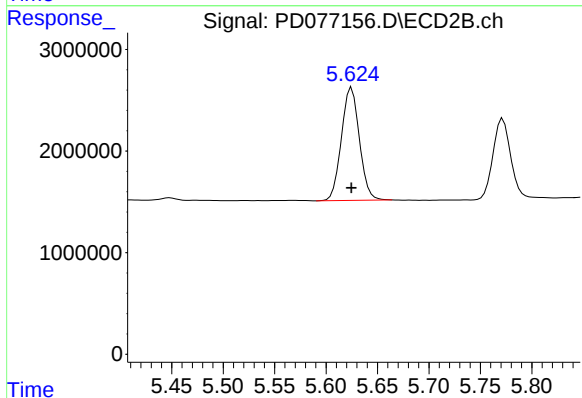


#14 Endrin

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 13524390
Conc: 9.77 ng/ml

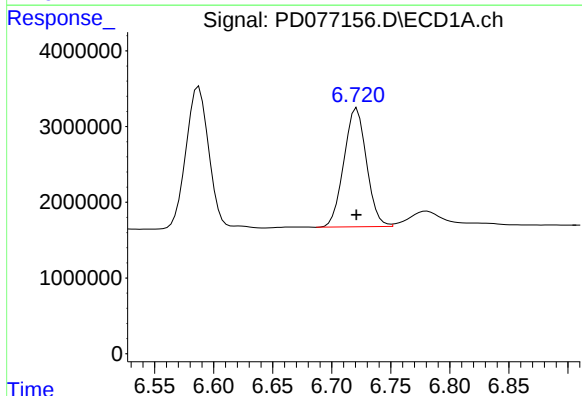


#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: 0.000 min
Response: 20885840
Conc: 9.76 ng/ml

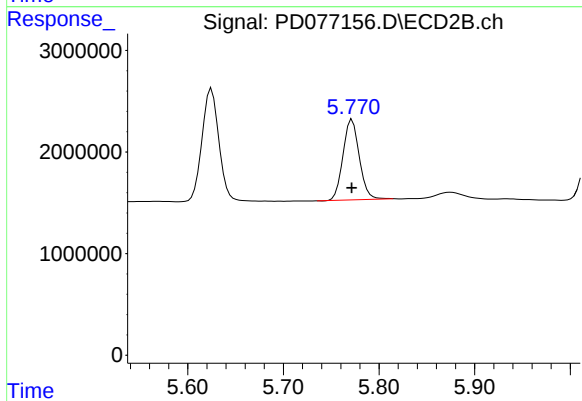

#16 4,4'-DDD


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 9441584
Conc: 9.52 ng/ml

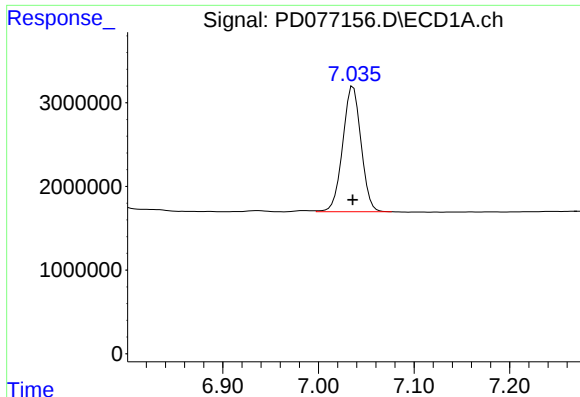

#17 4,4'-DDT


R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 20039827
Conc: 9.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

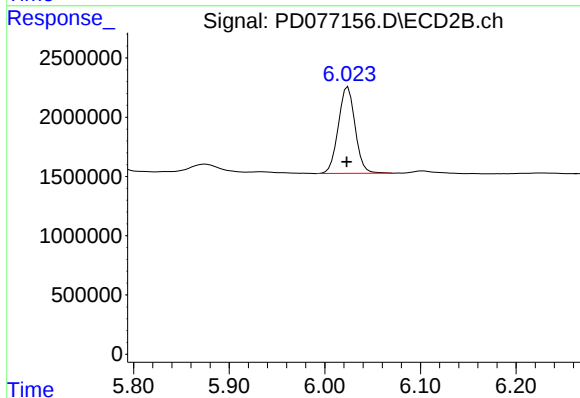


#17 4,4'-DDT

R.T.: 6.024 min
Delta R.T.: 0.001 min
Response: 8928654
Conc: 8.65 ng/ml

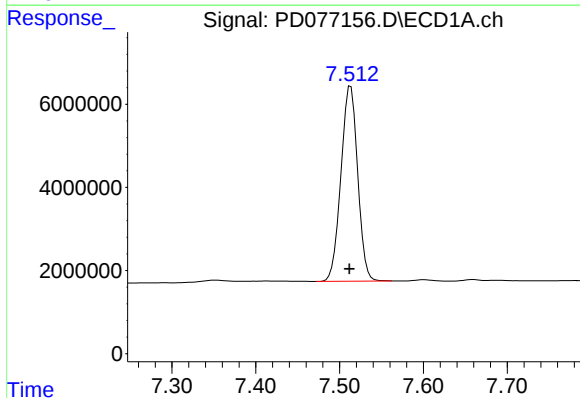


#20 Methoxychlor

R.T.: 7.513 min
Delta R.T.: 0.002 min
Response: 65173477
Conc: 50.76 ng/ml

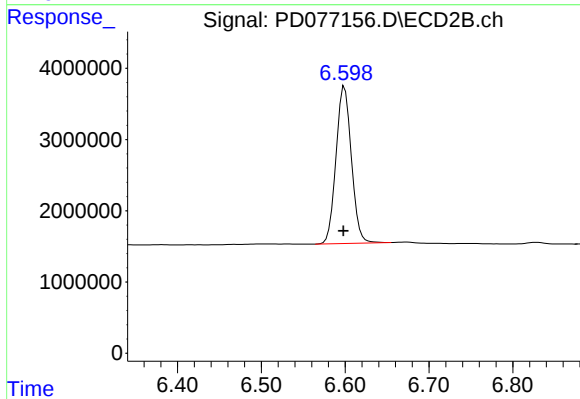

#20 Methoxychlor


R.T.: 6.599 min
Delta R.T.: 0.001 min
Response: 28169215
Conc: 49.11 ng/ml

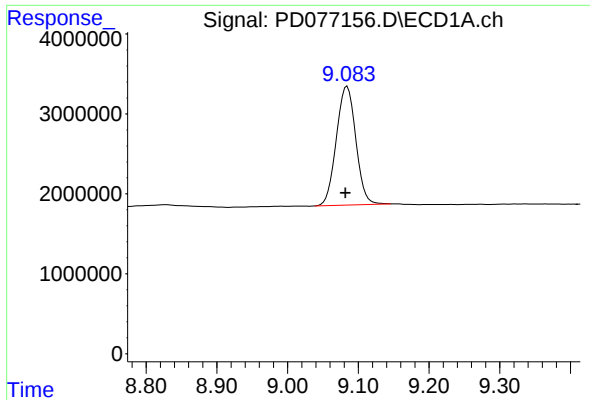

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.002 min
Response: 28493937
Conc: 11.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

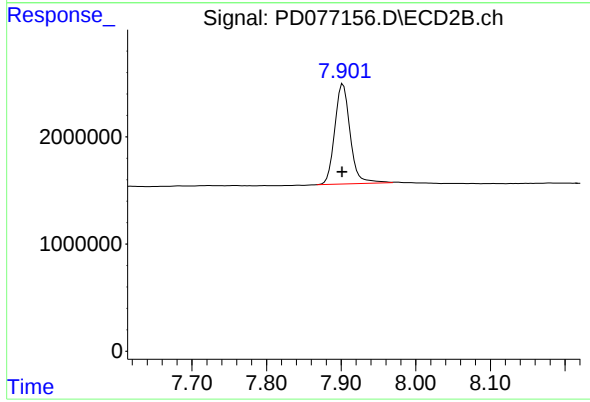

#27 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.001 min
Response: 13416791
Conc: 10.84 ng/ml