

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 11:55
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:31:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:29:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	22264975	12700238	10.139	10.177
27)	SA Decachlor...	9.084	7.902	53348393	25564458	21.202	20.651
Target Compounds							
2)	A alpha-BHC	3.999	3.262	34287929	17646096	9.529	9.715
3)	MA gamma-BHC...	4.332	3.592	32844919	16855999	9.690	9.843
4)	MA Heptachlor	4.923	3.931	34305103	16892046	9.921	9.880
9)	A Endosulfan I	6.081	5.084	28207806	13992747	10.076	9.862
13)	MA Dieldrin	6.357	5.349	60229874	30647622	19.430	19.354
14)	MA Endrin	6.587	5.625	49510189	27179936	19.565	19.626
16)	A 4,4'-DDD	6.721	5.772	42234393	19119261	19.742	19.270
17)	MA 4,4'-DDT	7.036	6.024	41791958	19099639	19.094	18.508
20)	A Methoxychlor	7.512	6.599	129.4E6	57162095	100.810	99.660


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 11:55
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:31:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:29:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

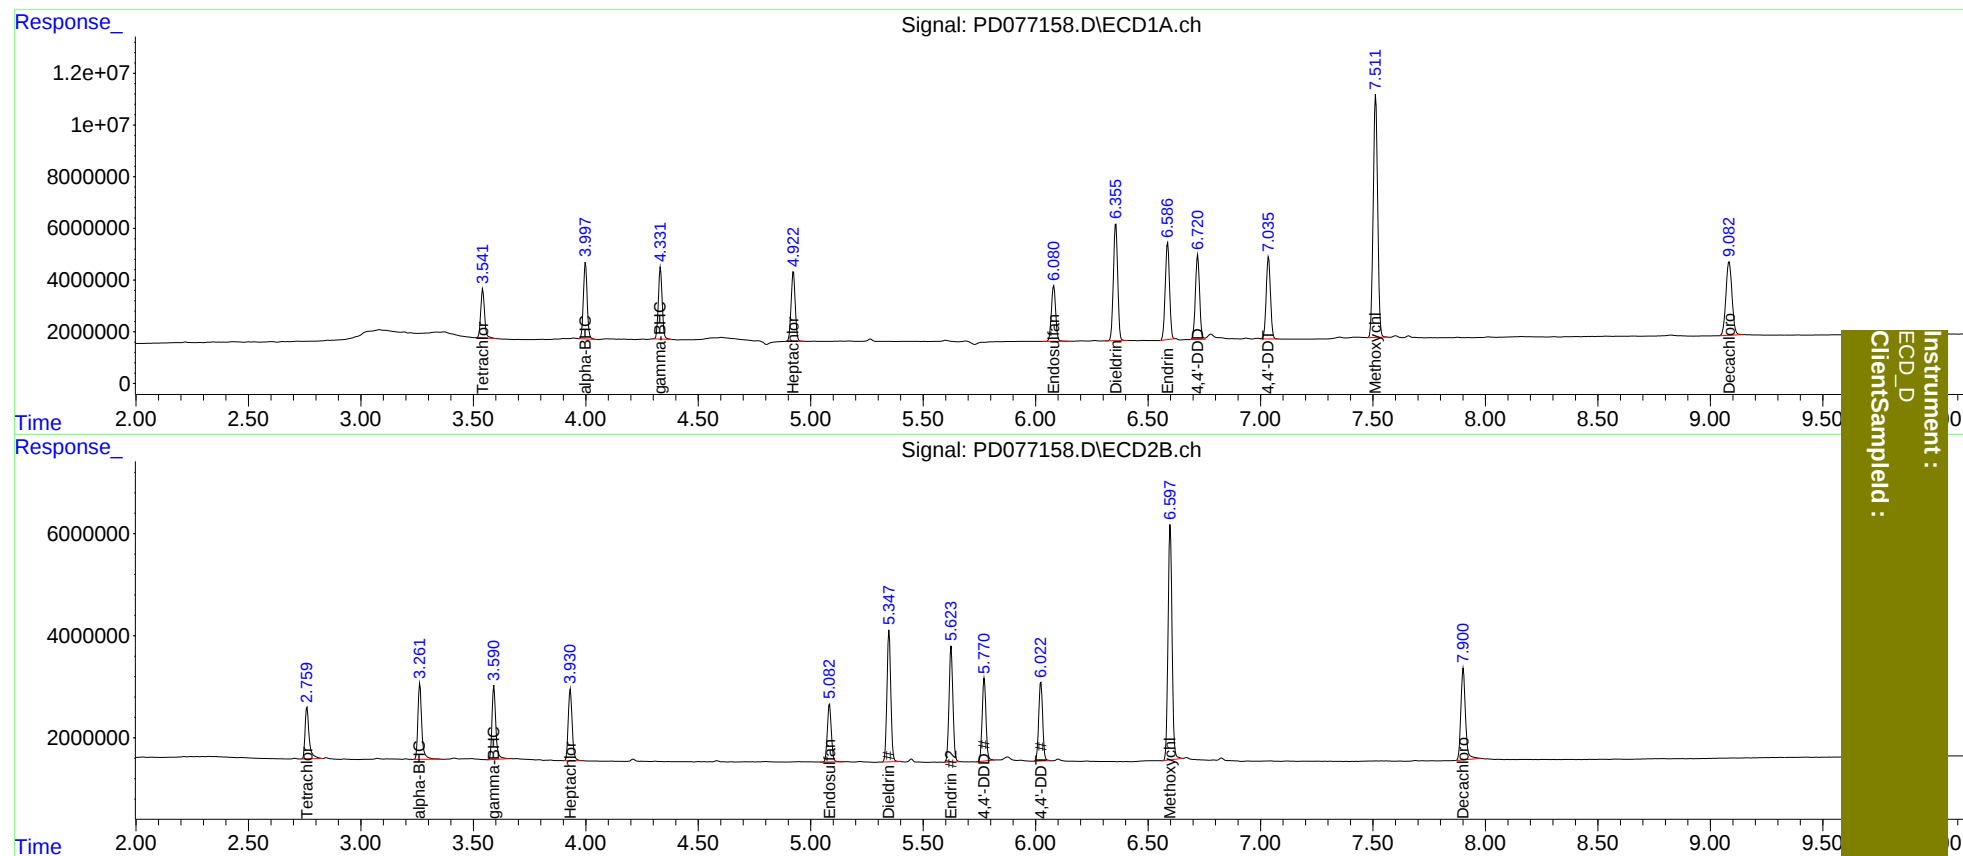


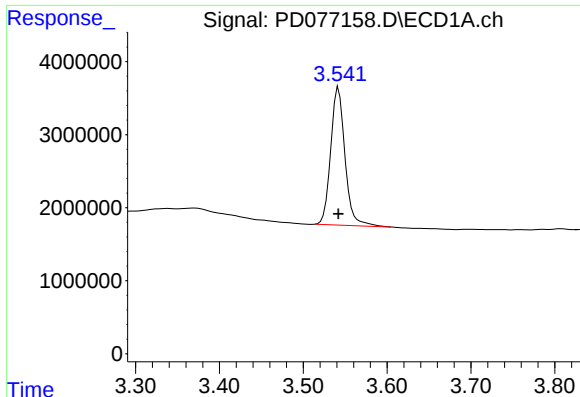

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 22264975
Conc: 10.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

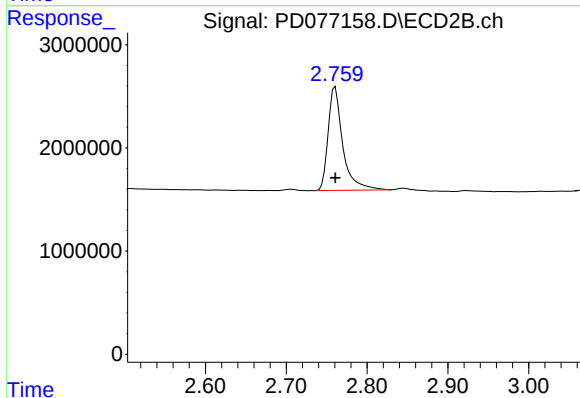


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 12700238
Conc: 10.18 ng/ml

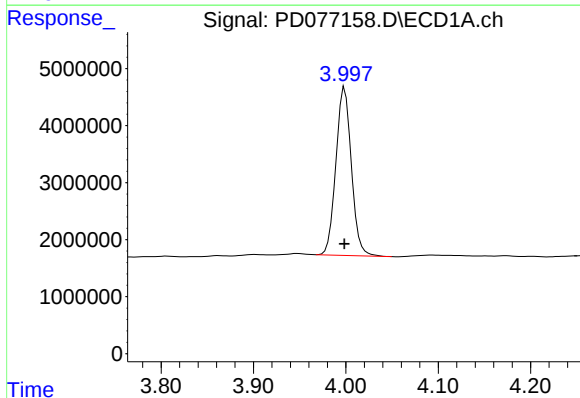


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 34287929
Conc: 9.53 ng/ml

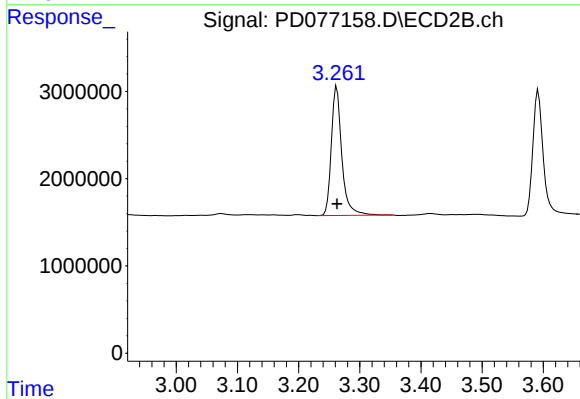

#2 alpha-BHC


R.T.: 3.262 min
Delta R.T.: 0.000 min
Response: 17646096
Conc: 9.72 ng/ml

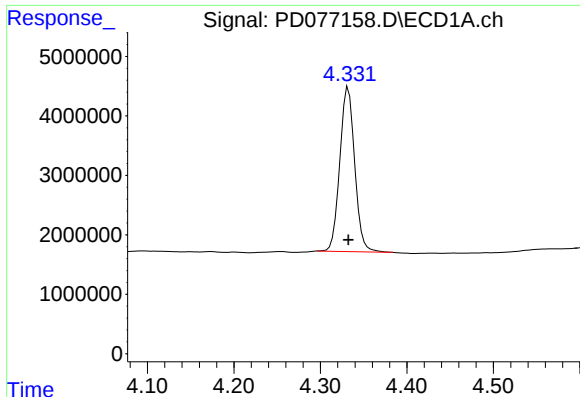

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 32844919
Conc: 9.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

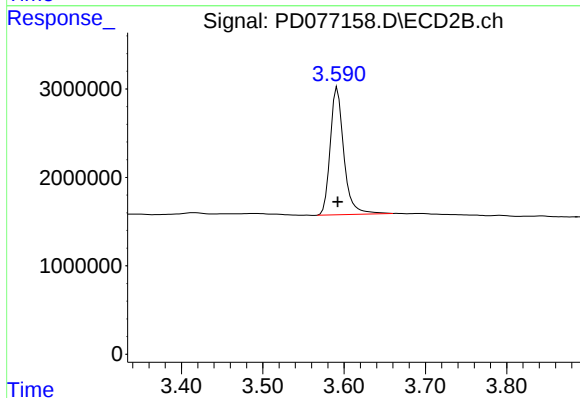


#3 gamma-BHC (Lindane)

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 16855999
Conc: 9.84 ng/ml

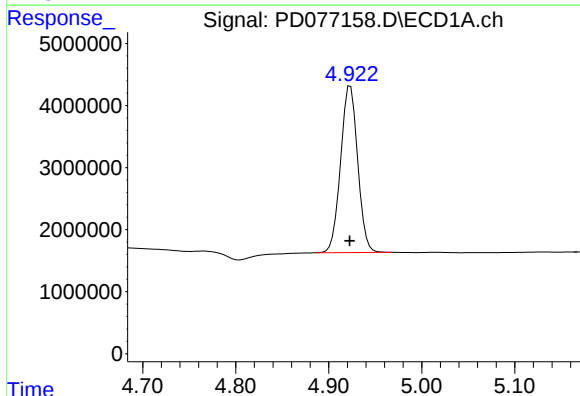


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 34305103
Conc: 9.92 ng/ml

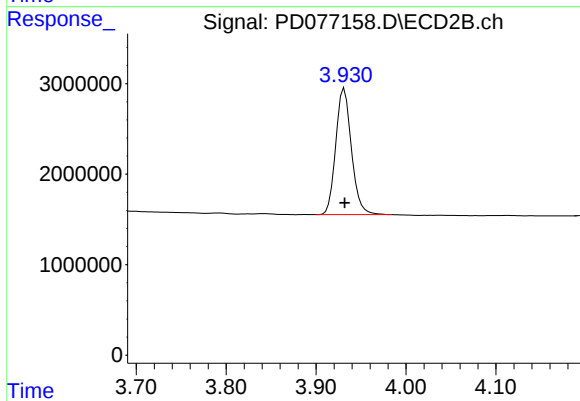

#4 Heptachlor


R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 16892046
Conc: 9.88 ng/ml

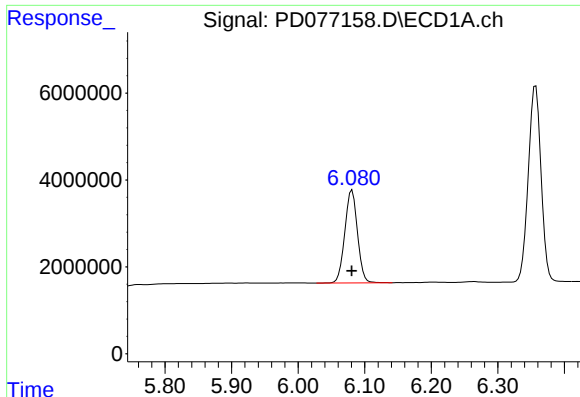

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 28207806
Conc: 10.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

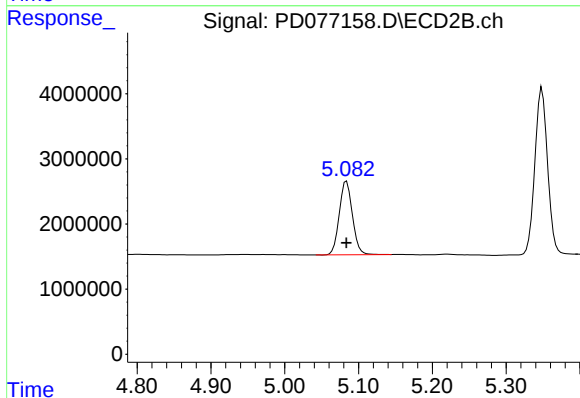


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 13992747
Conc: 9.86 ng/ml

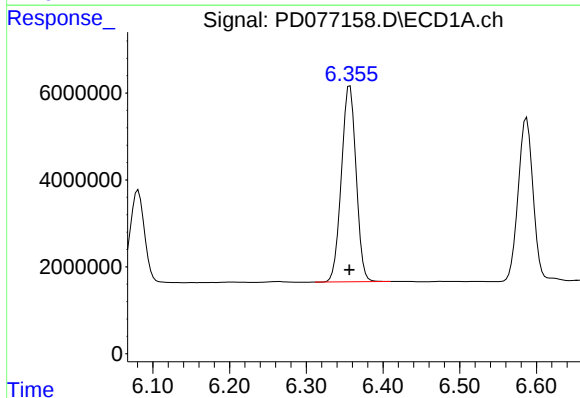


#13 Dieldrin

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 60229874
Conc: 19.43 ng/ml

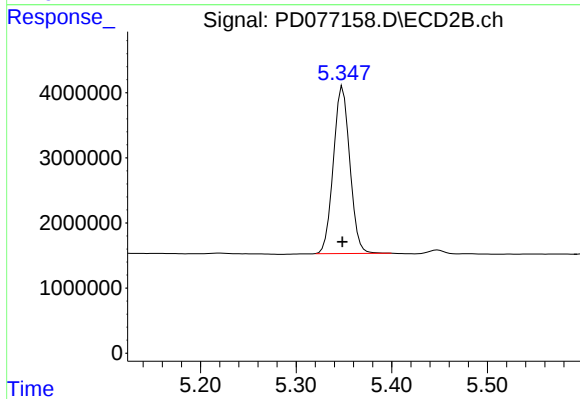

#13 Dieldrin


R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 30647622
Conc: 19.35 ng/ml

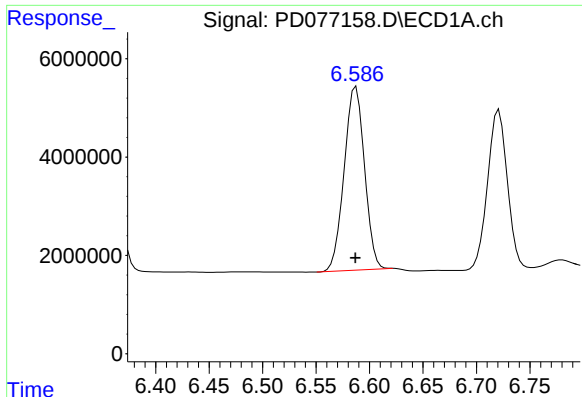

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 49510189
Conc: 19.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

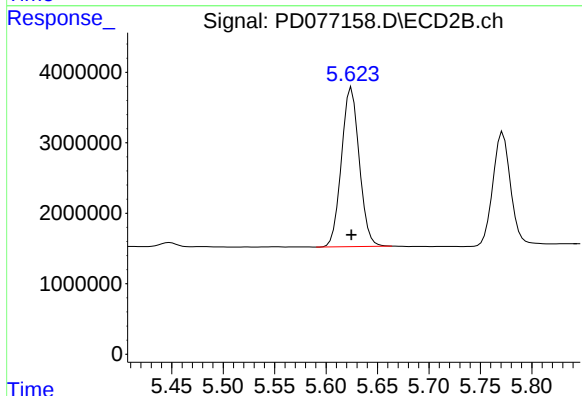


#14 Endrin

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 27179936
Conc: 19.63 ng/ml

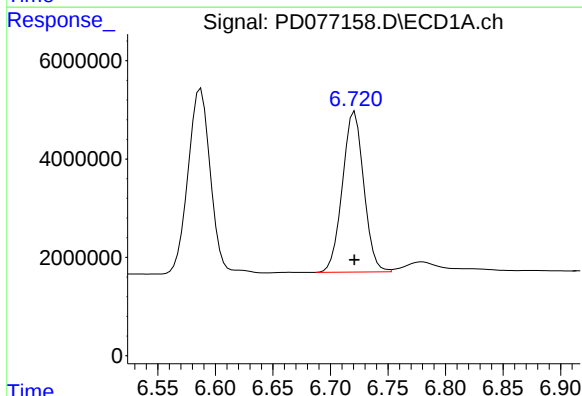


#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: 0.000 min
Response: 42234393
Conc: 19.74 ng/ml

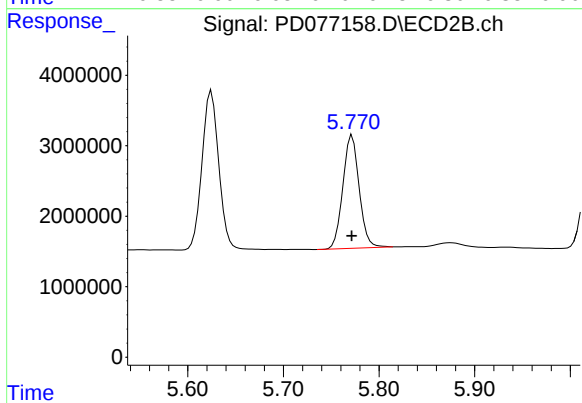

#16 4,4'-DDD


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 19119261
Conc: 19.27 ng/ml

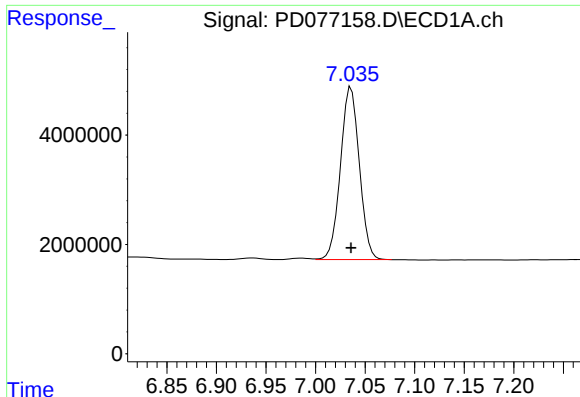

#17 4,4'-DDT


R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 41791958
Conc: 19.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

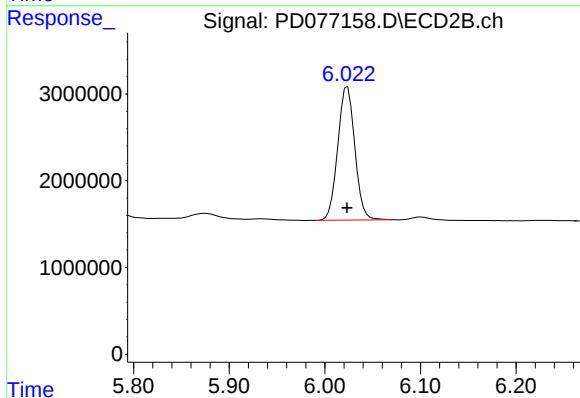


#17 4,4'-DDT

R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 19099639
Conc: 18.51 ng/ml

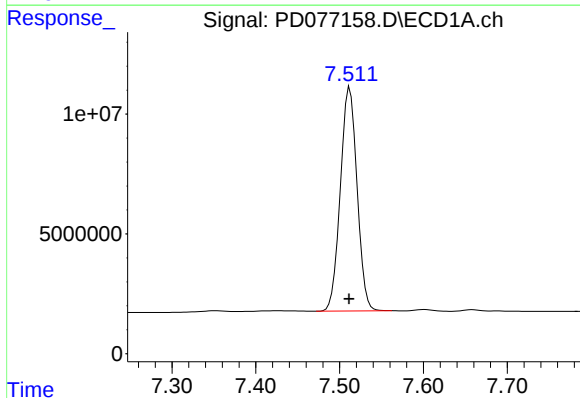


#20 Methoxychlor

R.T.: 7.512 min
Delta R.T.: 0.000 min
Response: 129431004
Conc: 100.81 ng/ml

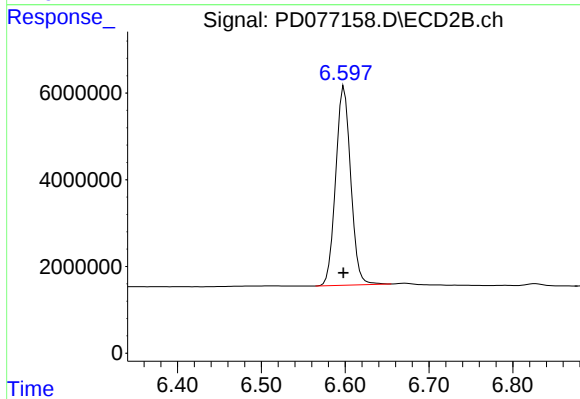

#20 Methoxychlor


R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 57162095
Conc: 99.66 ng/ml

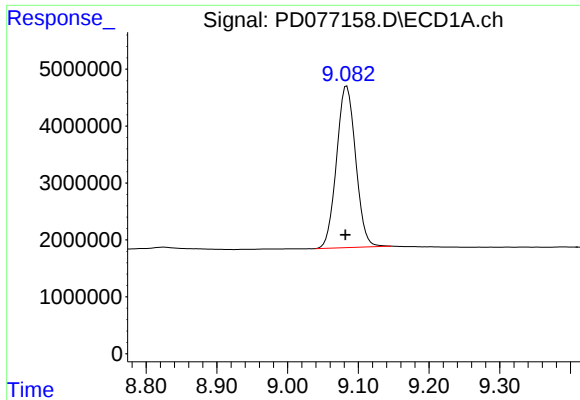

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.002 min
Response: 53348393
Conc: 21.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

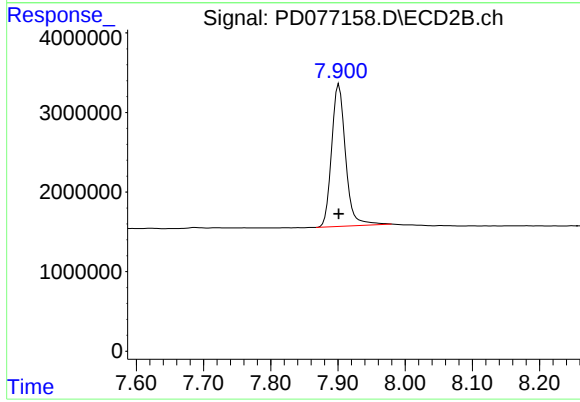

#27 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 25564458
Conc: 20.65 ng/ml