

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 12:22
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:31:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:29:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	43918837	24959499	20.000	20.000
27)	SA Decachlor...	9.082	7.901	100.6E6	49517930	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.998	3.263	71966501	36327438	20.000	20.000
3)	MA gamma-BHC...	4.332	3.592	67794534	34248752	20.000	20.000
4)	MA Heptachlor	4.923	3.932	69158794	34195376	20.000	20.000
9)	A Endosulfan I	6.080	5.084	55988457	28377694	20.000	20.000
13)	MA Dieldrin	6.356	5.349	124.0E6	63341735	40.000	40.000
14)	MA Endrin	6.587	5.625	101.2E6	55395497	40.000	40.000
16)	A 4,4'-DDD	6.721	5.772	85574706	39686329	40.000	40.000
17)	MA 4,4'-DDT	7.036	6.023	87548279	41505778	40.000	40.220
20)	A Methoxychlor	7.512	6.598	256.8E6	114.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 12:22
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:31:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:29:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

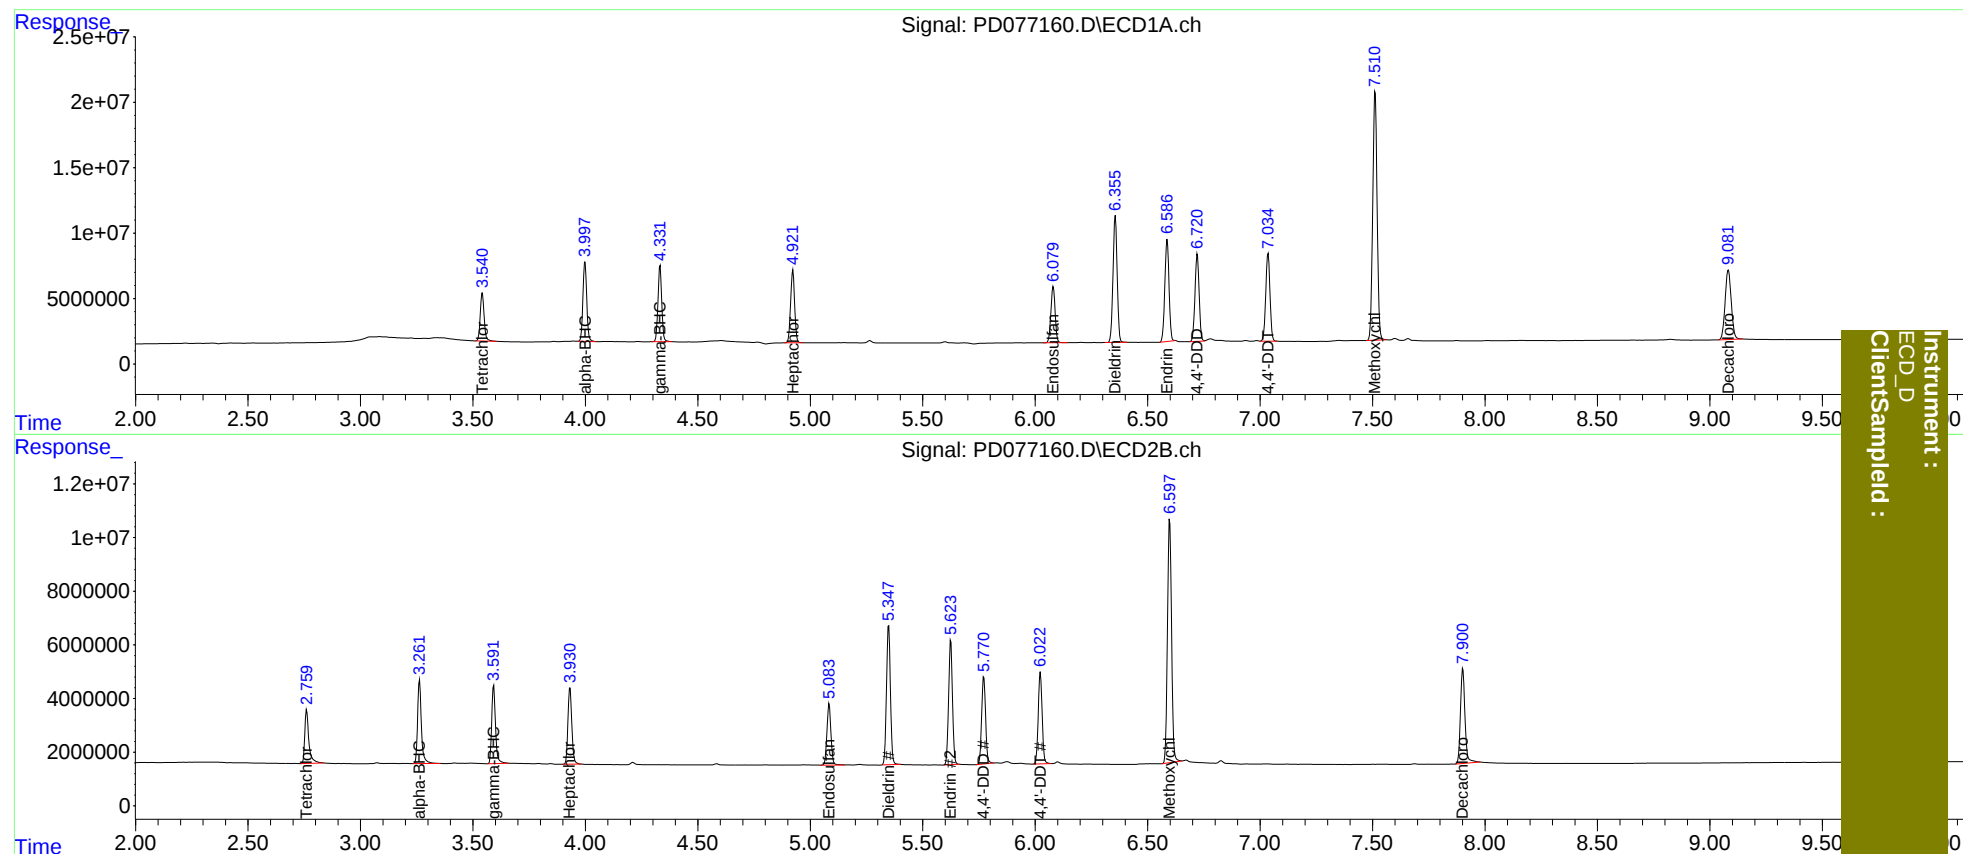


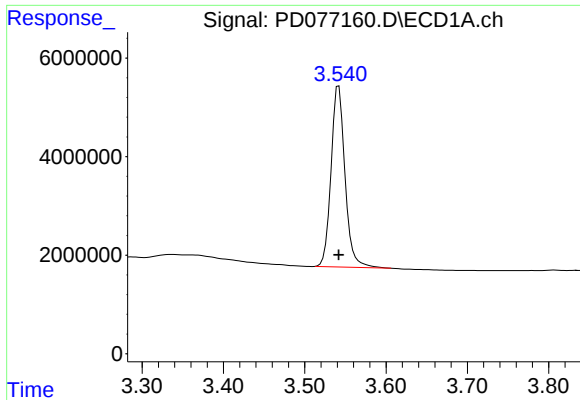

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 43918837
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

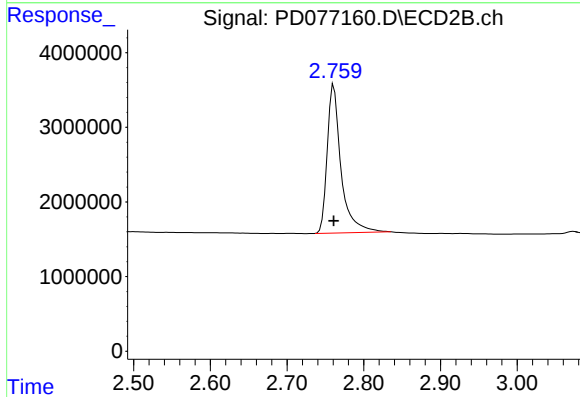


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 24959499
Conc: 20.00 ng/ml

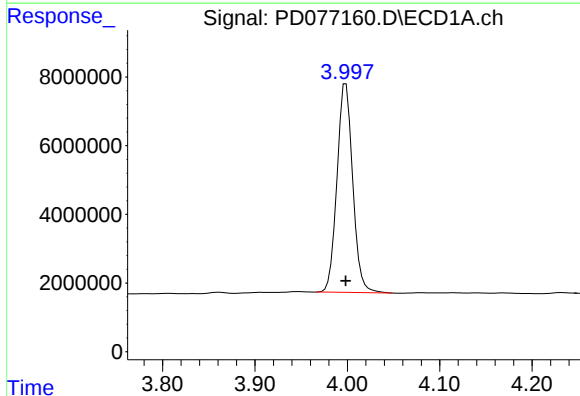


#2 alpha-BHC

R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 71966501
Conc: 20.00 ng/ml

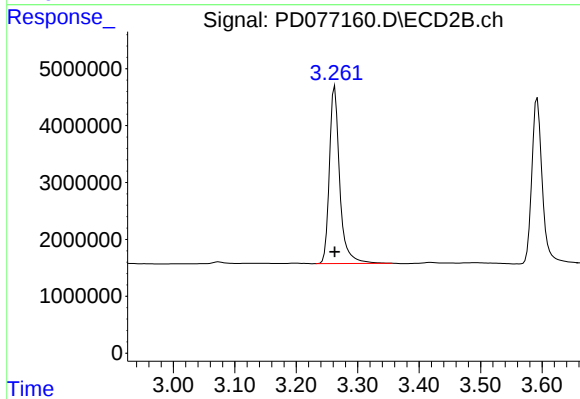

#2 alpha-BHC


R.T.: 3.263 min
Delta R.T.: 0.000 min
Response: 36327438
Conc: 20.00 ng/ml

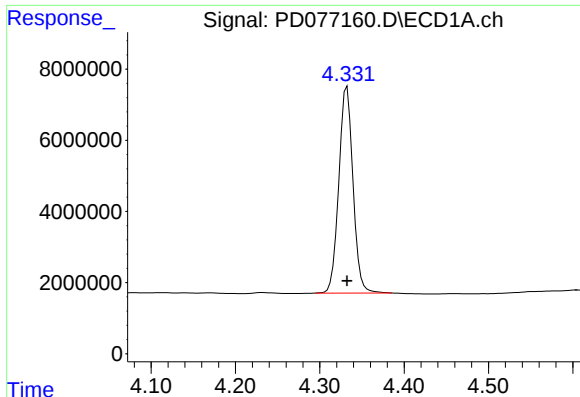

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 67794534
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

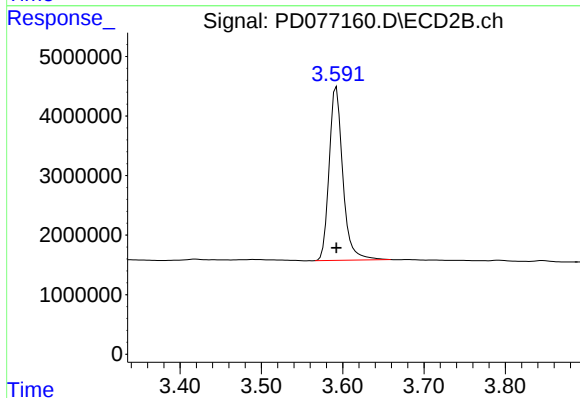


#3 gamma-BHC (Lindane)

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 34248752
Conc: 20.00 ng/ml

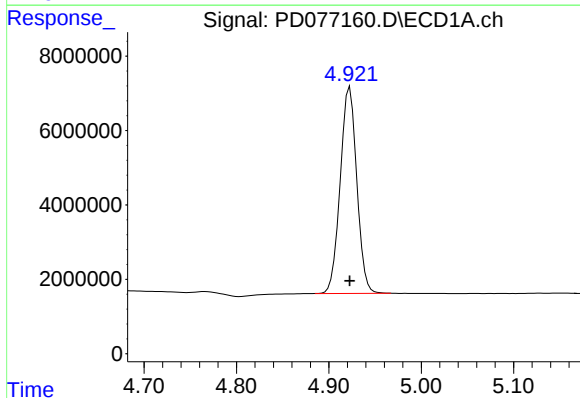


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 69158794
Conc: 20.00 ng/ml

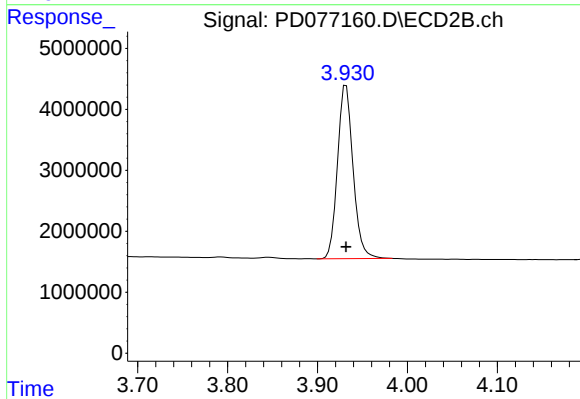

#4 Heptachlor


R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 34195376
Conc: 20.00 ng/ml

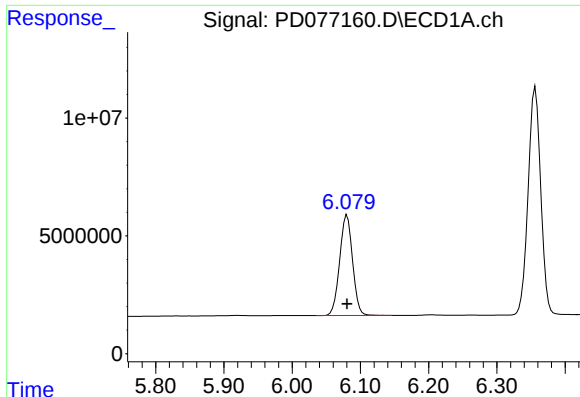

#9 Endosulfan I


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 55988457
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

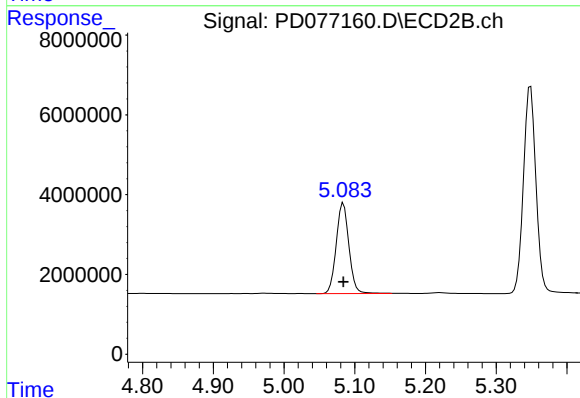


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 28377694
Conc: 20.00 ng/ml

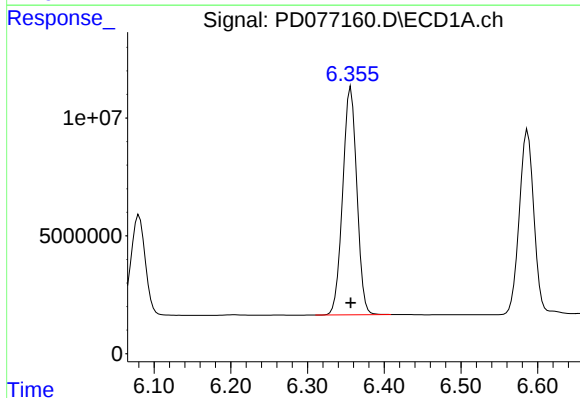


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 123993406
Conc: 40.00 ng/ml

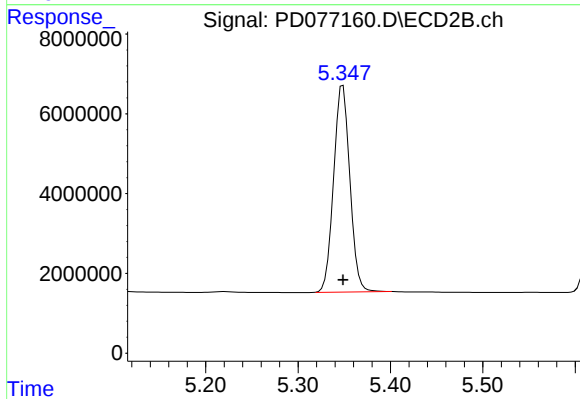

#13 Dieldrin


R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 63341735
Conc: 40.00 ng/ml

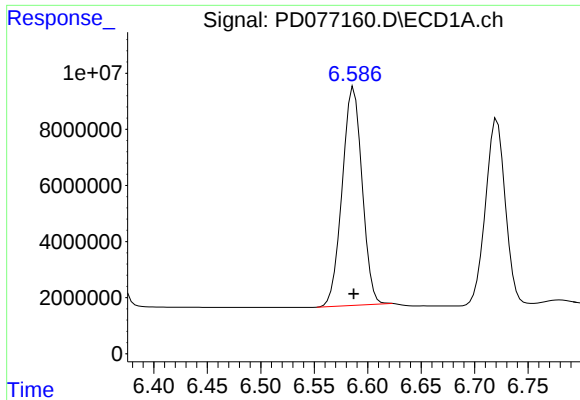

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 101219702
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

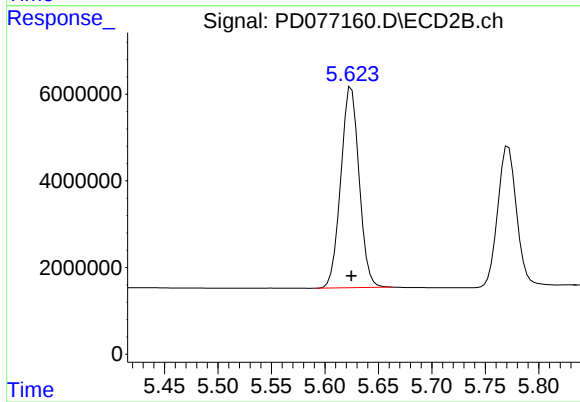


#14 Endrin

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 55395497
Conc: 40.00 ng/ml

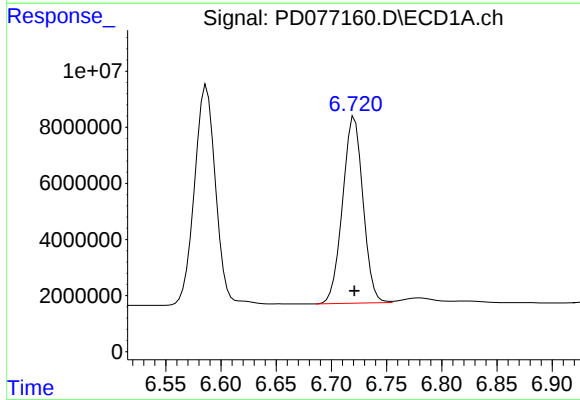


#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: 0.000 min
Response: 85574706
Conc: 40.00 ng/ml

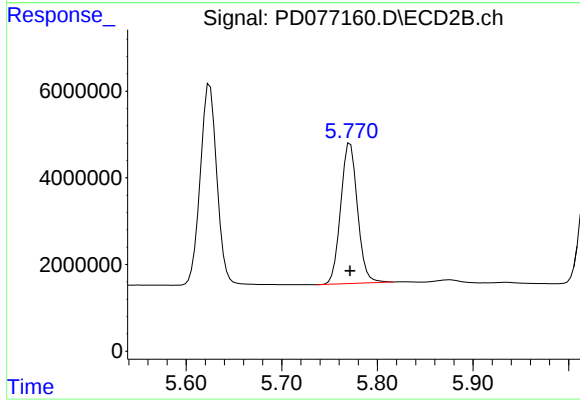

#16 4,4'-DDD


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 39686329
Conc: 40.00 ng/ml

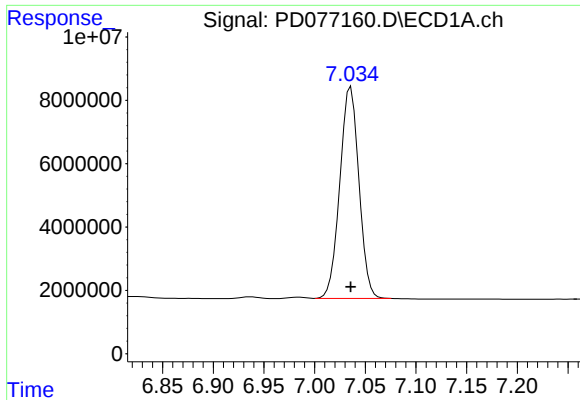

#17 4,4'-DDT


R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 87548279
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

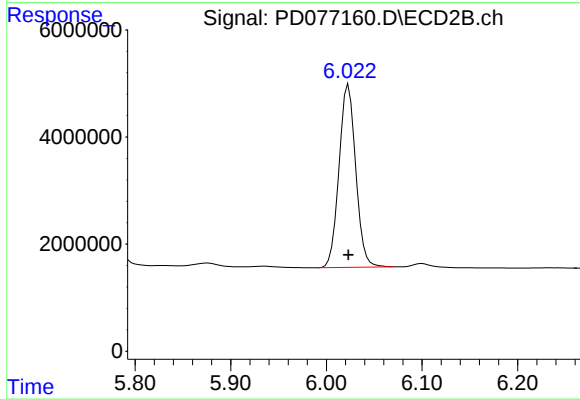


#17 4,4'-DDT

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 41505778
Conc: 40.22 ng/ml

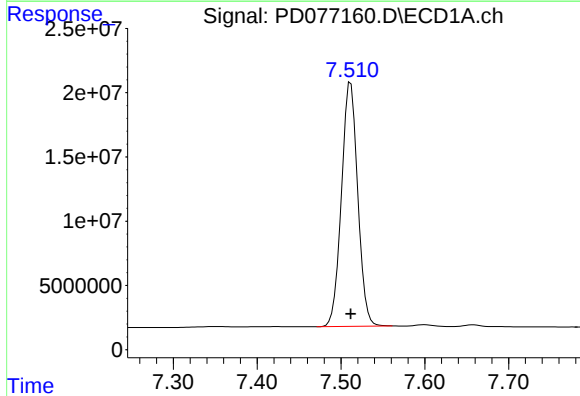


#20 Methoxychlor

R.T.: 7.512 min
Delta R.T.: 0.000 min
Response: 256780987
Conc: 200.00 ng/ml

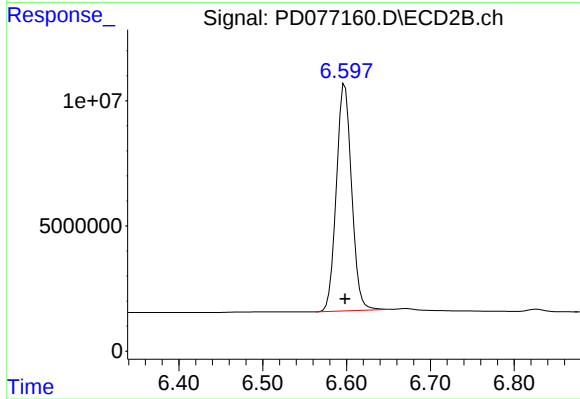

#20 Methoxychlor


R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 114713655
Conc: 200.00 ng/ml

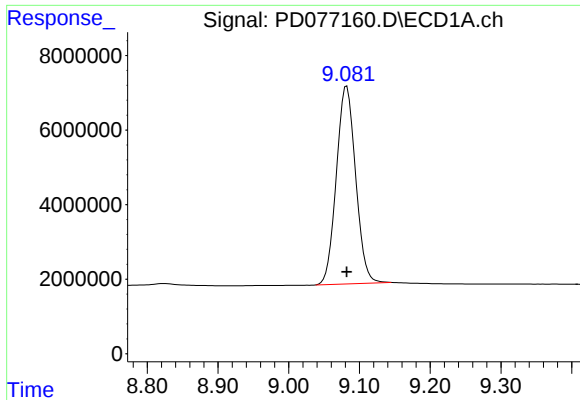

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 100649435
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

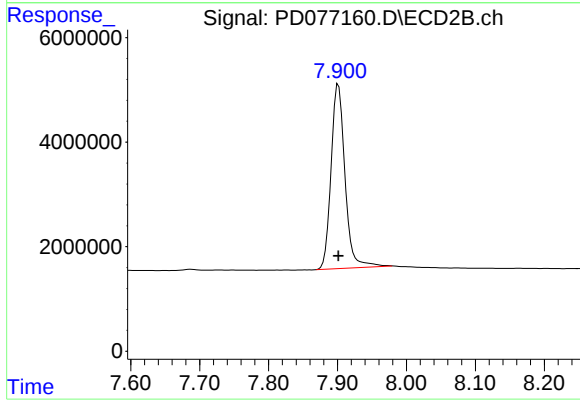

#27 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 49517930
Conc: 40.00 ng/ml