

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 12:49
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:31:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:29:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	86693674	48725182	39.479	39.043
27)	SA Decachlor...	9.083	7.902	193.5E6	97232984	76.888	78.544
Target Compounds							
2)	A alpha-BHC	3.998	3.262	151.8E6	75804615	42.177	41.734
3)	MA gamma-BHC...	4.332	3.592	140.7E6	70119565	41.515	40.947
4)	MA Heptachlor	4.923	3.932	142.2E6	69422299	41.121	40.603
9)	A Endosulfan I	6.081	5.084	112.8E6	56379916	40.276	39.735
13)	MA Dieldrin	6.356	5.348	258.2E6	131.3E6	83.305	82.947
14)	MA Endrin	6.587	5.624	210.2E6	113.9E6	83.052	82.247
16)	A 4,4'-DDD	6.721	5.772	179.8E6	82821069	84.023	83.476
17)	MA 4,4'-DDT	7.035	6.023	187.8E6	90025121	85.814	87.236
20)	A Methoxychlor	7.512	6.598	518.8E6	229.2E6	404.088	399.634


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 12:49
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:31:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:29:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

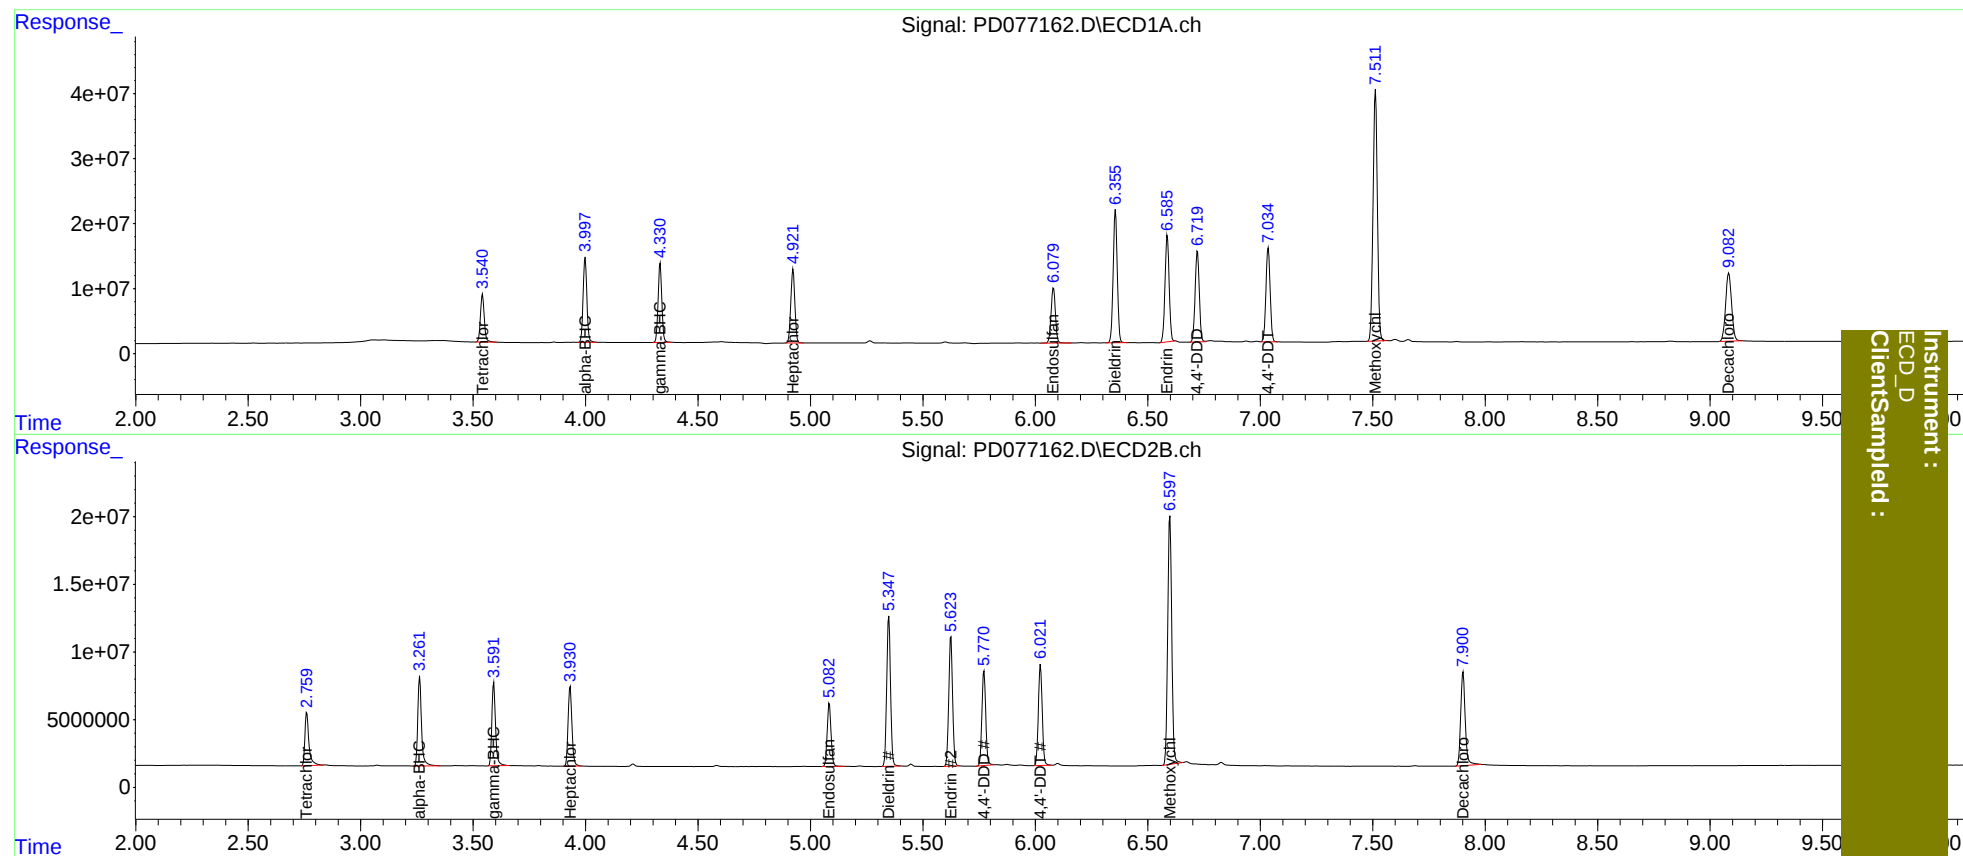


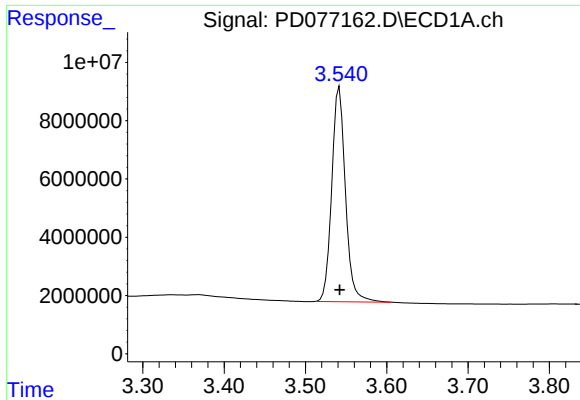

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 86693674
Conc: 39.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

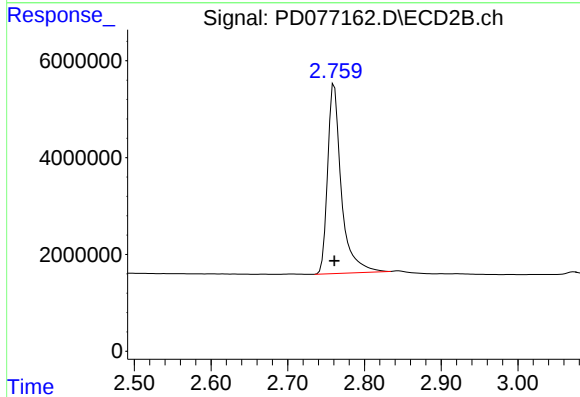


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 48725182
Conc: 39.04 ng/ml

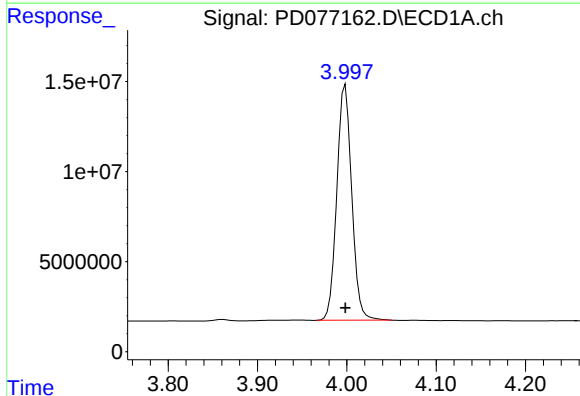


#2 alpha-BHC

R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 151766615
Conc: 42.18 ng/ml

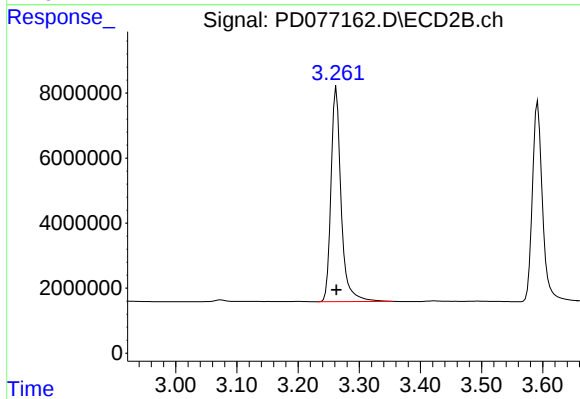

#2 alpha-BHC


R.T.: 3.262 min
Delta R.T.: 0.000 min
Response: 75804615
Conc: 41.73 ng/ml

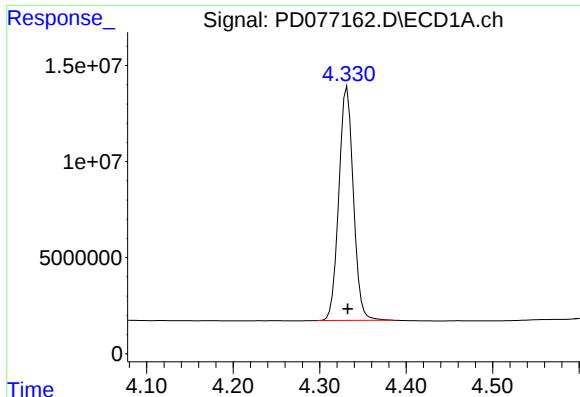

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 140723760
Conc: 41.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

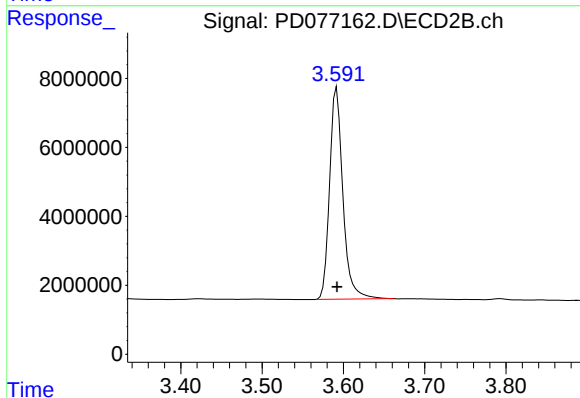


#3 gamma-BHC (Lindane)

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 70119565
Conc: 40.95 ng/ml

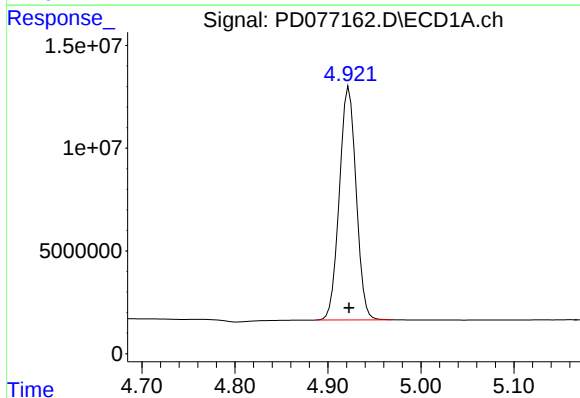


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 142193639
Conc: 41.12 ng/ml

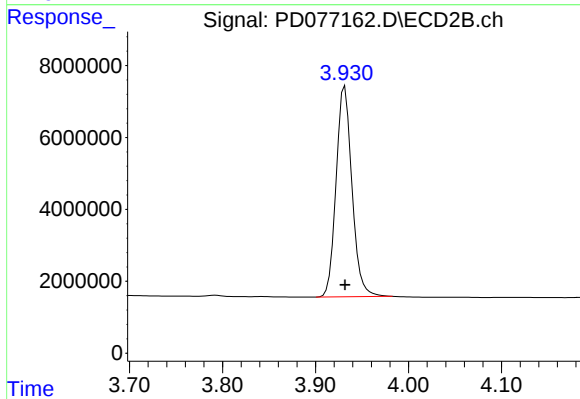

#4 Heptachlor


R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 69422299
Conc: 40.60 ng/ml

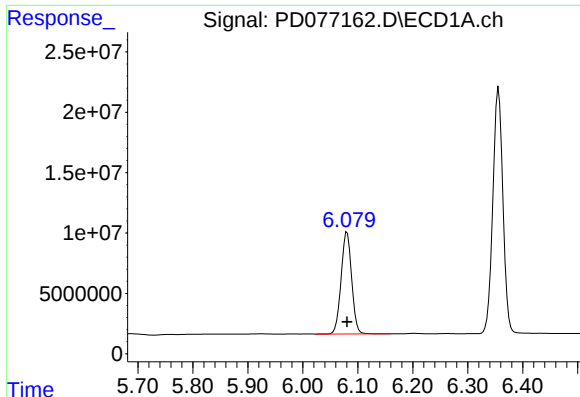

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 112750106
Conc: 40.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

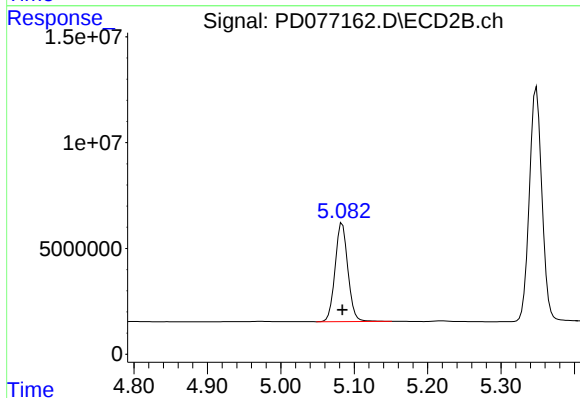


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 56379916
Conc: 39.74 ng/ml

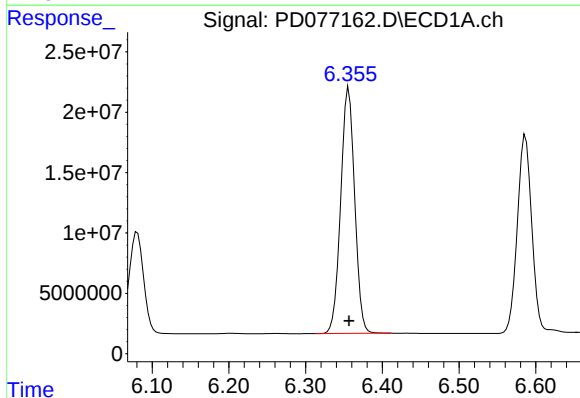


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 258231009
Conc: 83.30 ng/ml

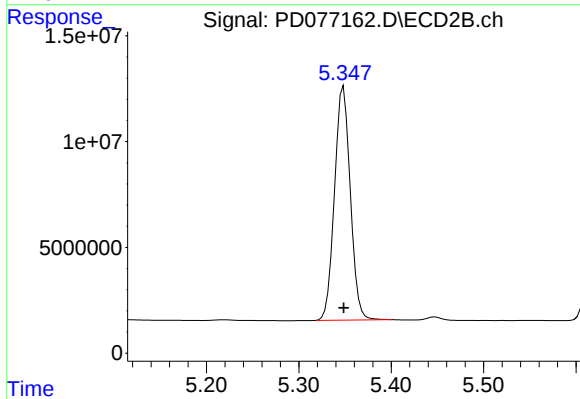

#13 Dieldrin


R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 131349457
Conc: 82.95 ng/ml

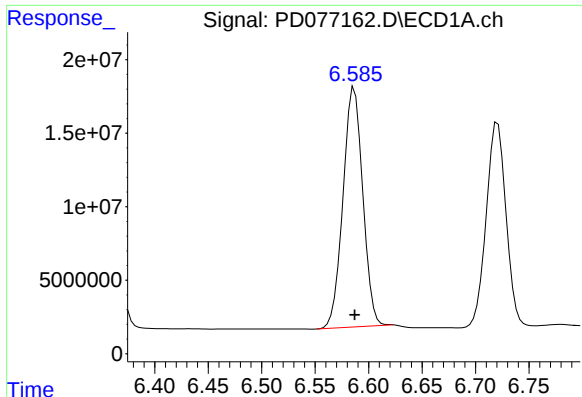

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 210162192
Conc: 83.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

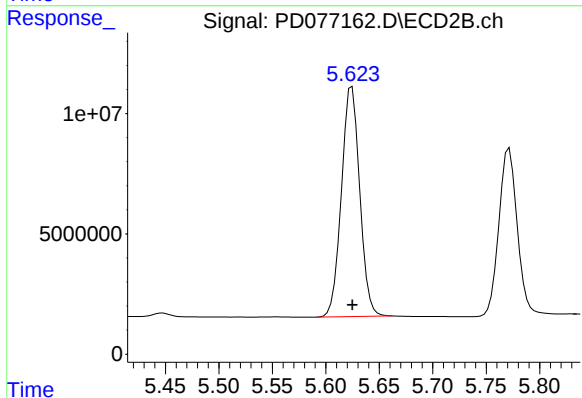


#14 Endrin

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 113902175
Conc: 82.25 ng/ml

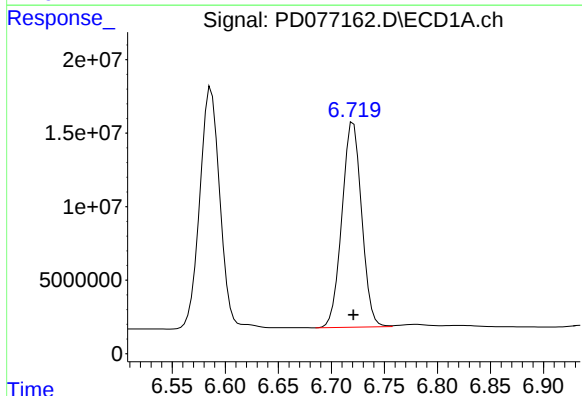


#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: 0.000 min
Response: 179756325
Conc: 84.02 ng/ml

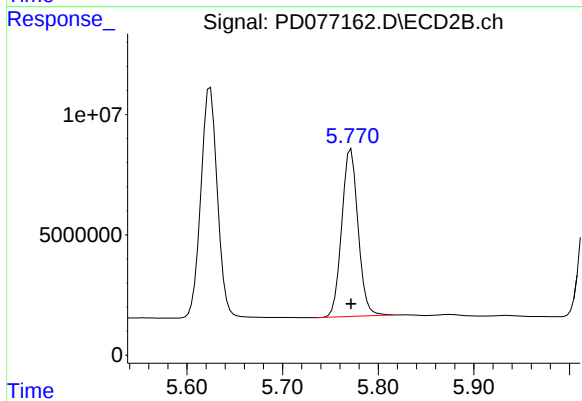

#16 4,4'-DDD


R.T.: 5.772 min
Delta R.T.: 0.000 min
Response: 82821069
Conc: 83.48 ng/ml

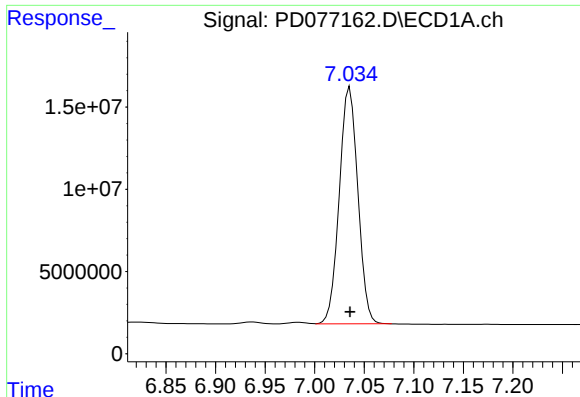

#17 4,4'-DDT


R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 187820640
Conc: 85.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

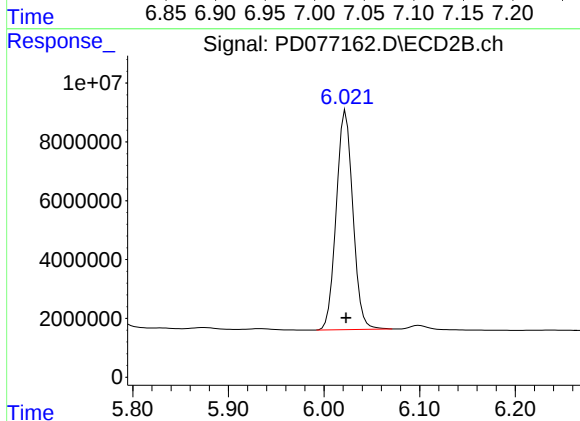


#17 4,4'-DDT

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 90025121
Conc: 87.24 ng/ml

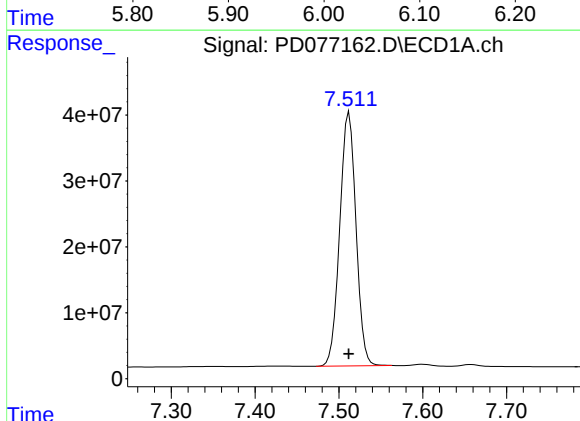


#20 Methoxychlor

R.T.: 7.512 min
Delta R.T.: 0.000 min
Response: 518811073
Conc: 404.09 ng/ml

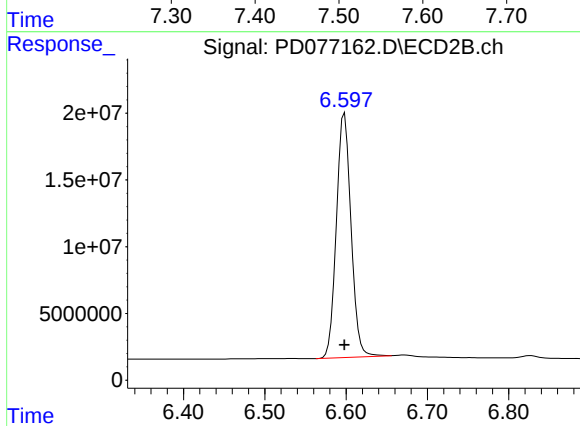

#20 Methoxychlor

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 229217604
Conc: 399.63 ng/ml

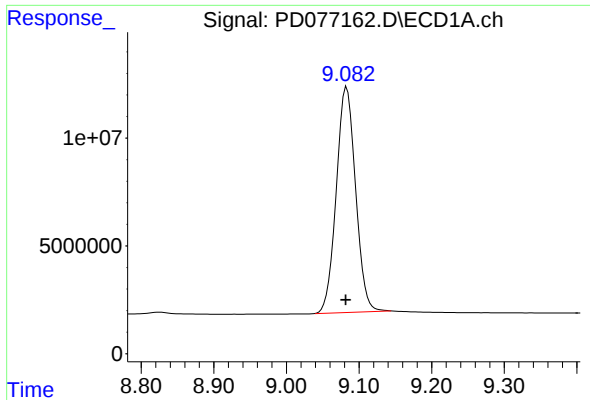

#27 Decachlorobiphenyl


R.T.: 9.083 min

Delta R.T.: 0.001 min

Response: 193469174

Conc: 76.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

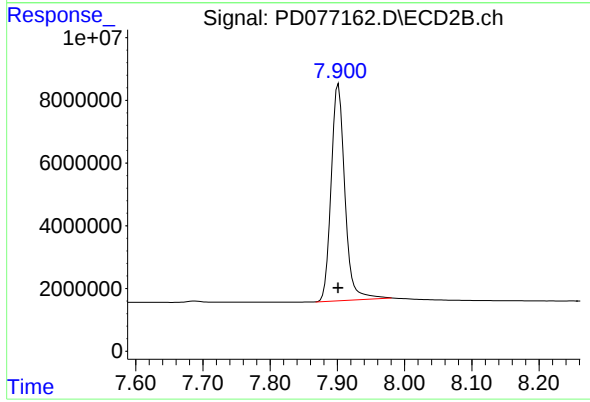

#27 Decachlorobiphenyl

R.T.: 7.902 min

Delta R.T.: 0.000 min

Response: 97232984

Conc: 78.54 ng/ml