

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 17:27
 Operator : AR\AJ
 Sample : PB154780BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:58:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	42729328	24047245	19.463	19.303
2)	SA Decachlor...	9.086	7.903	91893661	45832048	36.113	36.768
Target Compounds							
6)	B beta-BHC	0.000	3.851f	0	869624	N.D.	1.065
15)	B Endosulfa...	6.781	5.876f	1676316	134574	0.593	0.101 #
16)	A 4,4'-DDD	6.781f	0.000	1676316	0	0.771	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 17:27
Operator : AR\AJ
Sample : PB154780BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:58:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

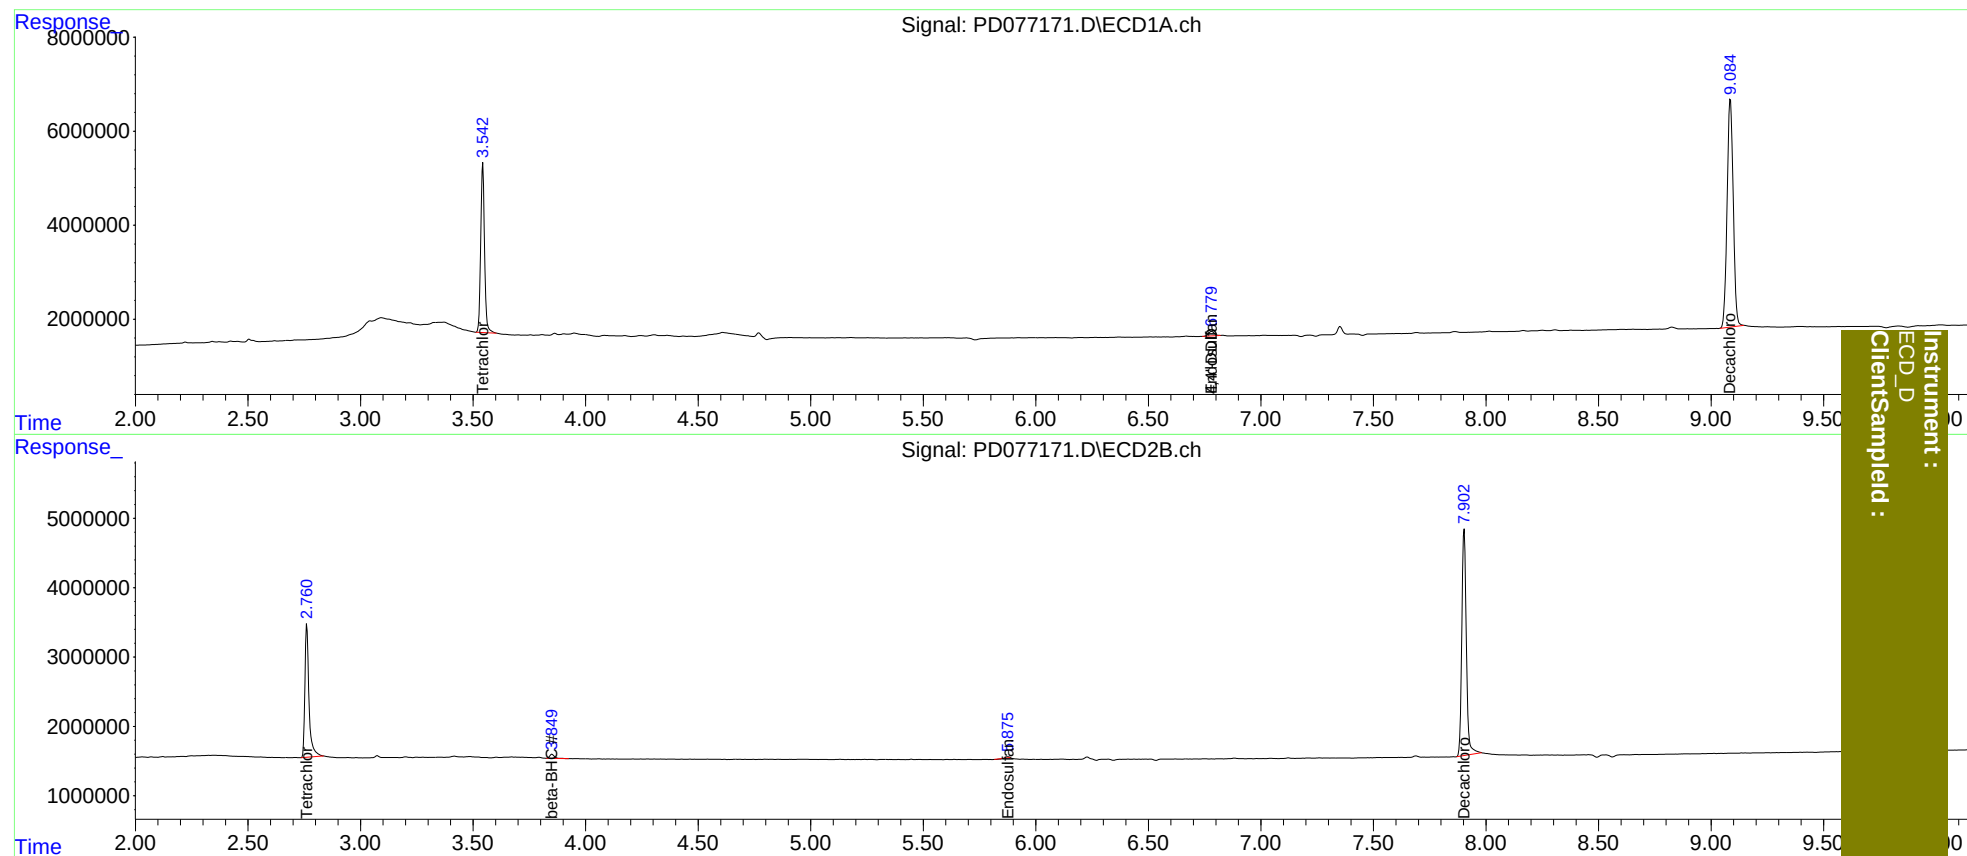


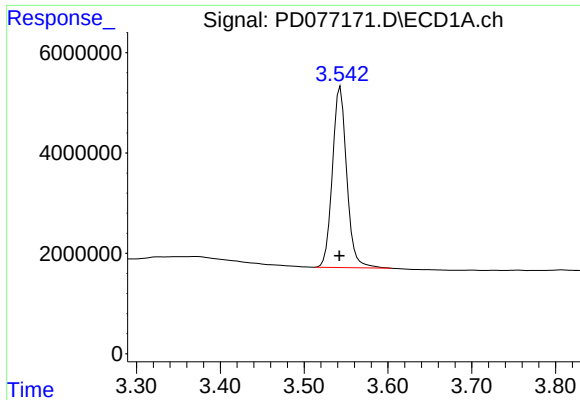

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.001 min
Response: 42729328
Conc: 19.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

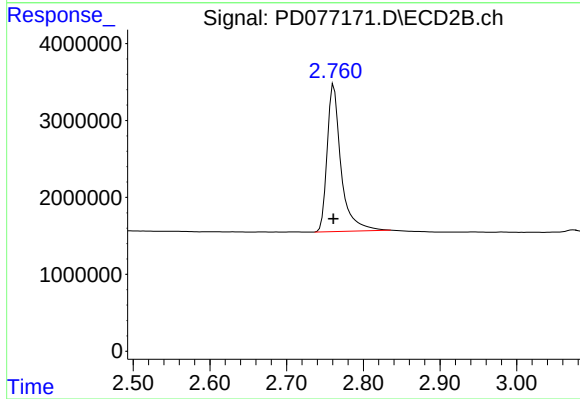


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 24047245
Conc: 19.30 ng/ml

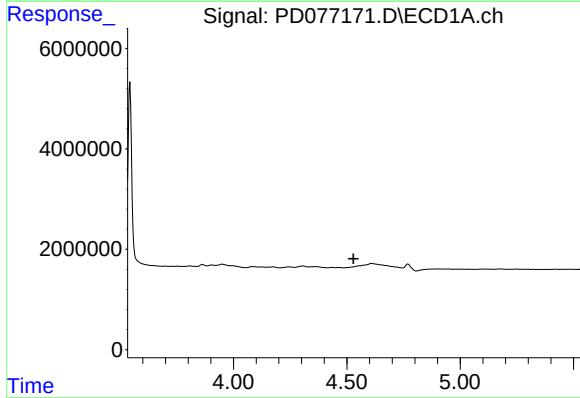


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

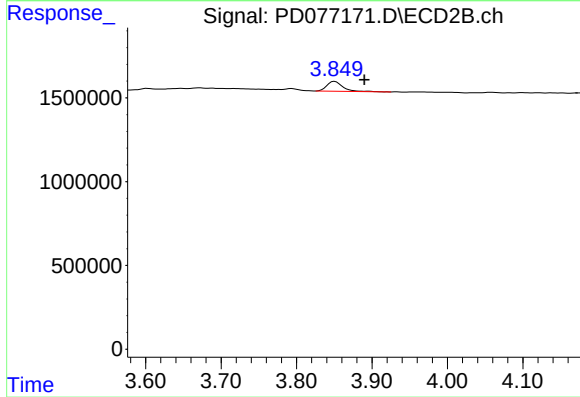

#6 beta-BHC


R.T.: 3.851 min
Delta R.T.: -0.039 min
Response: 869624
Conc: 1.07 ng/ml

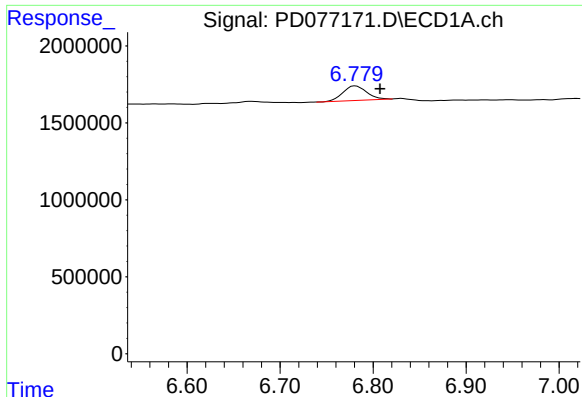

#15 Endosulfan II


R.T.: 6.781 min
Delta R.T.: -0.026 min
Response: 1676316
Conc: 0.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

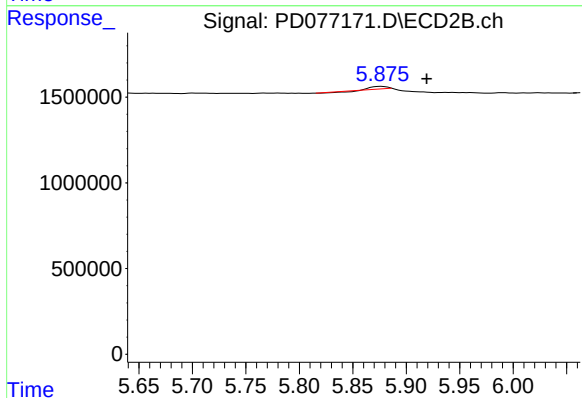


#15 Endosulfan II

R.T.: 5.876 min
Delta R.T.: -0.043 min
Response: 134574
Conc: 0.10 ng/ml

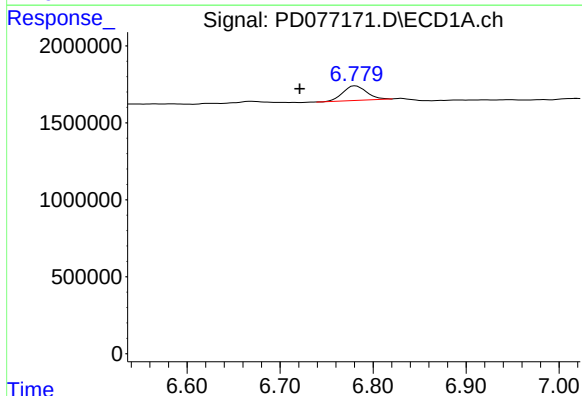


#16 4,4'-DDD

R.T.: 6.781 min
Delta R.T.: 0.060 min
Response: 1676316
Conc: 0.77 ng/ml

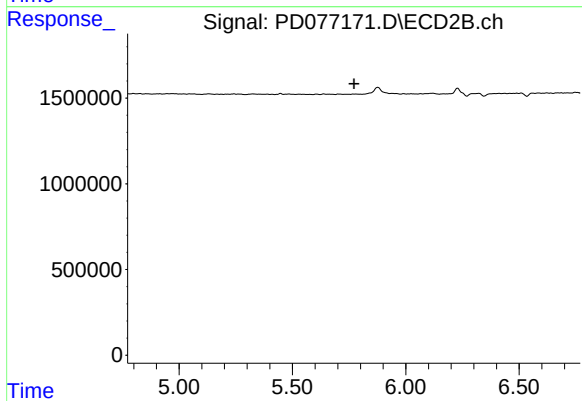

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.772 min
Response: 0
Conc: N.D.

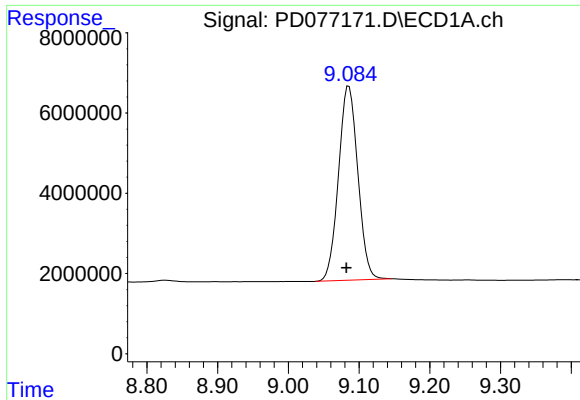

#27 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.004 min
Response: 91893661
Conc: 36.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

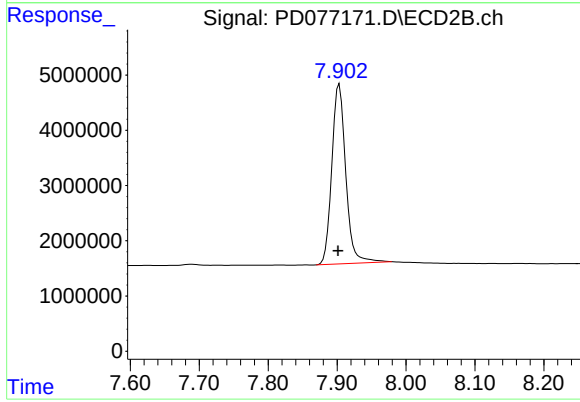

#27 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: 0.002 min
Response: 45832048
Conc: 36.77 ng/ml