

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
 Data File : PD077172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 17:40
 Operator : AR\AJ
 Sample : 03573-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2023-05

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/15/2023
 Supervised By :Ankita Jodhani 08/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 01:58:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	41861104	23808264	19.068	19.112
27)	SA Decachlor...	9.084	7.902	94817849	46554006	37.262	37.347
Target Compounds							
2)	A alpha-BHC	3.999	3.263	3205245	1817366	0.887	0.989
3)	MA gamma-BHC...	4.332	3.593	3368668	1614202	0.987	0.936
4)	MA Heptachlor	4.923	3.932	3513779	1741686	1.004	1.011
5)	MB Aldrin	5.266	4.212	3532817	1684701	1.020	0.973
6)	B beta-BHC	4.530	3.890	1304687	903706	0.841	1.107 #
7)	B delta-BHC	4.775	4.119	5605913	1551708	1.691	0.893 #
8)	B Heptachlo...	5.693	4.714	3700572	1693211	1.160	1.035
9)	A Endosulfan I	6.081	5.085	3071412	1490457	1.087	1.058
10)	B trans-Chl...	5.951	4.965	3082541	1629167	0.998	1.055
11)	B cis-Chlor...	6.030	5.029	3277993	1627865	1.024	1.011
12)	B 4,4'-DDE	6.203	5.217	2747347	1281300	0.959	0.941
13)	MA Dieldrin	6.357	5.349	3378239	1572914	1.084	0.992
14)	MA Endrin	6.587	5.625	2580603	1440567	1.015	1.038
15)	B Endosulfa...	6.805	5.920	3942585	1161245	1.395m	0.868 #
16)	A 4,4'-DDD	6.721	5.772	2148514	1043356	0.989	1.049
17)	MA 4,4'-DDT	7.036	6.024	2012376	692241	0.912	0.669 #
18)	B Endrin al...	6.938	6.100	2509223	1238946	1.166	1.141
19)	B Endosulfa...	7.172	6.322	2770965	1392042	1.113	1.112
20)	A Methoxychlor	7.513	6.600	1423450	578204	1.106	1.025
21)	B Endrin ke...	7.659	6.829	3228663	1525201	1.147	1.036

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081423\
Data File : PD077172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 17:40
Operator : AR\AJ
Sample : 03573-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 01:58:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

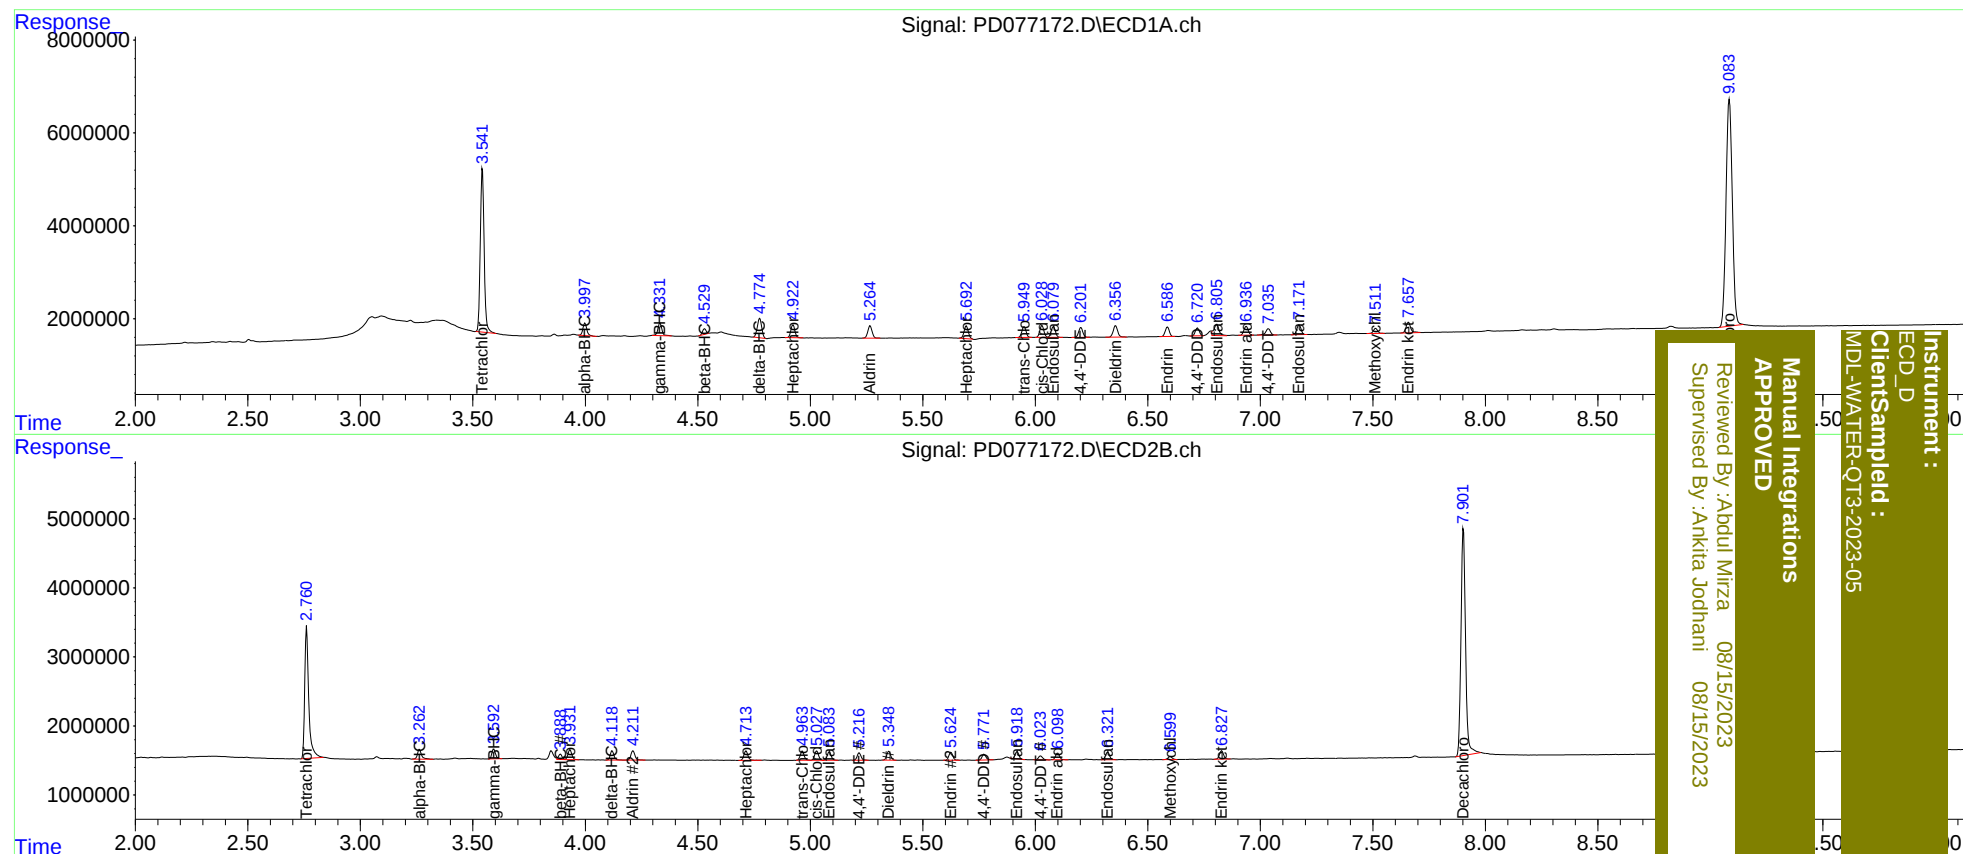

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/15/2023
Supervised By: Ankita Jodhani 08/15/2023

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT3-2023-05