

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
 Data File : PD084425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 21:38
 Operator : AR\AJ
 Sample : P3481-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 02:10:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.928	11003394	65719852	13.125	12.484
27)	SA Decachlor...	9.111	8.136	36435434	84759432	20.948	22.555
Target Compounds							
6)	B beta-BHC	0.000	4.032f	0	147.0E6	N.D.	40.862
7)	B delta-BHC	4.812	0.000	1225840	0	0.710	N.D. #
9)	A Endosulfan I	6.096	5.319	3877303	8993634	2.434	1.516 #
10)	B trans-Chl...	6.036f	0.000	1480520	0	0.897	N.D. #
11)	B cis-Chlor...	6.036	5.319f	1480520	8993634	0.860	1.429 #
12)	B 4,4'-DDE	6.256	5.445	5019074	13272221	2.869	2.176
15)	B Endosulfa...	6.851	0.000	2098152	0	1.273	N.D. #
19)	B Endosulfa...	7.166	6.591f	2965002	6610770	1.953	1.416 #
20)	A Methoxychlor	7.473f	0.000	1260582	0	1.581	N.D. #
25)	Toxaphene-4	7.166	0.000	2965002	0	88.375	N.D. #
26)	Toxaphene-5	7.955	7.436f	8795256	19515473	354.514	355.870


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
Data File : PD084425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 21:38
Operator : AR\AJ
Sample : P3481-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 02:10:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

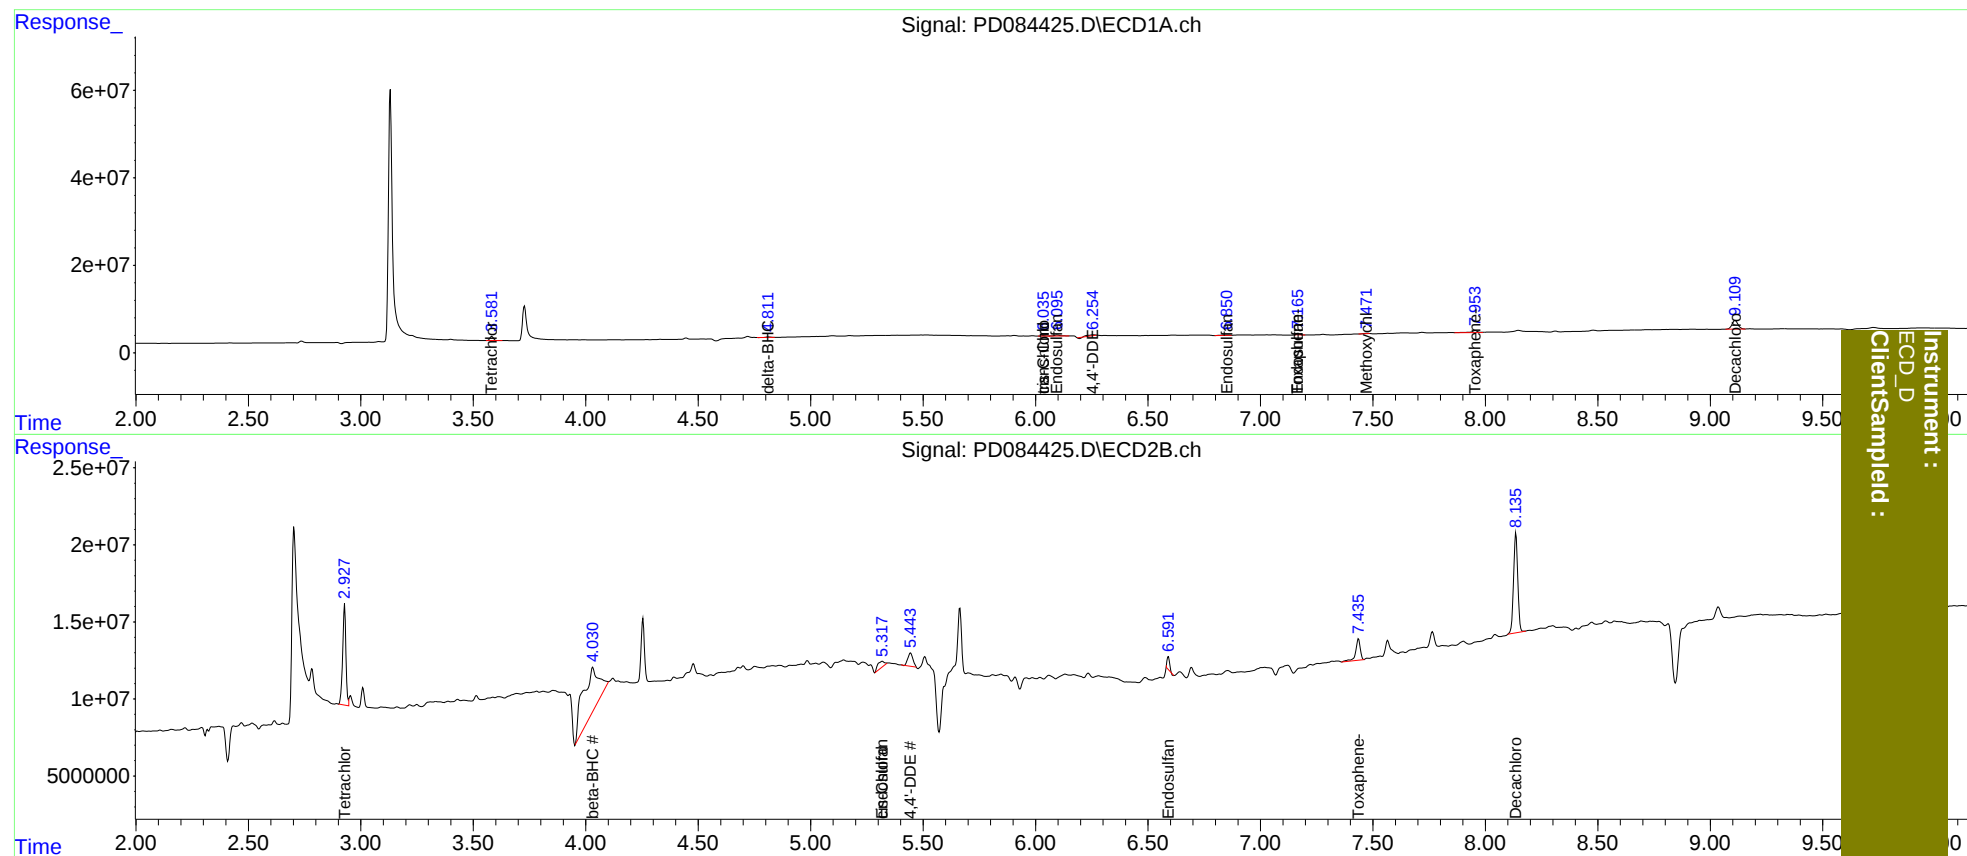


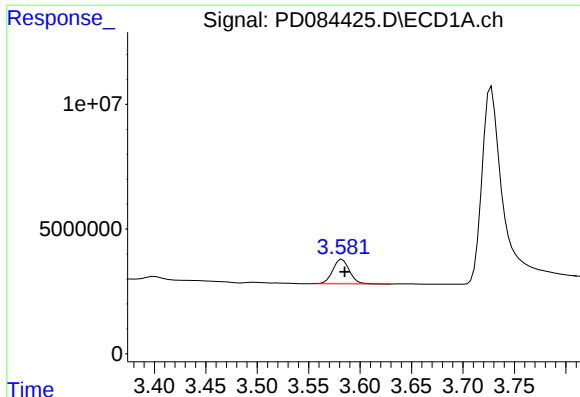

#1 Tetrachloro-m-xylene


R.T.: 3.583 min
Delta R.T.: -0.002 min
Response: 11003394
Conc: 13.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

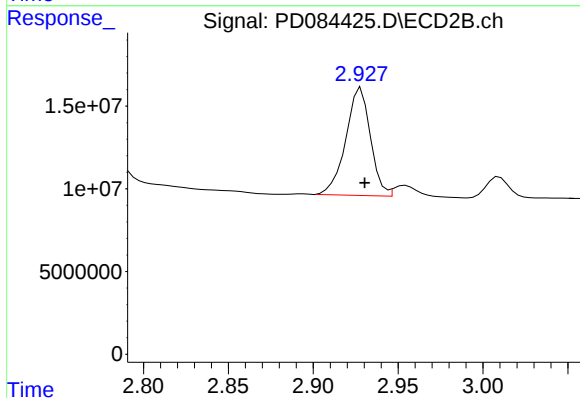


#1 Tetrachloro-m-xylene

R.T.: 2.928 min
Delta R.T.: -0.002 min
Response: 65719852
Conc: 12.48 ng/ml

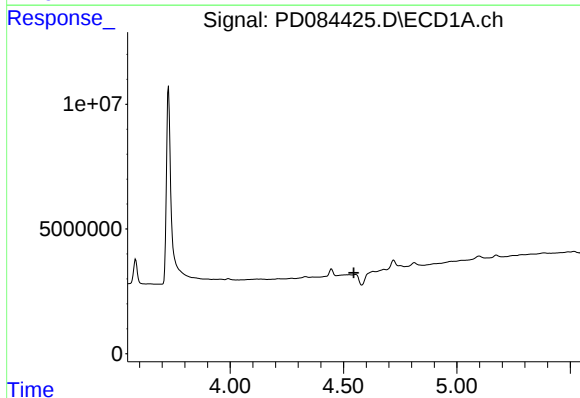


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.546 min
Response: 0
Conc: N.D.

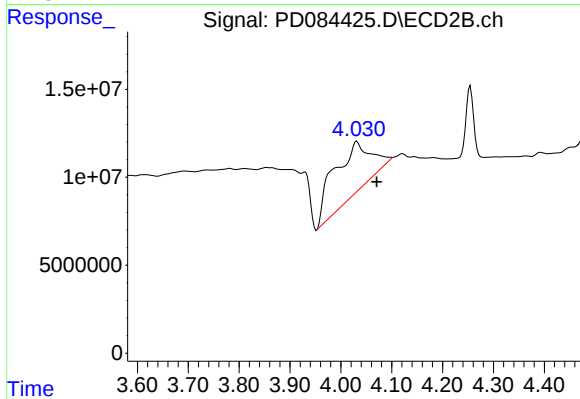

#6 beta-BHC


R.T.: 4.032 min
Delta R.T.: -0.039 min
Response: 146956567
Conc: 40.86 ng/ml

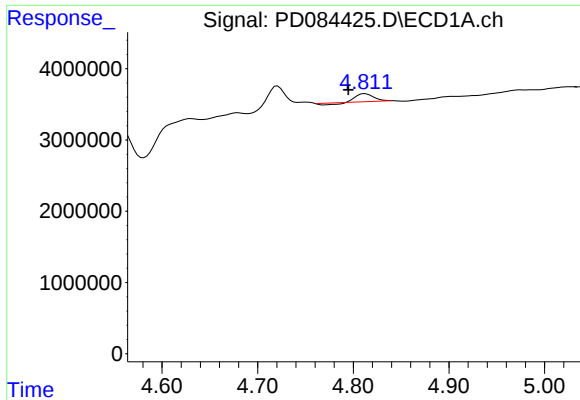

#7 delta-BHC


R.T.: 4.812 min
Delta R.T.: 0.017 min
Response: 1225840
Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

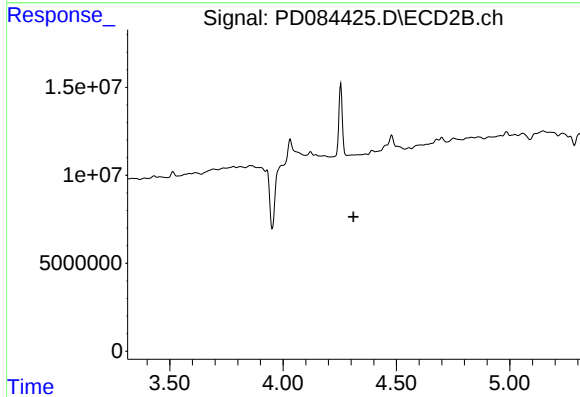


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.311 min
Response: 0
Conc: N.D.

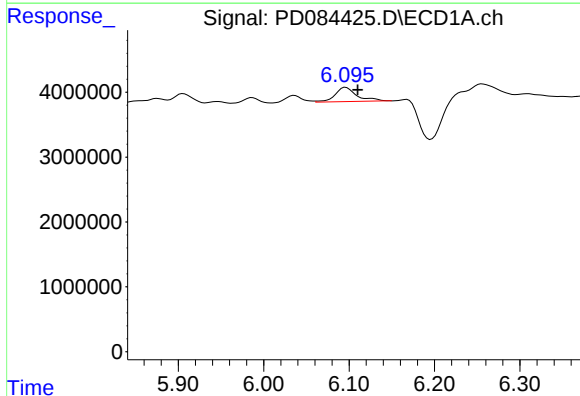


#9 Endosulfan I

R.T.: 6.096 min
Delta R.T.: -0.014 min
Response: 3877303
Conc: 2.43 ng/ml

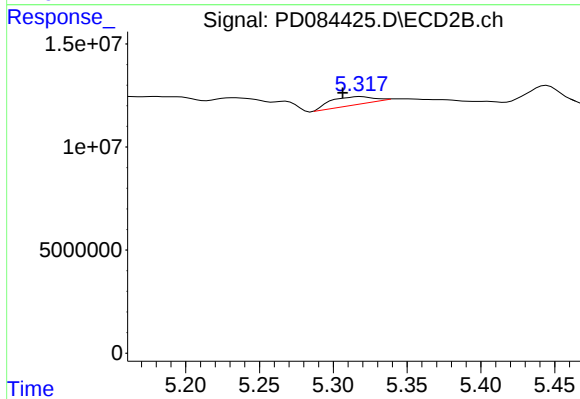

#9 Endosulfan I


R.T.: 5.319 min
Delta R.T.: 0.012 min
Response: 8993634
Conc: 1.52 ng/ml

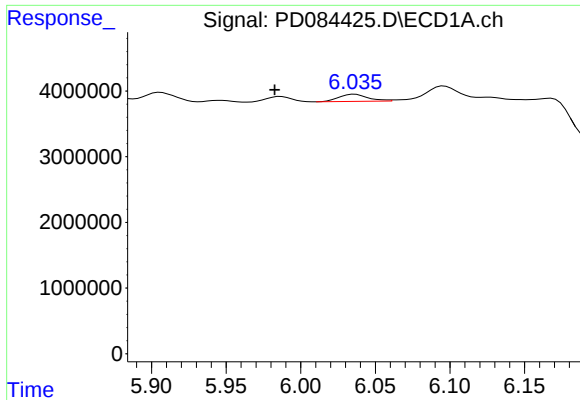

#10 trans-Chlordane


R.T.: 6.036 min
Delta R.T.: 0.054 min
Response: 1480520
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

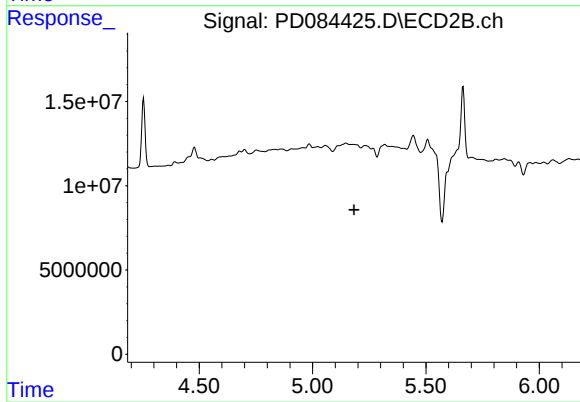


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

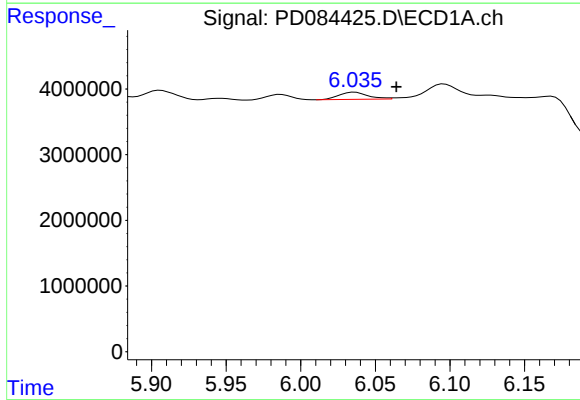


#11 cis-Chlordane

R.T.: 6.036 min
Delta R.T.: -0.028 min
Response: 1480520
Conc: 0.86 ng/ml

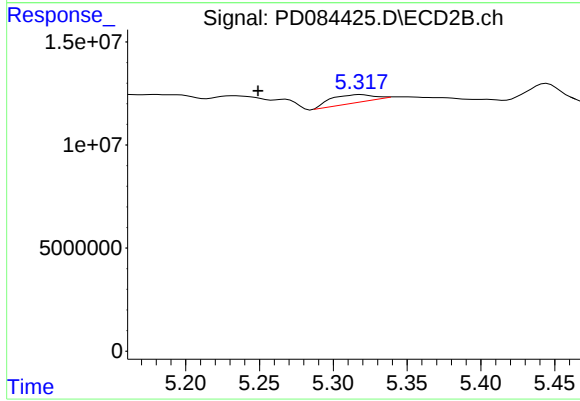

#11 cis-Chlordane


R.T.: 5.319 min
Delta R.T.: 0.070 min
Response: 8993634
Conc: 1.43 ng/ml

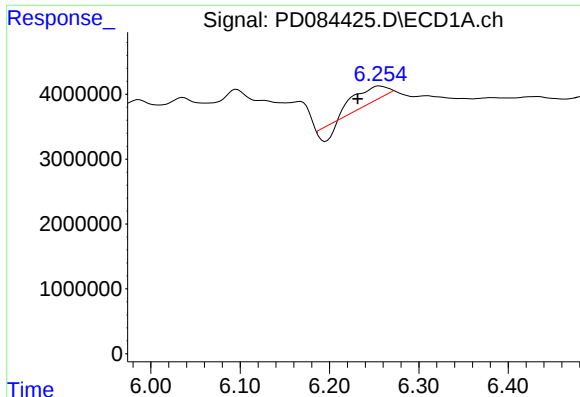

#12 4,4'-DDE


R.T.: 6.256 min
Delta R.T.: 0.025 min
Response: 5019074
Conc: 2.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

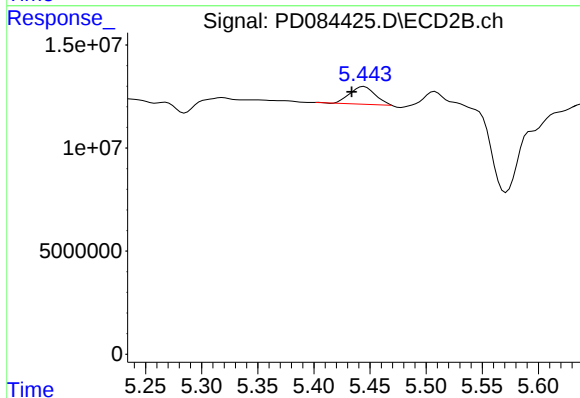


#12 4,4'-DDE

R.T.: 5.445 min
Delta R.T.: 0.011 min
Response: 13272221
Conc: 2.18 ng/ml

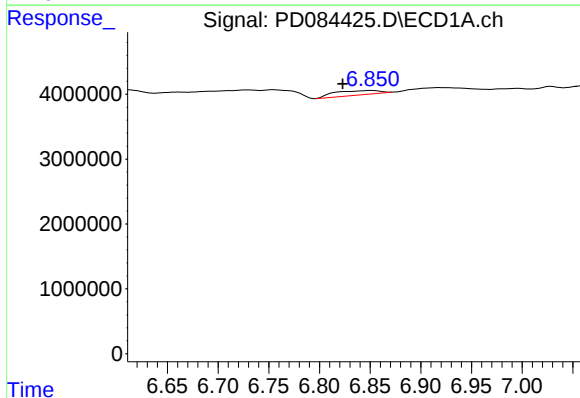


#15 Endosulfan II

R.T.: 6.851 min
Delta R.T.: 0.028 min
Response: 2098152
Conc: 1.27 ng/ml

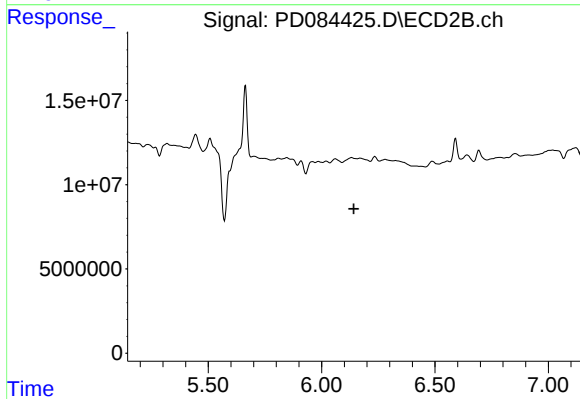

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.142 min
Response: 0
Conc: N.D.

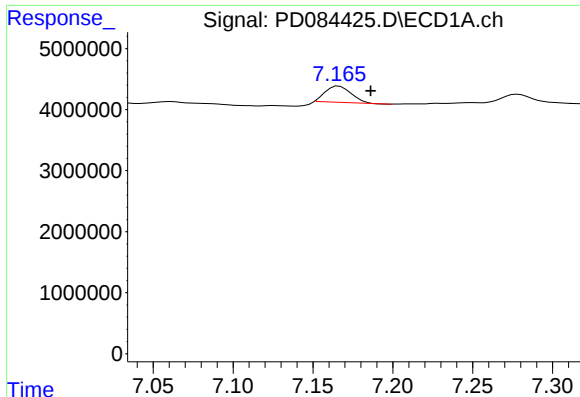

#19 Endosulfan Sulfate


R.T.: 7.166 min
Delta R.T.: -0.020 min
Response: 2965002
Conc: 1.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

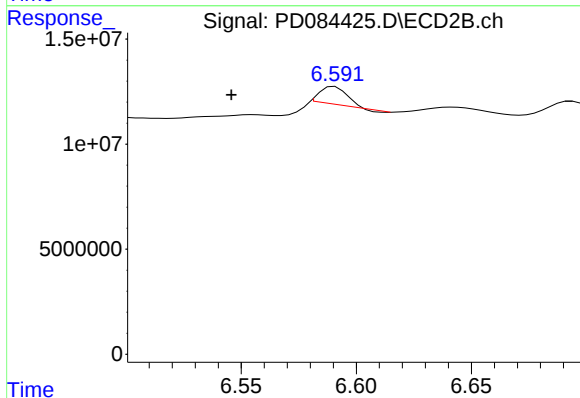


#19 Endosulfan Sulfate

R.T.: 6.591 min
Delta R.T.: 0.045 min
Response: 6610770
Conc: 1.42 ng/ml

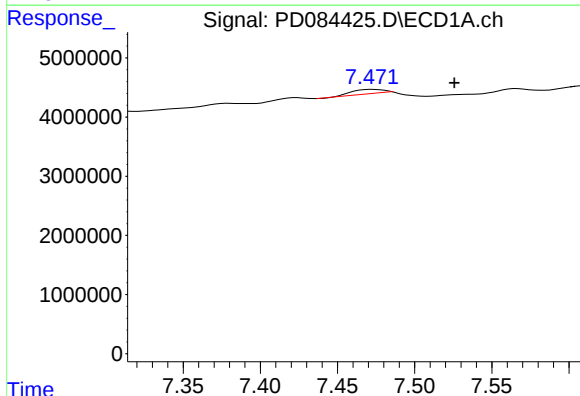


#20 Methoxychlor

R.T.: 7.473 min
Delta R.T.: -0.053 min
Response: 1260582
Conc: 1.58 ng/ml

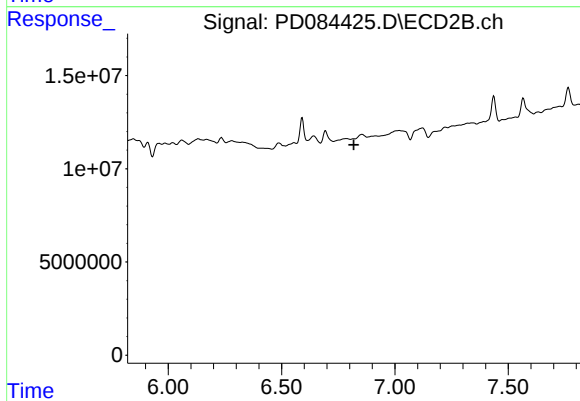

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.819 min
Response: 0
Conc: N.D.

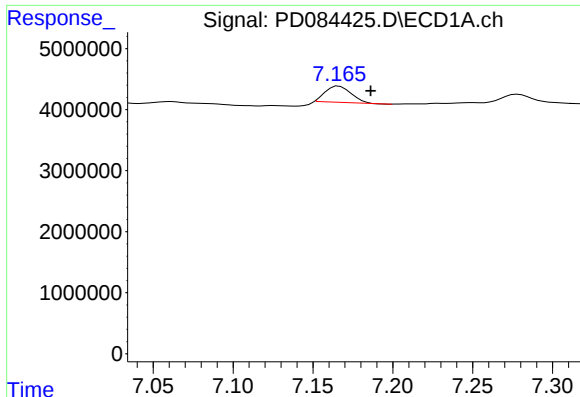

#25 Toxaphene-4


R.T.: 7.166 min
Delta R.T.: -0.020 min
Response: 2965002
Conc: 88.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

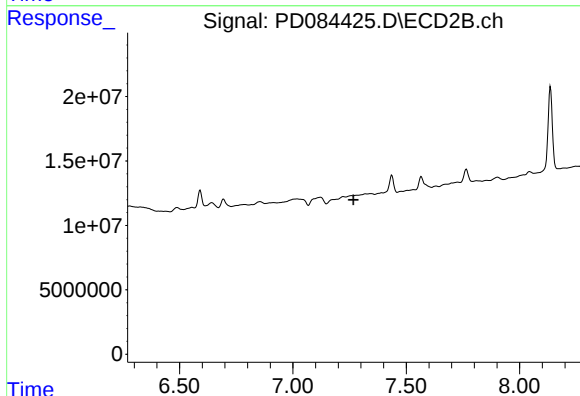


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.267 min
Response: 0
Conc: N.D.

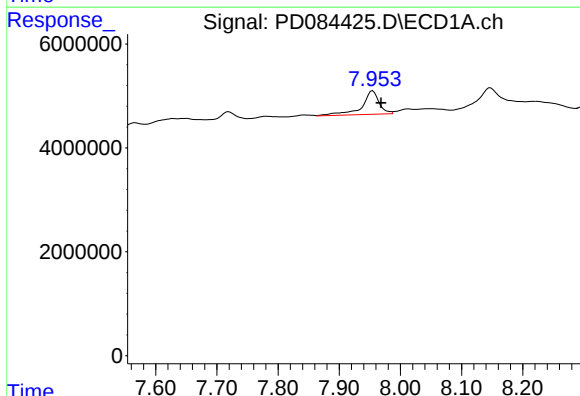


#26 Toxaphene-5

R.T.: 7.955 min
Delta R.T.: -0.014 min
Response: 8795256
Conc: 354.51 ng/ml

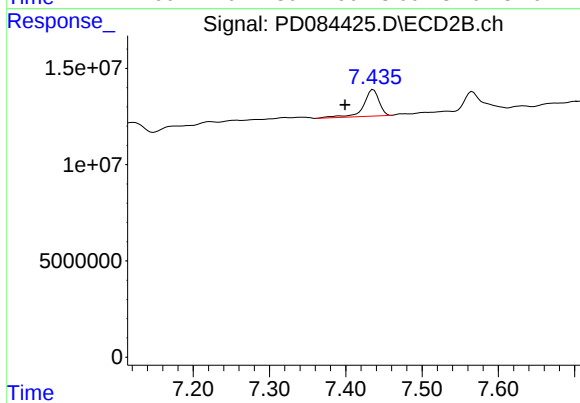

#26 Toxaphene-5


R.T.: 7.436 min
Delta R.T.: 0.037 min
Response: 19515473
Conc: 355.87 ng/ml

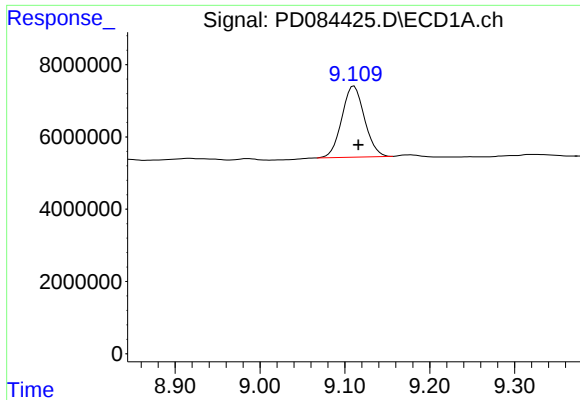

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.005 min
Response: 36435434
Conc: 20.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

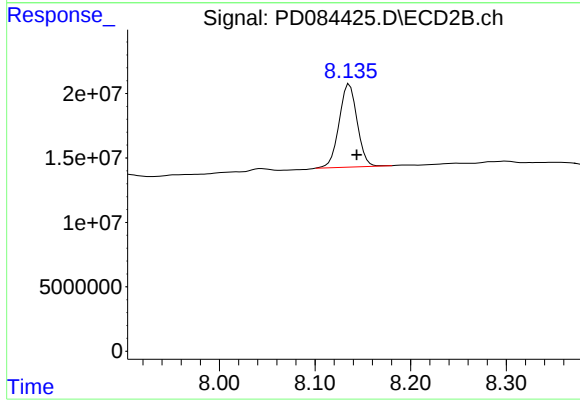

#27 Decachlorobiphenyl

R.T.: 8.136 min
Delta R.T.: -0.008 min
Response: 84759432
Conc: 22.55 ng/ml