

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD081424\  
 Data File : PD084427.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Aug 2024 22:04  
 Operator : AR\AJ  
 Sample : P3481-15  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 15 02:11:05 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD081224CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Aug 12 16:40:36 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
-----						
System Monitoring Compounds						
1) SA Tetrachlo...	3.583	2.929	9284940	56094376	11.075	10.656
2) SA Decachlor...	9.111	8.137	24039825	57075602	13.821	15.188
Target Compounds						
6) B beta-BHC	0.000	4.033f	0	170.4E6	N.D.	47.388
7) B delta-BHC	4.813	0.000	1887970	0	1.093	N.D. #
9) A Endosulfan I	6.096	0.000	2686623	0	1.687	N.D. #
10) B trans-Chl...	6.037f	0.000	1659170	0	1.005	N.D. #
11) B cis-Chlor...	6.037	0.000	1659170	0	0.964	N.D. #
12) B 4,4'-DDE	6.254	0.000	6820365	0	3.899	N.D. #
20) A Methoxychlor	7.472f	0.000	1118553	0	1.403	N.D. #
26) Toxaphene-5	7.956	7.436f	-912667	22737678	N.D.	414.628
-----						


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD081424\  
 Data File : PD084427.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Aug 2024 22:04  
 Operator : AR\AJ  
 Sample : P3481-15  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 15 02:11:05 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD081224CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Aug 12 16:40:36 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

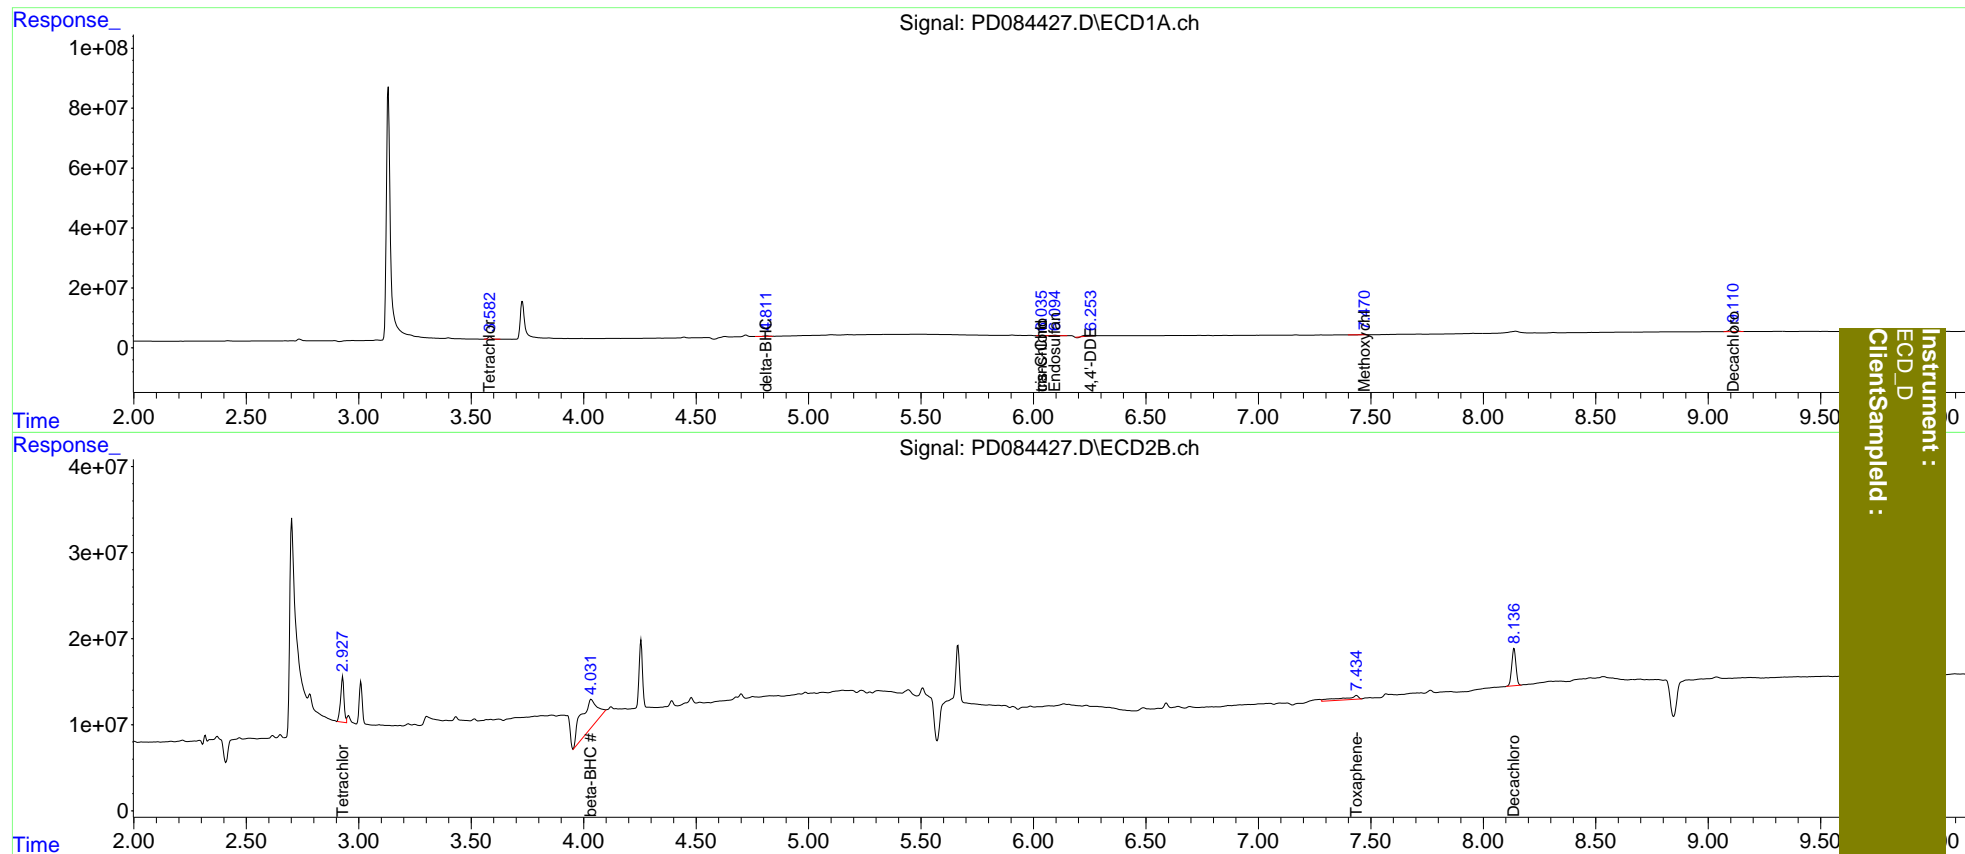


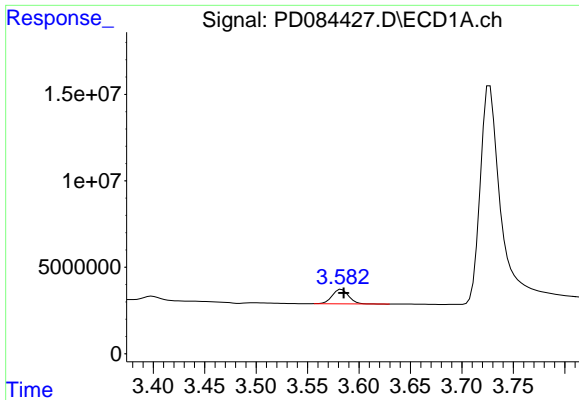

#1 Tetrachloro-m-xylene


R.T.: 3.583 min  
 Delta R.T.: -0.002 min  
 Response: 9284940  
 Conc: 11.07 ng/ml

Instrument :  
 ECD\_D  
 ClientSampleId :

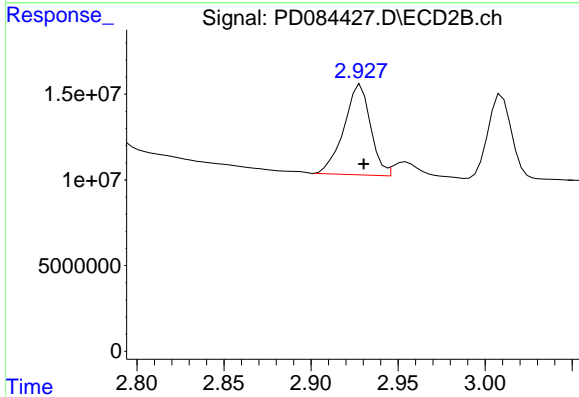


#1 Tetrachloro-m-xylene

R.T.: 2.929 min  
 Delta R.T.: -0.002 min  
 Response: 56094376  
 Conc: 10.66 ng/ml

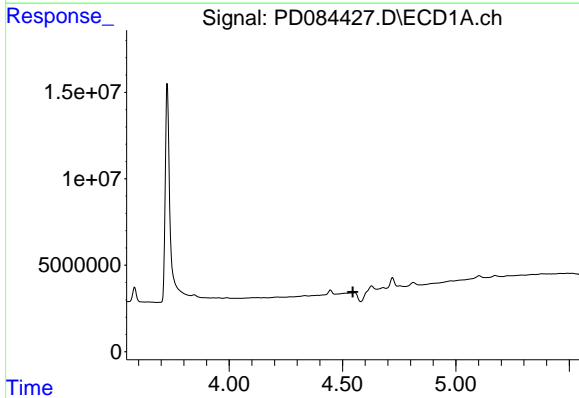


#6 beta-BHC

R.T.: 0.000 min  
 Exp R.T. : 4.546 min  
 Response: 0  
 Conc: N.D.

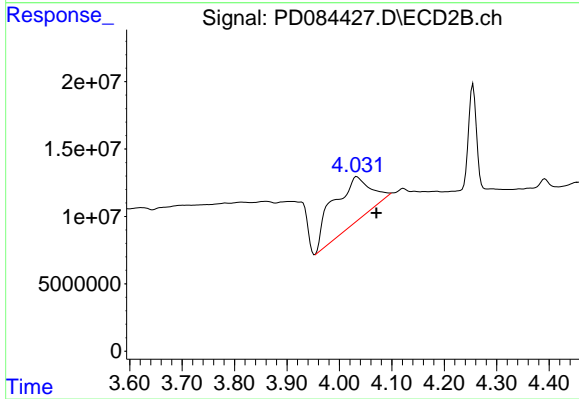

#6 beta-BHC


R.T.: 4.033 min  
 Delta R.T.: -0.037 min  
 Response: 170425372  
 Conc: 47.39 ng/ml

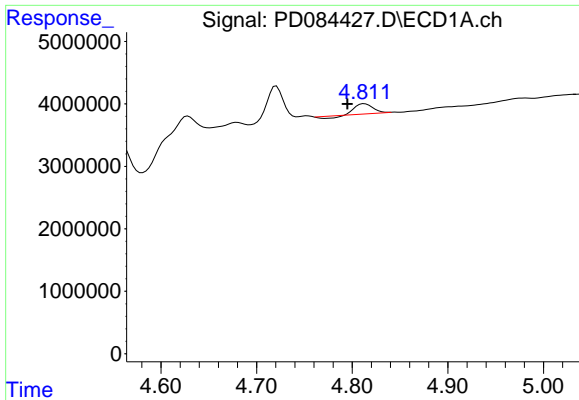

#7 delta-BHC


R.T.: 4.813 min  
 Delta R.T.: 0.018 min  
 Response: 1887970  
 Conc: 1.09 ng/ml

Instrument :  
 ECD\_D  
 ClientSampleId :

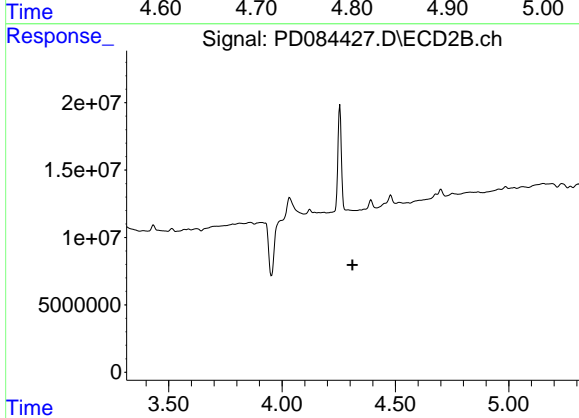


#7 delta-BHC

R.T.: 0.000 min  
 Exp R.T. : 4.311 min  
 Response: 0  
 Conc: N.D.

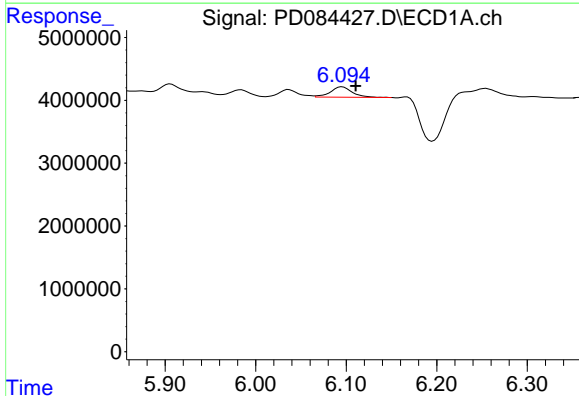


#9 Endosulfan I

R.T.: 6.096 min  
 Delta R.T.: -0.015 min  
 Response: 2686623  
 Conc: 1.69 ng/ml

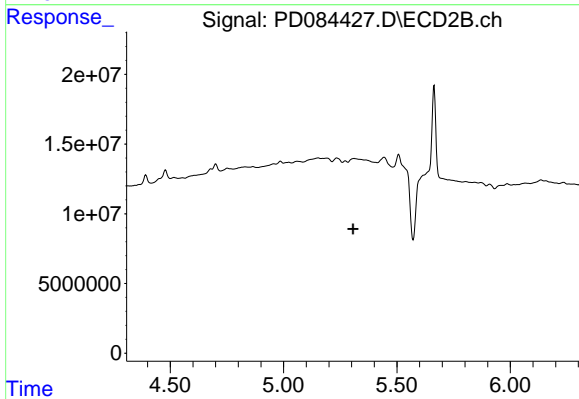

#9 Endosulfan I


R.T.: 0.000 min  
 Exp R.T. : 5.306 min  
 Response: 0  
 Conc: N.D.

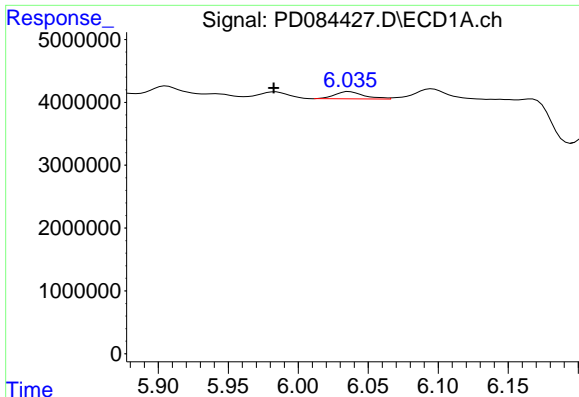

#10 trans-Chlordane


R.T.: 6.037 min  
 Delta R.T.: 0.054 min  
 Response: 1659170  
 Conc: 1.00 ng/ml

Instrument :  
 ECD\_D  
 ClientSampleId :

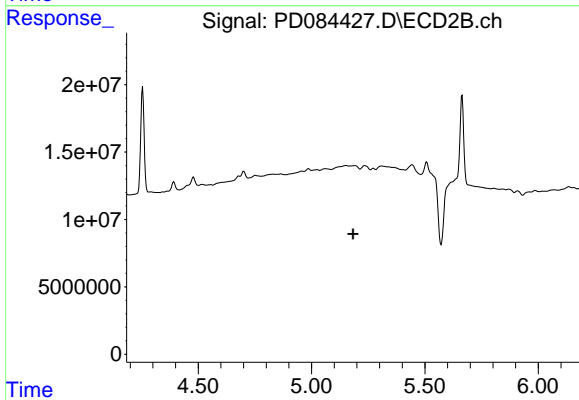


#10 trans-Chlordane

R.T.: 0.000 min  
 Exp R.T. : 5.184 min  
 Response: 0  
 Conc: N.D.

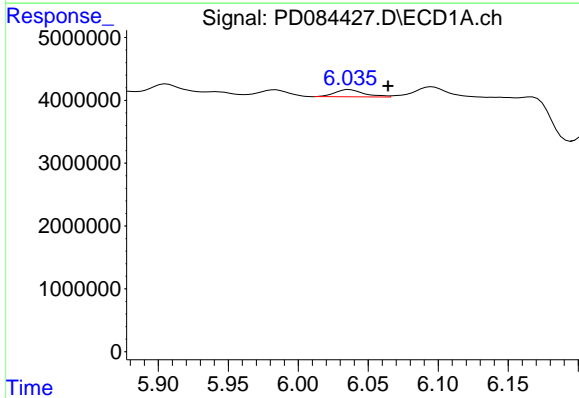


#11 cis-Chlordane

R.T.: 6.037 min  
 Delta R.T.: -0.027 min  
 Response: 1659170  
 Conc: 0.96 ng/ml

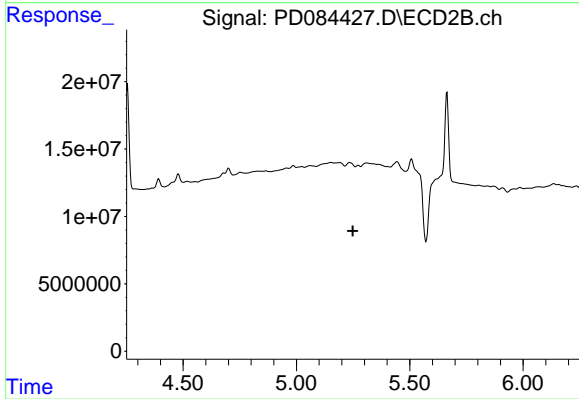


#11 cis-Chlordane

R.T.: 0.000 min  
 Exp R.T. : 5.249 min  
 Response: 0  
 Conc: N.D.

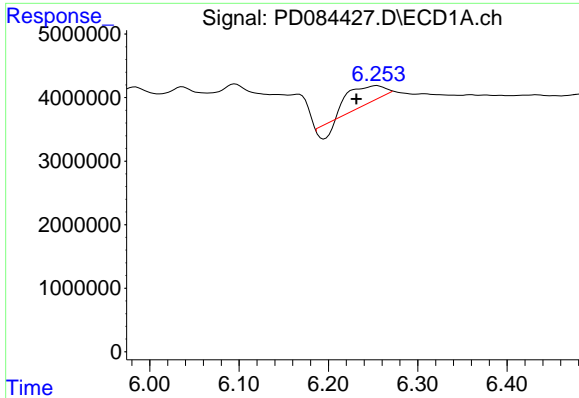


#12 4,4'-DDE  
 R.T.: 6.254 min  
 Delta R.T.: 0.023 min  
 Response: 6820365  
 Conc: 3.90 ng/ml


Instrument :  
 ECD\_D  
 ClientSampleId :

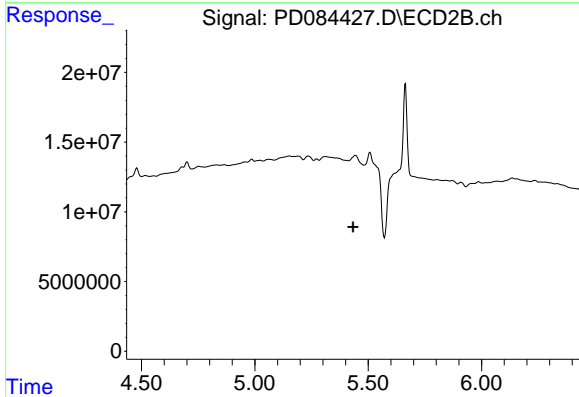


#12 4,4'-DDE  
 R.T.: 0.000 min  
 Exp R.T. : 5.434 min  
 Response: 0  
 Conc: N.D.

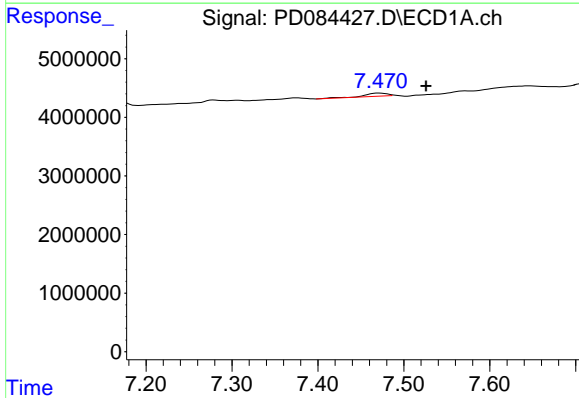

#20 Methoxychlor  
 R.T.: 7.472 min  
 Delta R.T.: -0.054 min  
 Response: 1118553  
 Conc: 1.40 ng/ml

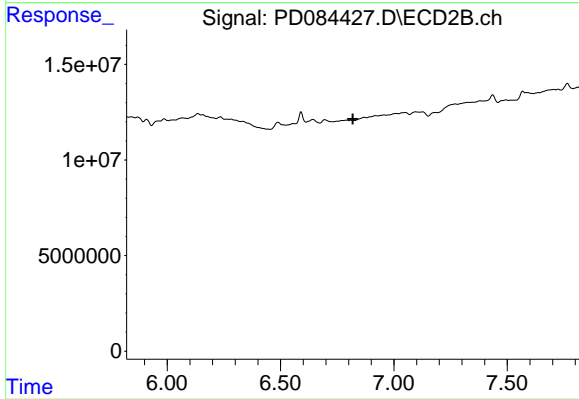


#20 Methoxychlor  
 R.T.: 0.000 min  
 Exp R.T. : 6.819 min  
 Response: 0  
 Conc: N.D.

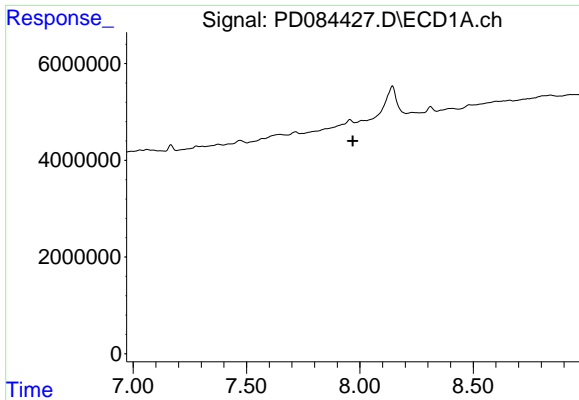

#26 Toxaphene-5


R.T.: 7.956 min  
 Delta R.T.: -0.012 min  
 Response: -912667  
 Conc: N.D.

Instrument :  
 ECD\_D  
 ClientSampleId :

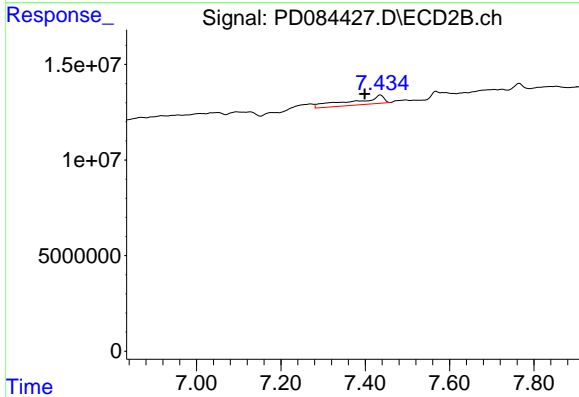


#26 Toxaphene-5

R.T.: 7.436 min  
 Delta R.T.: 0.037 min  
 Response: 22737678  
 Conc: 414.63 ng/ml

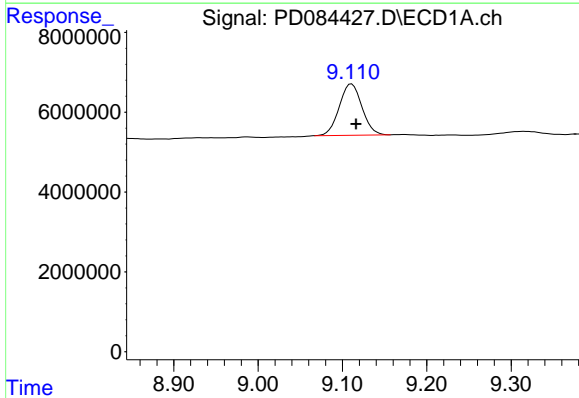

#27 Decachlorobiphenyl

R.T.: 9.111 min  
 Delta R.T.: -0.005 min  
 Response: 24039825  
 Conc: 13.82 ng/ml

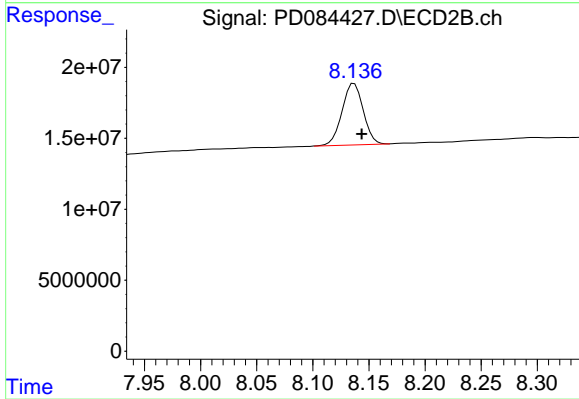

#27 Decachlorobiphenyl

R.T.: 8.137 min  
 Delta R.T.: -0.007 min  
 Response: 57075602  
 Conc: 15.19 ng/ml