

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
 Data File : PD084405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 16:43
 Operator : AR\AJ
 Sample : P3171-02DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVT1DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/19/2024
 Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 02:07:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.927	7137746	53066942	8.514	10.081
27)	SA Decachlor...	9.113	8.138	17134863	48600001	9.852	12.933 #
Target Compounds							
2)	A alpha-BHC	4.032	3.441	651.2E6	2009.2E6	430.270	246.479 #
3)	MA gamma-BHC...	4.362	3.777	713.3E6	2233.9E6	457.955	289.858 #
4)	MA Heptachlor	4.963	4.134	1282.7E6	3054.1E6	734.916	405.254m#
5)	MB Aldrin	5.305	4.422	531.5E6	1362.0E6	301.174	185.844 #
6)	B beta-BHC	4.544	4.070	302.8E6	1137.2E6	419.103	316.216
7)	B delta-BHC	4.794	4.309	394.2E6	1324.8E6	228.257	157.944 #
8)	B Heptachlo...	5.724	4.927	417.1E6	1168.8E6	245.390	175.173 #
9)	A Endosulfan I	6.108	5.302	434.7E6	1114.3E6	272.857	187.808m#
10)	B trans-Chl...	5.978	5.181	387.6E6	1108.1E6	234.752	173.894 #
11)	B cis-Chlor...	6.060	5.246	322.4E6	924.5E6	187.337	146.889
12)	B 4,4'-DDE	6.228	5.429	1132.6E6	2803.6E6	647.546	459.734m#
13)	MA Dieldrin	6.381	5.569	1002.0E6	2377.5E6	557.699	386.482m#
14)	MA Endrin	6.609	5.847	179.3E6	572.5E6	119.662	103.703
15)	B Endosulfa...	6.819	6.139	694.0E6	1678.4E6	420.915	323.246
16)	A 4,4'-DDD	6.737	5.985	727.2E6	1969.2E6	565.412	401.385m#
17)	MA 4,4'-DDT	7.052	6.243	707.0E6	1817.1E6	521.484m	366.810 #
18)	B Endrin al...	6.948	6.317	93588176	294.4E6	82.341	78.689
19)	B Endosulfa...	7.182	6.542	178.5E6	493.3E6	117.607	105.663
20)	A Methoxychlor	7.524	6.814	104.3E6	324.1E6	130.754	150.486
21)	B Endrin ke...	7.664	7.053	780.6E6	1842.3E6	471.386	353.775

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
Data File : PD084405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 16:43
Operator : AR\AJ
Sample : P3171-02DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 02:07:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

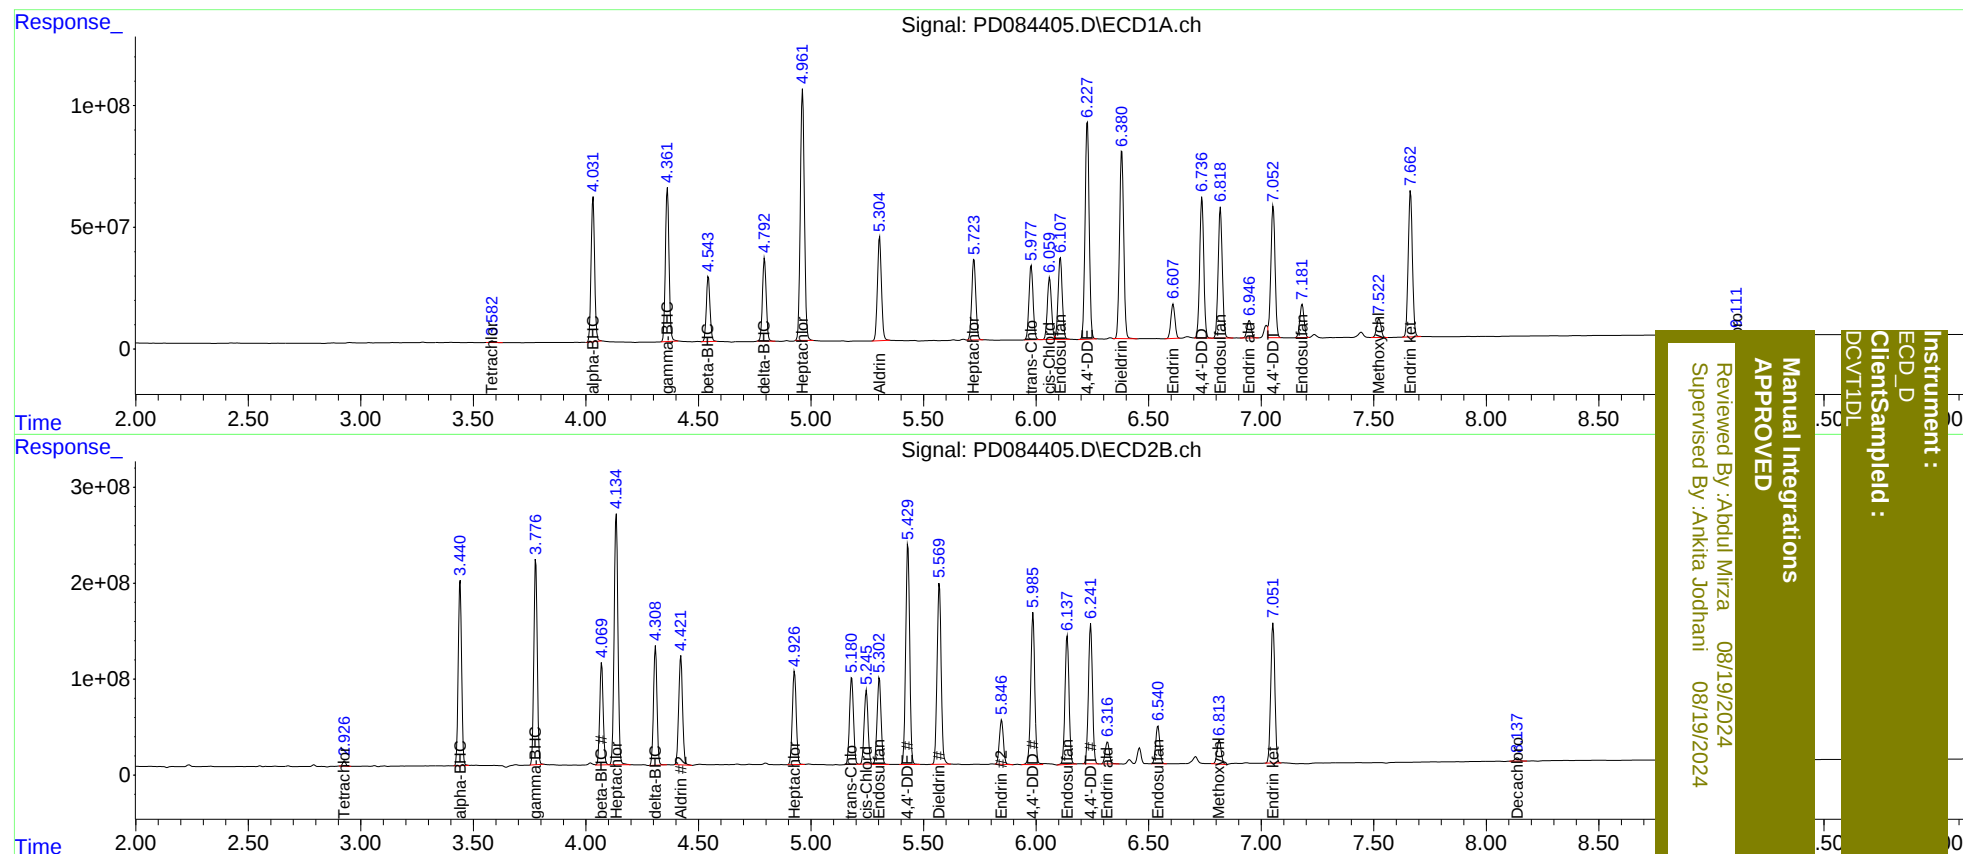

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Instrument :
ECD_D
Client Sampled :
DCVTIDL