

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
 Data File : PD084406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 16:56
 Operator : AR\AJ
 Sample : P3171-02DL2 20X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVT1DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/19/2024
 Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 02:07:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.928	671733	6447921	0.801m	1.225 #
27)	SA Decachlor...	9.113	8.137	2320461	4796939	1.334	1.276m
Target Compounds							
2)	A alpha-BHC	4.032	3.442	53306554	278.8E6	35.220	34.204
3)	MA gamma-BHC...	4.362	3.778	60666946	291.0E6	38.951	37.764
4)	MA Heptachlor	4.963	4.134	116.0E6	440.5E6	66.466	58.447m
5)	MB Aldrin	5.305	4.422	47774622	200.5E6	27.070	27.362
6)	B beta-BHC	4.544	4.070	30550996	154.7E6	42.285	43.014
7)	B delta-BHC	4.794	4.309	33292748	175.1E6	19.279	20.871
8)	B Heptachlo...	5.725	4.927	39608607	166.6E6	23.304	24.963
9)	A Endosulfan I	6.108	5.302	42145056	160.7E6	26.457	27.084m
10)	B trans-Chl...	5.979	5.181	36307952	153.3E6	21.989	24.065
11)	B cis-Chlor...	6.061	5.246	30983185	127.8E6	18.006	20.308
12)	B 4,4'-DDE	6.228	5.431	105.9E6	381.3E6	60.563	62.522
13)	MA Dieldrin	6.381	5.570	91196111	332.1E6	50.760	53.978
14)	MA Endrin	6.609	5.847	16864149	78292642	11.257	14.181 #
15)	B Endosulfa...	6.820	6.139	66970190	232.8E6	40.618	44.841
16)	A 4,4'-DDD	6.737	5.985	64862047	272.7E6	50.430	55.580m
17)	MA 4,4'-DDT	7.053	6.242	64346318	242.7E6	47.460m	48.991
18)	B Endrin al...	6.949	6.317	9455018	38477377	8.319	10.284
19)	B Endosulfa...	7.182	6.542	18019919	66758313	11.871	14.299
20)	A Methoxychlor	7.524	6.815	10945725	43016612	13.725	19.976 #
21)	B Endrin ke...	7.664	7.053	77479871	255.9E6	46.785	49.138

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
Data File : PD084406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 16:56
Operator : AR\AJ
Sample : P3171-02DL2 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 02:07:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

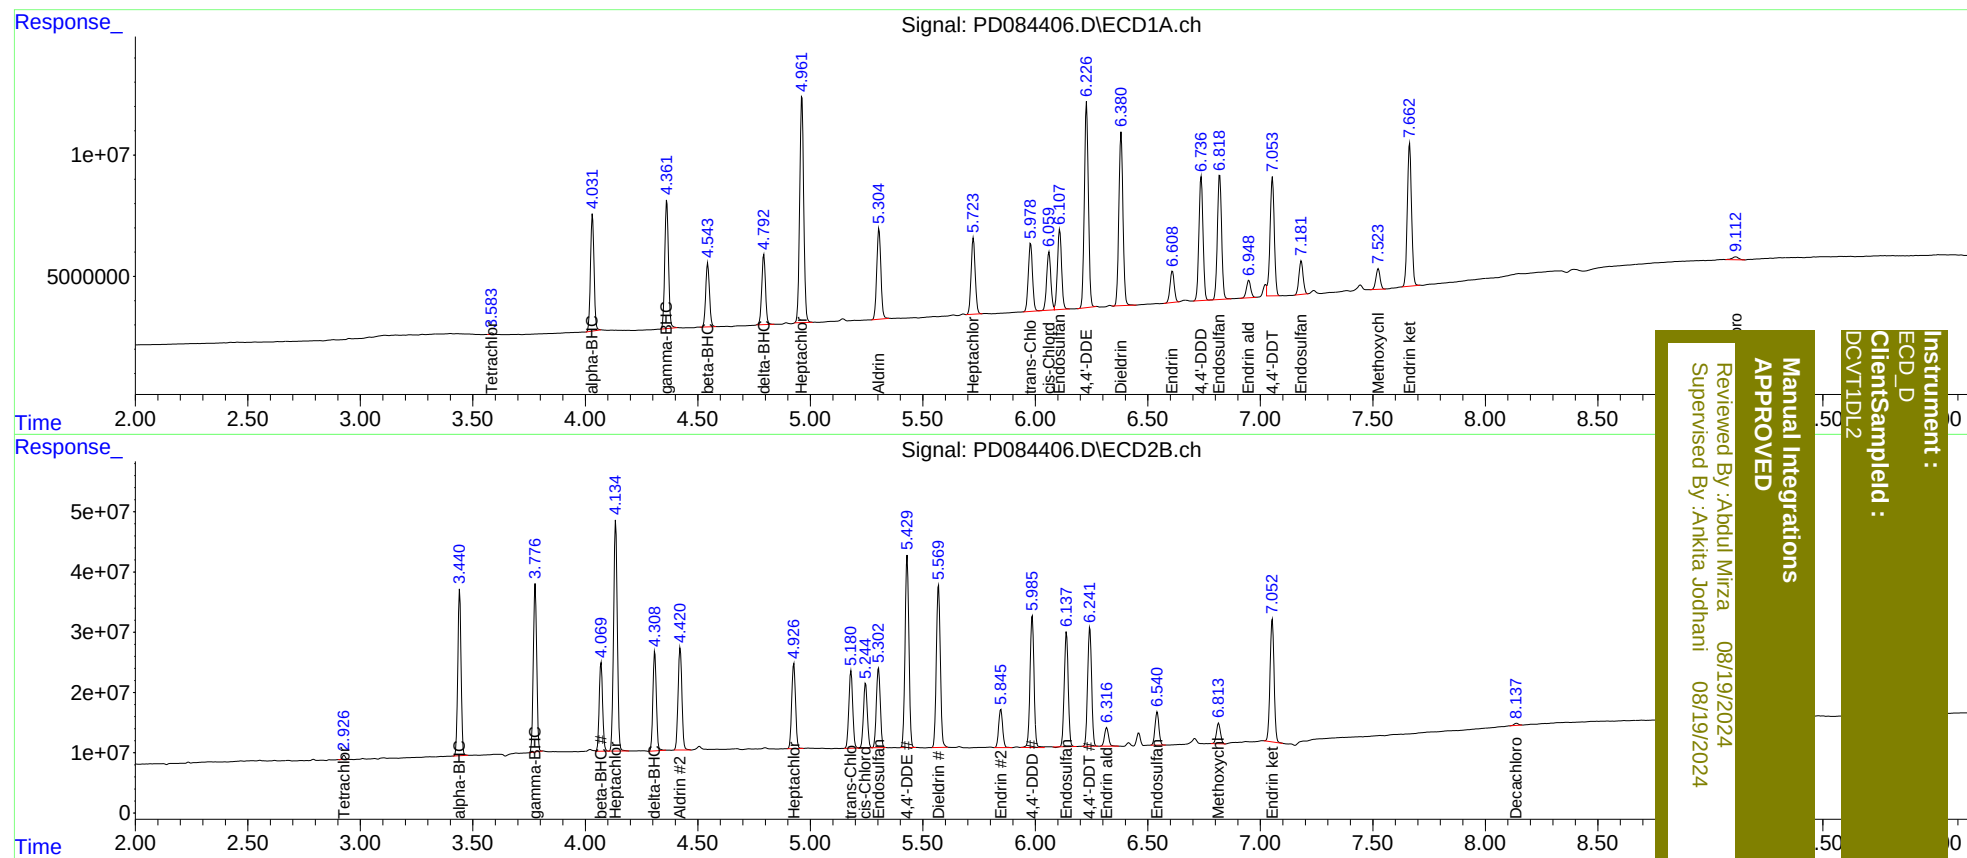

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Instrument :
ECD_D
Client Sampled :
DCVT1DL2