

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
 Data File : PD084434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 23:38
 Operator : AR\AJ
 Sample : P3481-09MS
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AE4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/19/2024
 Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 02:12:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.928	9334378	62609974	11.134	11.894
27)	SA Decachlor...	9.109	8.136	22007819	39119064	12.653	10.410
Target Compounds							
2)	A alpha-BHC	4.032	3.441	75964908	376.7E6	50.190	46.212
3)	MA gamma-BHC...	4.362	3.777	76792586	352.2E6	49.304	45.696
4)	MA Heptachlor	4.962	4.134	85172133	325.0E6	48.800	43.129
5)	MB Aldrin	5.304	4.421	84023813	276.3E6	47.610	37.696
6)	B beta-BHC	4.543	4.069	24924398	128.7E6	34.497	35.773
7)	B delta-BHC	4.793	4.309	75422956	339.6E6	43.675	40.482
8)	B Heptachlo...	5.724	4.926	81009499	294.1E6	47.662	44.081
9)	A Endosulfan I	6.108	5.301	76741248	261.6E6	48.175	44.093m
10)	B trans-Chl...	5.978	5.180	76251340	274.9E6	46.181	43.144
11)	B cis-Chlor...	6.059	5.245	79933617	295.6E6	46.453	46.973
12)	B 4,4'-DDE	6.227	5.430	156.2E6	537.3E6	89.293	88.104
13)	MA Dieldrin	6.380	5.569	172.7E6	566.8E6	96.115	92.141
14)	MA Endrin	6.608	5.846	153.9E6	476.2E6	102.706	86.255
15)	B Endosulfa...	6.818	6.138	145.5E6	438.7E6	88.262	84.490
16)	A 4,4'-DDD	6.736	5.985	128.0E6	394.7E6	99.530	80.450
17)	MA 4,4'-DDT	7.051	6.241	125.8E6	410.2E6	92.777m	82.810
18)	B Endrin al...	6.947	6.316	108.6E6	292.6E6	95.559	78.204
19)	B Endosulfa...	7.181	6.540	142.6E6	377.0E6	93.921	80.758
20)	A Methoxychlor	7.523	6.814	354.5E6	885.5E6	444.545	411.193
21)	B Endrin ke...	7.662	7.051	153.6E6	412.4E6	92.744	79.183

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
Data File : PD084434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 23:38
Operator : AR\AJ
Sample : P3481-09MS
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 02:12:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

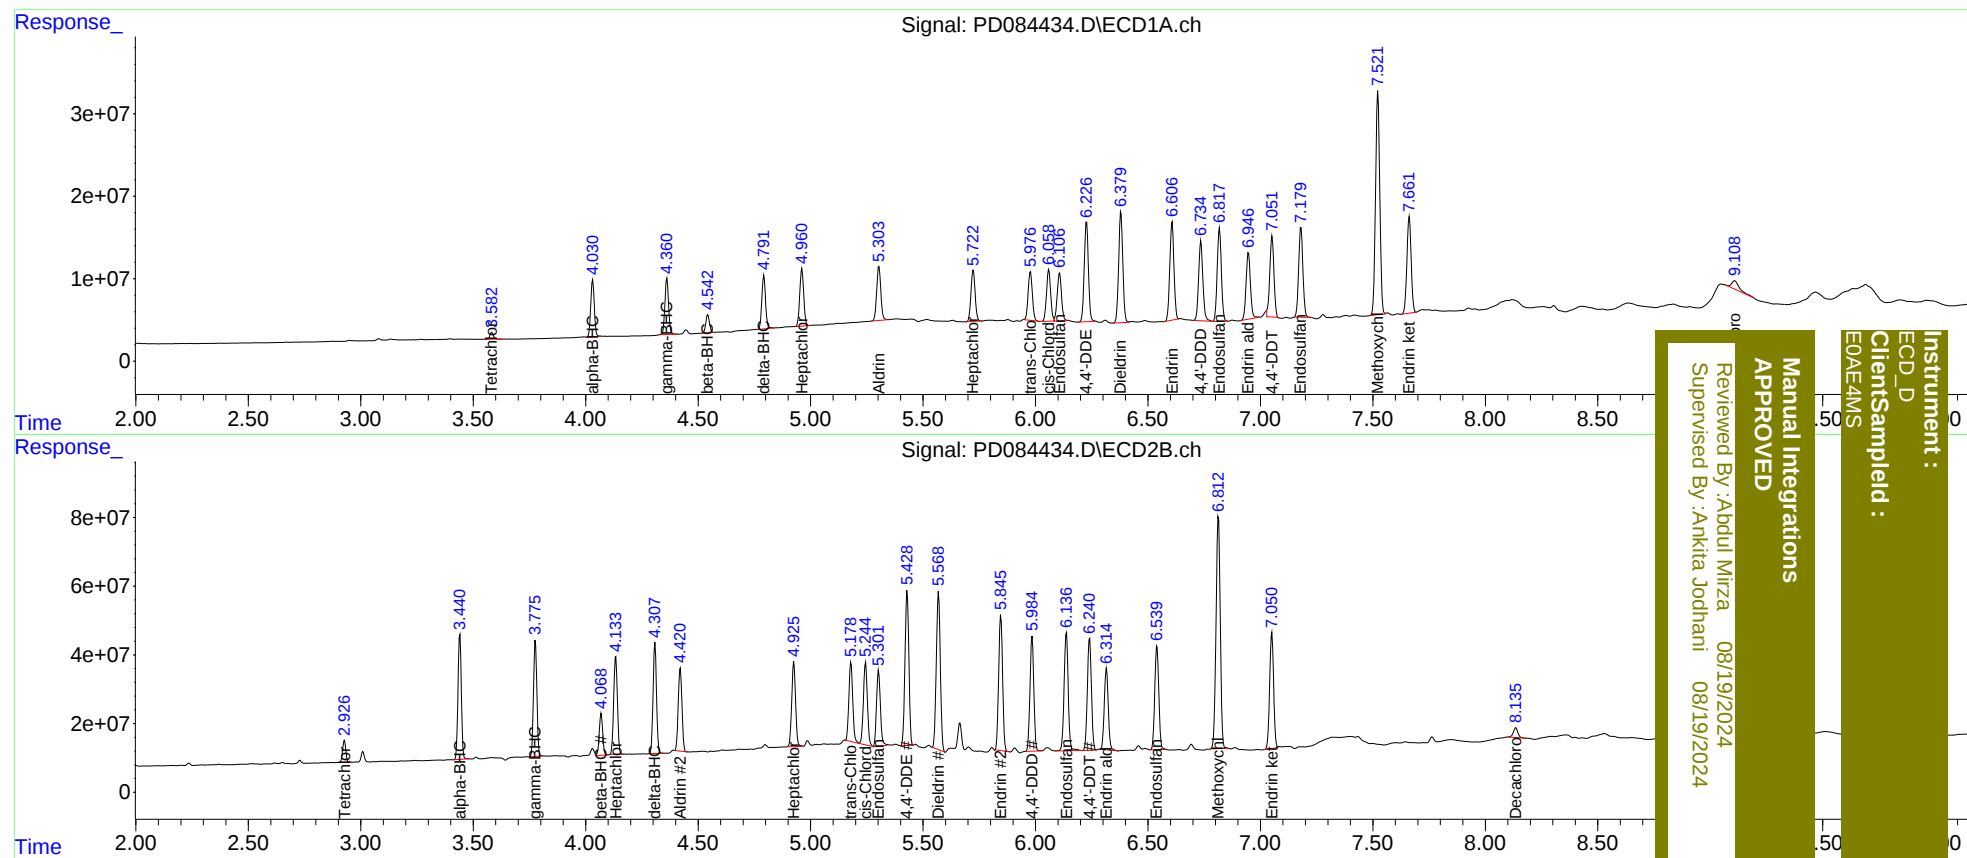

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Instrument :
ECD_D
Client Sampled :
EOAE4MS