

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
 Data File : PD084435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 23:51
 Operator : AR\AJ
 Sample : P3481-10MSD
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AE4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/19/2024
 Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 02:12:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.927	9354423	62328420	11.158	11.840
27)	SA Decachlor...	9.111	8.135	21245815	38463644	12.215	10.235
Target Compounds							
2)	A alpha-BHC	4.031	3.441	76256899	374.3E6	50.383	45.913
3)	MA gamma-BHC...	4.362	3.777	76900766	348.3E6	49.373	45.187
4)	MA Heptachlor	4.962	4.134	85592813	306.6E6	49.041	40.680
5)	MB Aldrin	5.304	4.421	84897502	264.4E6	48.105	36.082
6)	B beta-BHC	4.544	4.069	25178085	121.0E6	34.848	33.633
7)	B delta-BHC	4.793	4.308	75184209	327.5E6	43.537	39.045
8)	B Heptachlo...	5.723	4.925	80866326	292.7E6	47.578	43.872
9)	A Endosulfan I	6.108	5.301	76830872	257.1E6	48.231	43.329m
10)	B trans-Chl...	5.978	5.179	76397582	276.3E6	46.269	43.366
11)	B cis-Chlor...	6.060	5.244	80591818	294.7E6	46.835	46.828
12)	B 4,4'-DDE	6.227	5.429	156.1E6	531.3E6	89.268	87.119
13)	MA Dieldrin	6.380	5.568	170.5E6	564.5E6	94.918	91.762
14)	MA Endrin	6.608	5.845	154.4E6	477.8E6	103.078	86.537
15)	B Endosulfa...	6.818	6.137	147.7E6	452.2E6	89.577	87.089
16)	A 4,4'-DDD	6.736	5.985	127.6E6	406.7E6	99.176	82.900
17)	MA 4,4'-DDT	7.051	6.241	129.9E6	427.7E6	95.835m	86.332
18)	B Endrin al...	6.947	6.315	104.8E6	315.9E6	92.219	84.435
19)	B Endosulfa...	7.181	6.540	140.8E6	387.5E6	92.779	83.005
20)	A Methoxychlor	7.523	6.813	346.6E6	878.1E6	434.629	407.758
21)	B Endrin ke...	7.663	7.051	149.0E6	432.4E6	89.994	83.022

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081424\
Data File : PD084435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 23:51
Operator : AR\AJ
Sample : P3481-10MSD
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 02:12:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

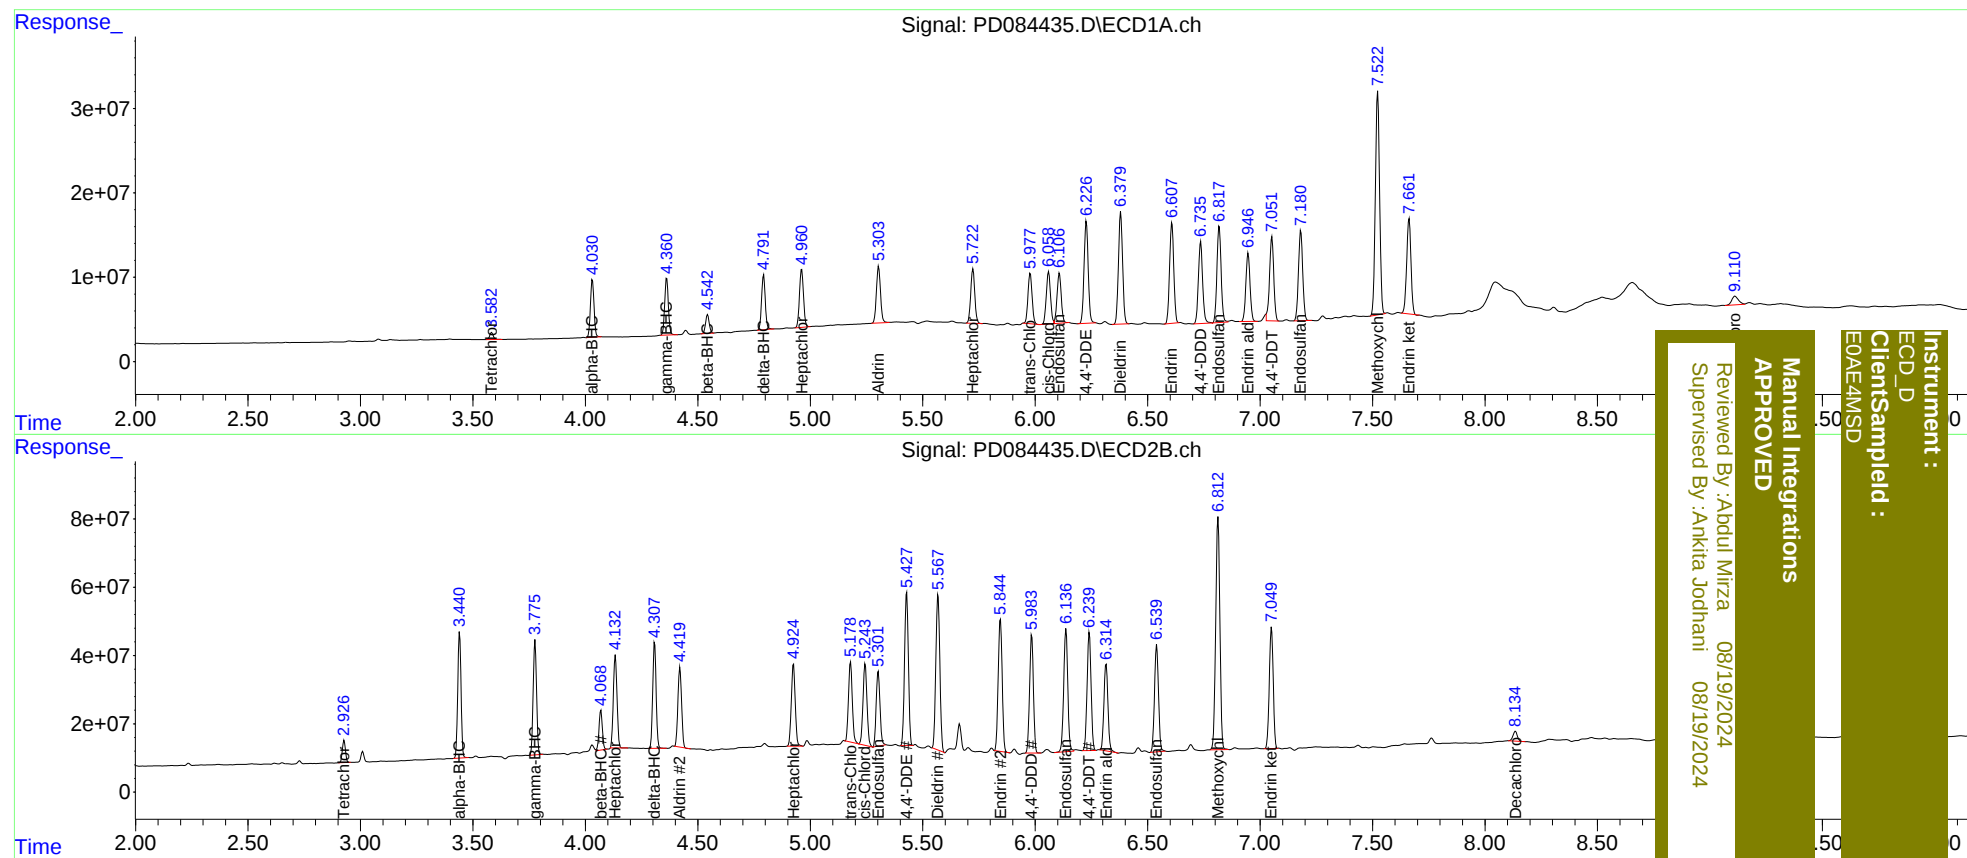

Instrument :
ECD_D
Client Sampled :
EOAE4MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024