

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081519\
 Data File : PD054291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Aug 2019 19:30
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 07:48:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 16 07:48:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	31166152	40885192	50.000	50.000
28)	SA Decachlor...	8.007	9.026	30949541	40498451	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.158	4.972	9948621	15849012	500.000	500.000
24)	Chlordane-2	4.651	5.437	12761105	17661632	500.000	500.000
25)	Chlordane-3	5.208	6.080	38705316	78475443	500.000	500.000
26)	Chlordane-4	5.265	6.154	34115225	95220336	500.000	500.000
27)	Chlordane-5	6.091	6.956	13496019	16958007	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081519\
Data File : PD054291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Aug 2019 19:30
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 07:48:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081519.M
Quant Title : GC Extractables
QLast Update : Fri Aug 16 07:48:14 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

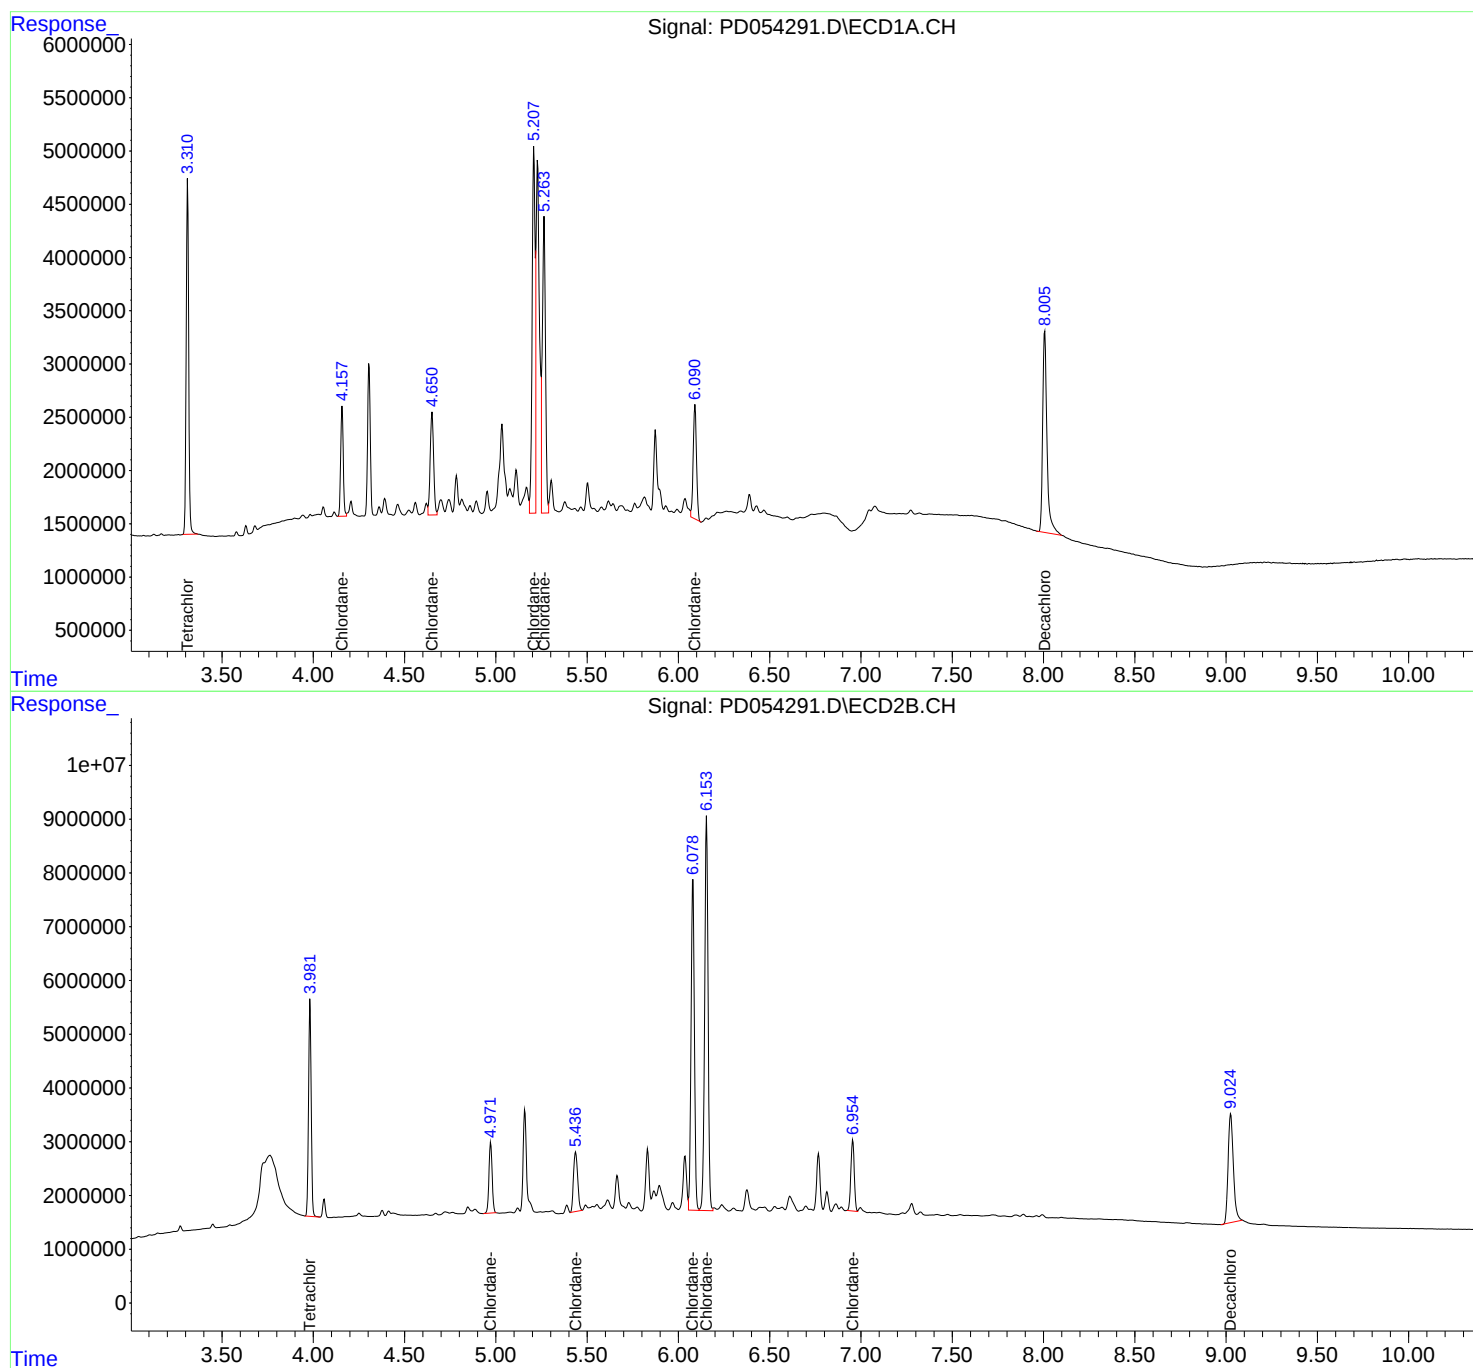


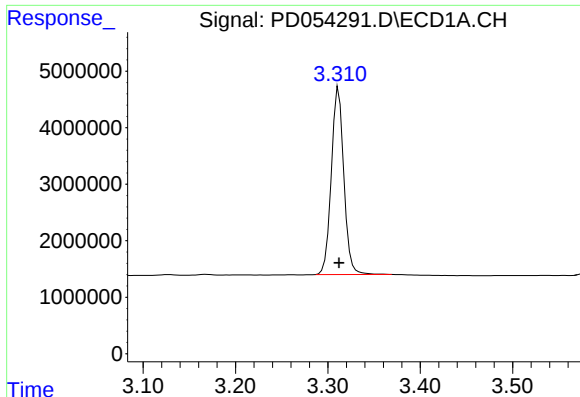

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 31166152
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

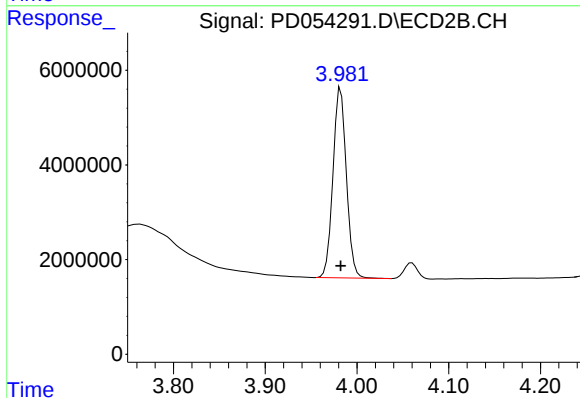


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 40885192
Conc: 50.00 ng/ml

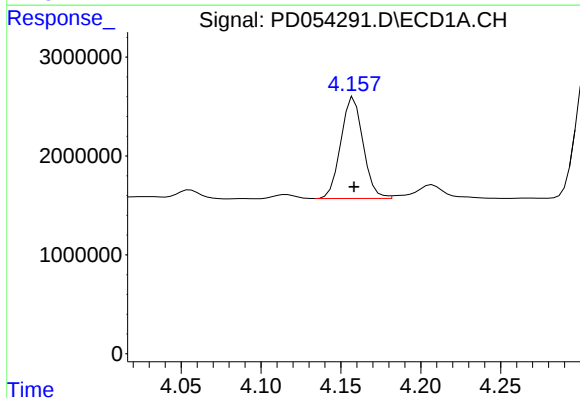


#23 Chlordane-1

R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 9948621
Conc: 500.00 ng/ml

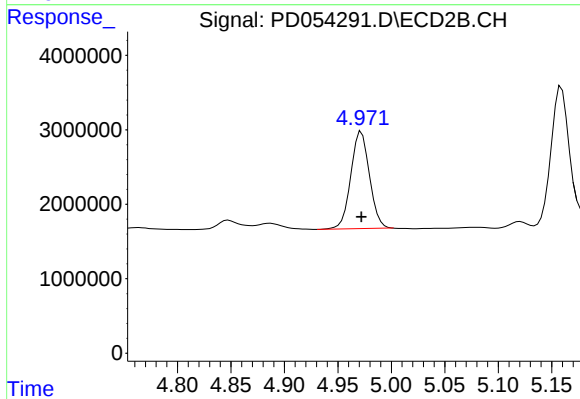

#23 Chlordane-1


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 15849012
Conc: 500.00 ng/ml

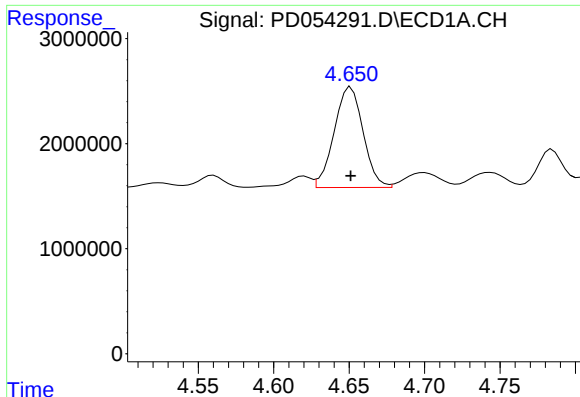

#24 Chlordane-2


R.T.: 4.651 min
Delta R.T.: 0.000 min
Response: 12761105
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

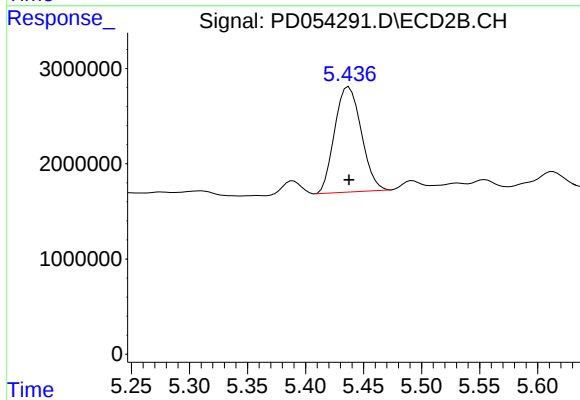


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 17661632
Conc: 500.00 ng/ml

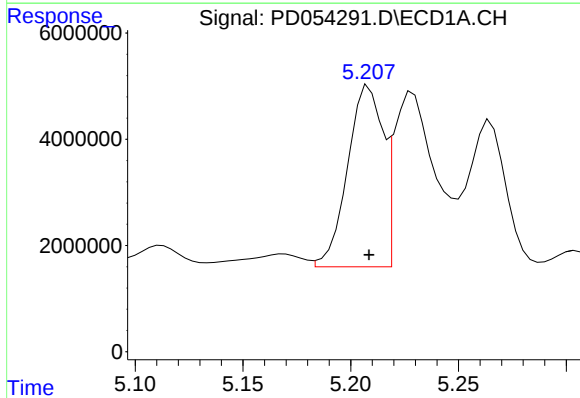


#25 Chlordane-3

R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 38705316
Conc: 500.00 ng/ml

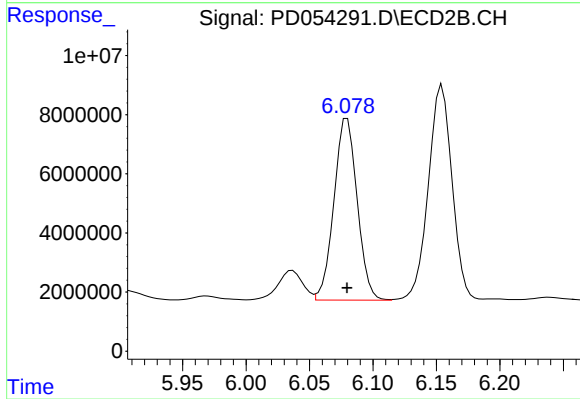

#25 Chlordane-3


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 78475443
Conc: 500.00 ng/ml

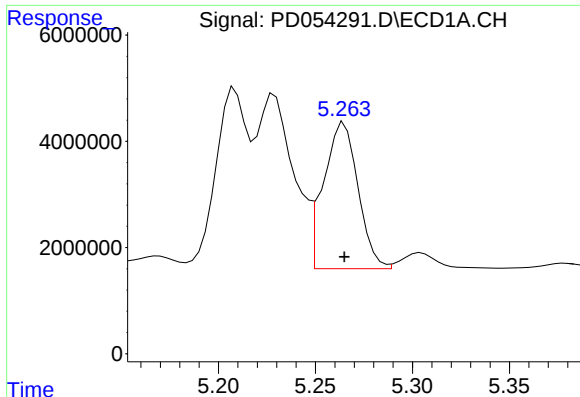

#26 Chlordane-4


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 34115225
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

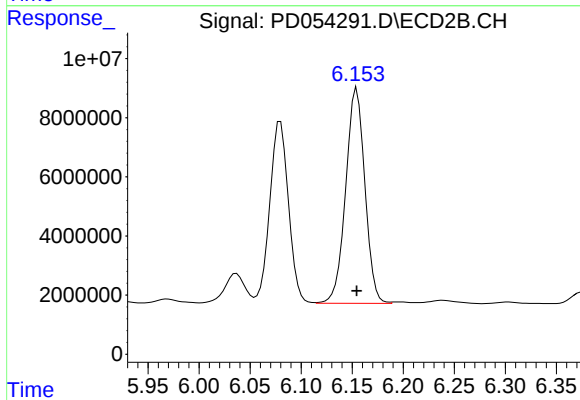


#26 Chlordane-4

R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 95220336
Conc: 500.00 ng/ml

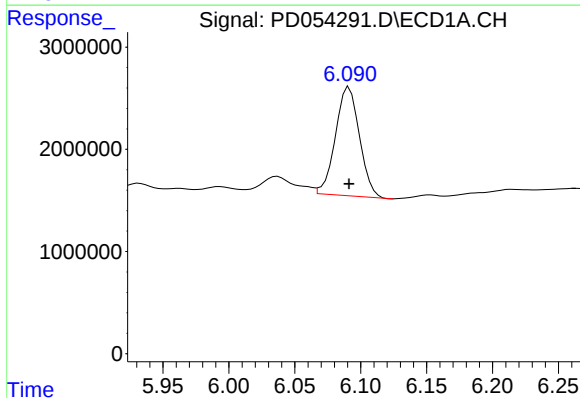


#27 Chlordane-5

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 13496019
Conc: 500.00 ng/ml

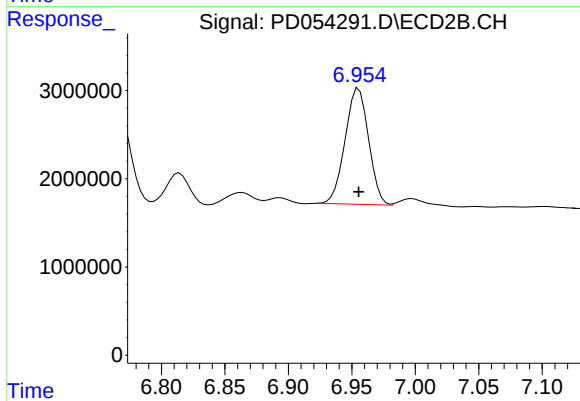

#27 Chlordane-5


R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 16958007
Conc: 500.00 ng/ml

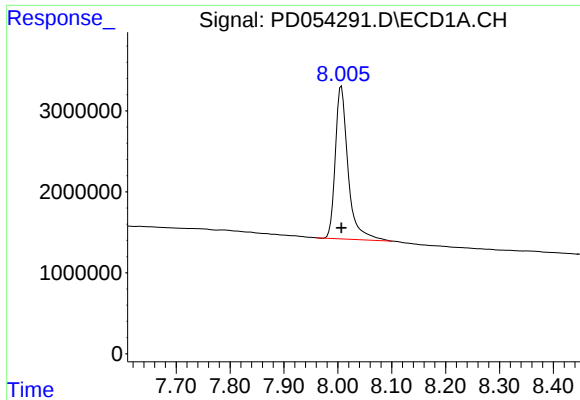

#28 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: 0.000 min
Response: 30949541
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

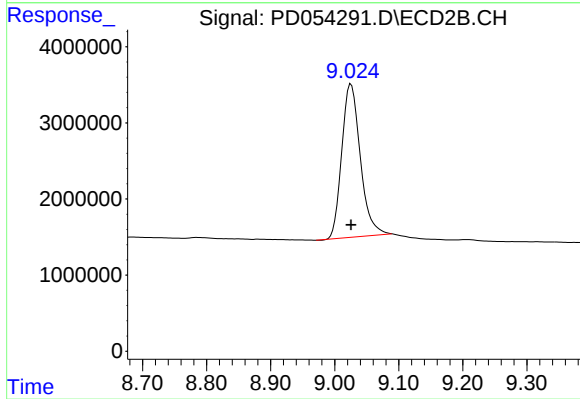

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.000 min
Response: 40498451
Conc: 50.00 ng/ml