

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
 Data File : PD071548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 17:39
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 05:42:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 05:36:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	62954934	701.4E6	23.036	23.931
28)	SA Decachlor...	7.999	9.089	68412847	245.5E6	23.554	24.061
Target Compounds							
9)	A Endosulfan I	5.160	6.104	39925815	203.6E6	11.546	13.085
10)	B gamma-Chl...	5.039	5.971	44329580	223.6E6	11.424	13.002
12)	B 4,4'-DDE	5.295	6.221	79080652	373.6E6	22.803	23.981
13)	MA Dieldrin	5.427	6.382	88417380	406.8E6	22.793	23.928
19)	B Endosulfa...	6.405	7.204	64400674	269.8E6	21.130	22.007
20)	A Methoxychlor	6.686	7.534	173.2E6	663.4E6	109.793	104.751
21)	B Endrin ke...	6.915	7.695	83177807	325.3E6	23.192	24.265



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
Data File : PD071548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 17:39
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 05:42:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 05:36:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

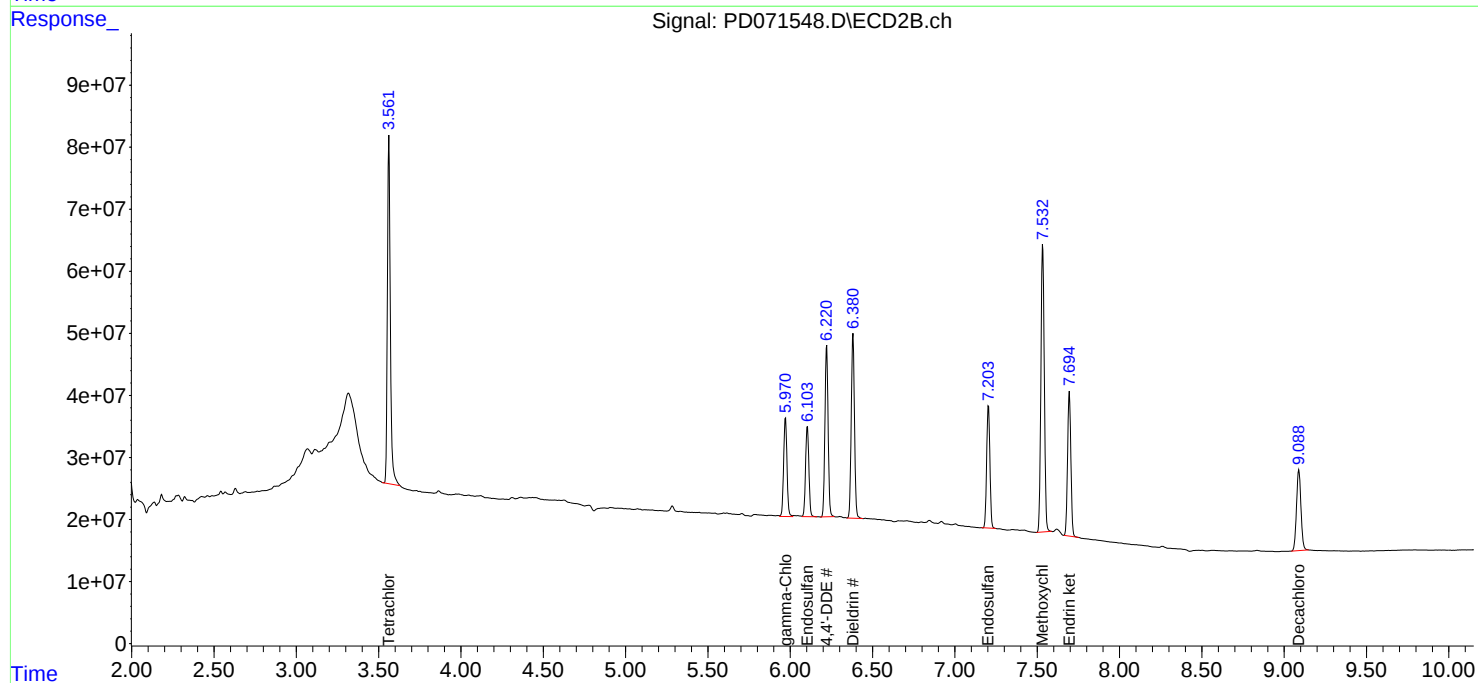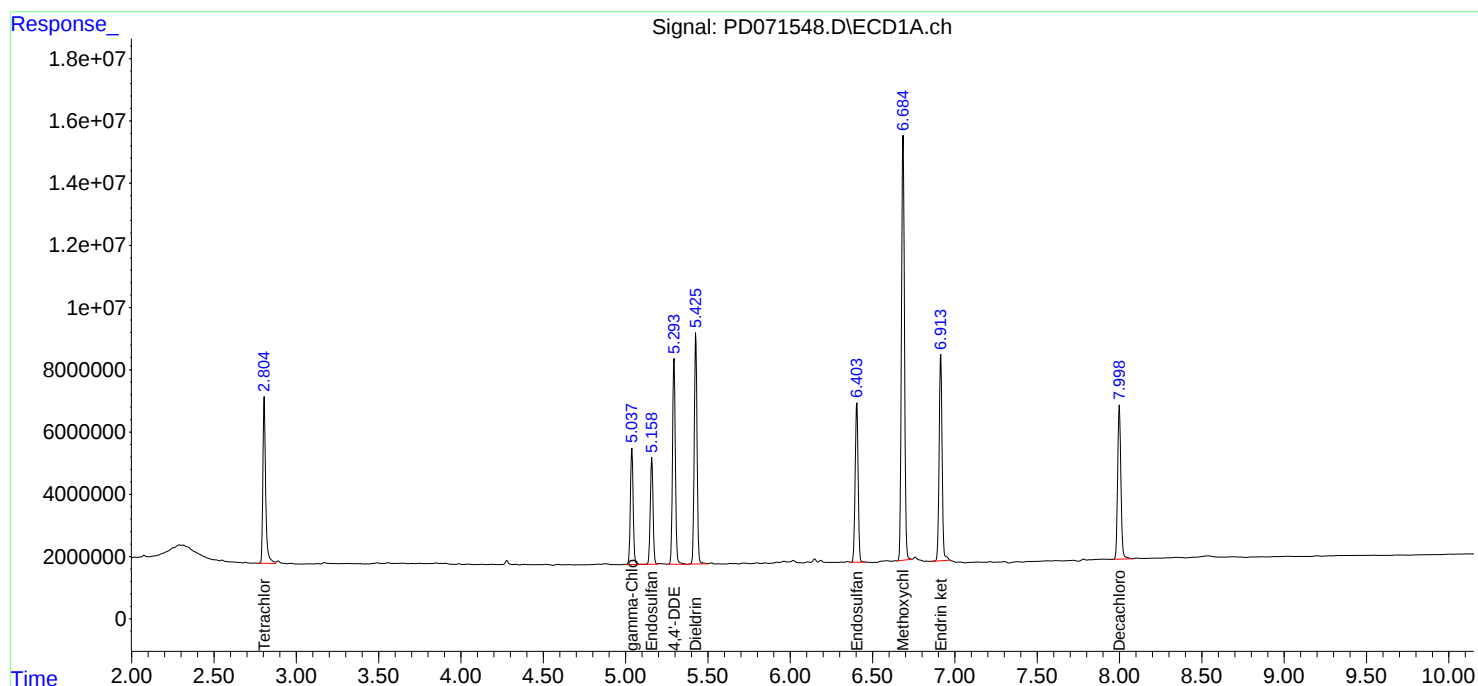


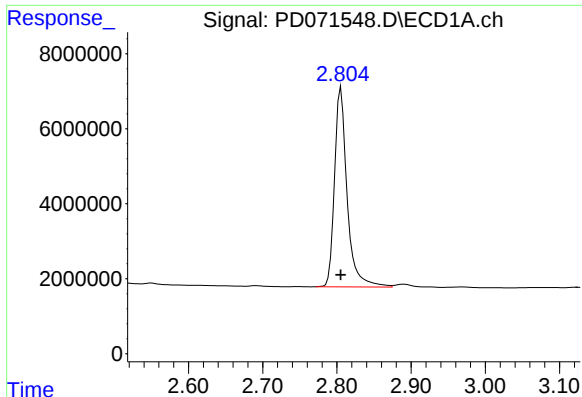

#1 Tetrachloro-m-xylene


R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 62954934
Conc: 23.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

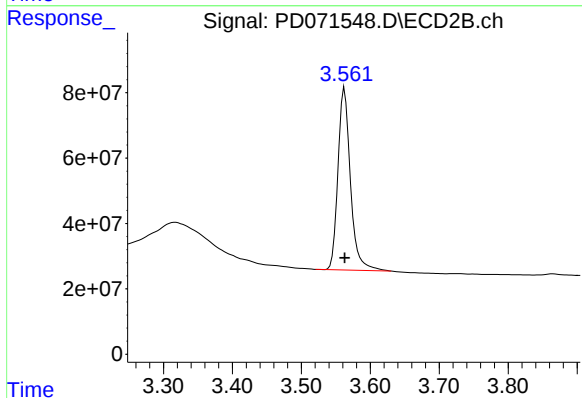


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 701418813
Conc: 23.93 ng/ml

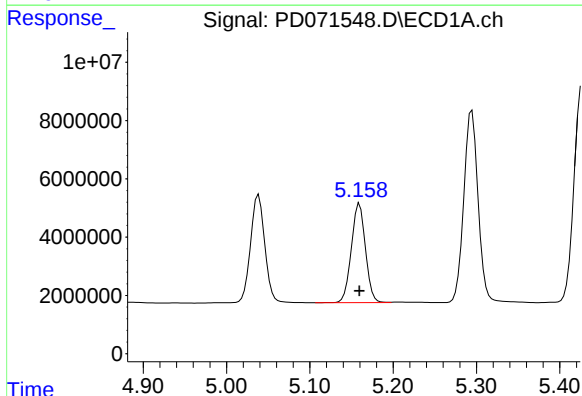


#9 Endosulfan I

R.T.: 5.160 min
Delta R.T.: 0.000 min
Response: 39925815
Conc: 11.55 ng/ml

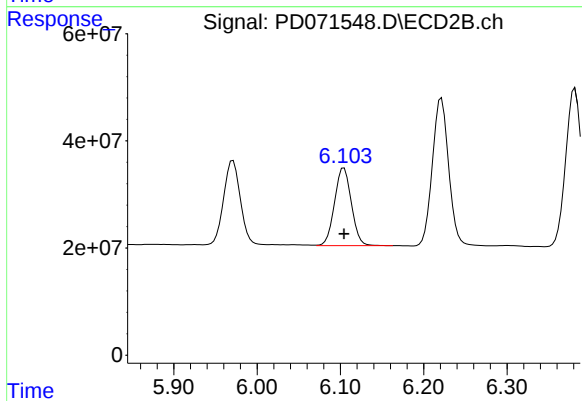

#9 Endosulfan I


R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 203560597
Conc: 13.09 ng/ml

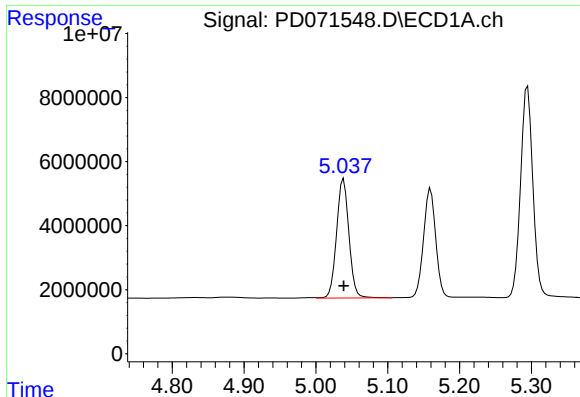

#10 gamma-Chlordane


R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 44329580
Conc: 11.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

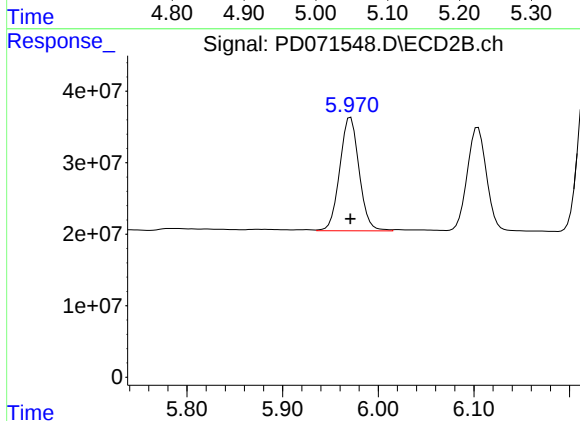


#10 gamma-Chlordane

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 223551227
Conc: 13.00 ng/ml

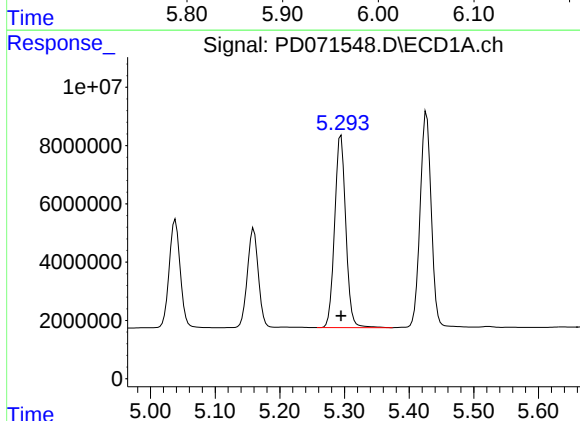


#12 4,4'-DDE

R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 79080652
Conc: 22.80 ng/ml

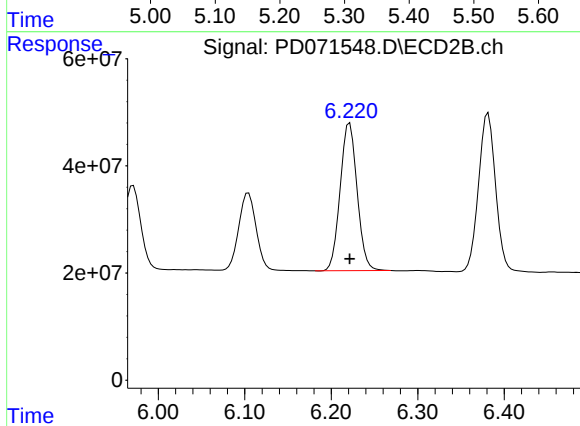

#12 4,4'-DDE


R.T.: 6.221 min
Delta R.T.: 0.000 min
Response: 373585190
Conc: 23.98 ng/ml

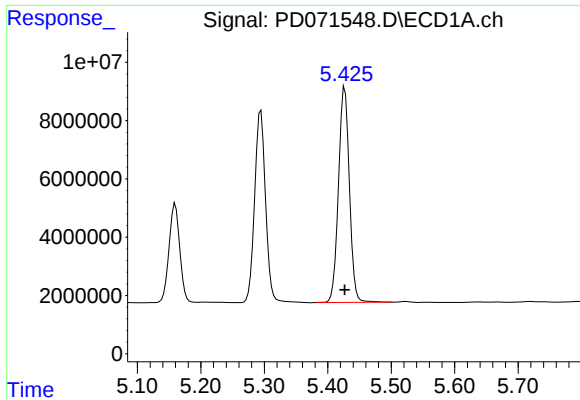

#13 Dieldrin


R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 88417380
Conc: 22.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

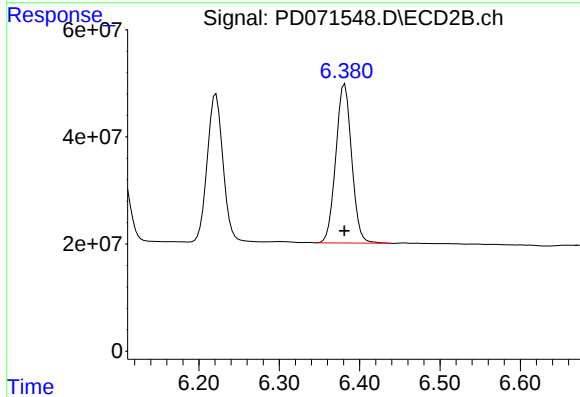


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 406847464
Conc: 23.93 ng/ml

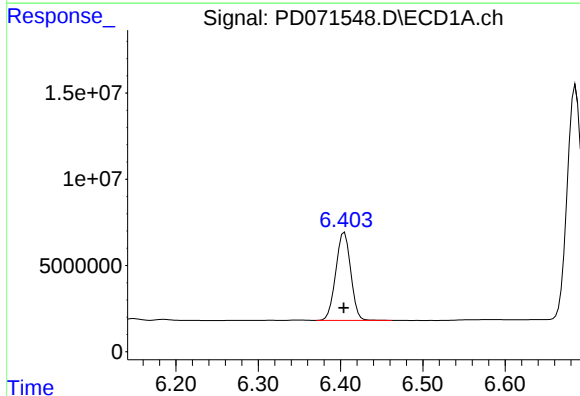


#19 Endosulfan Sulfate

R.T.: 6.405 min
Delta R.T.: 0.001 min
Response: 64400674
Conc: 21.13 ng/ml

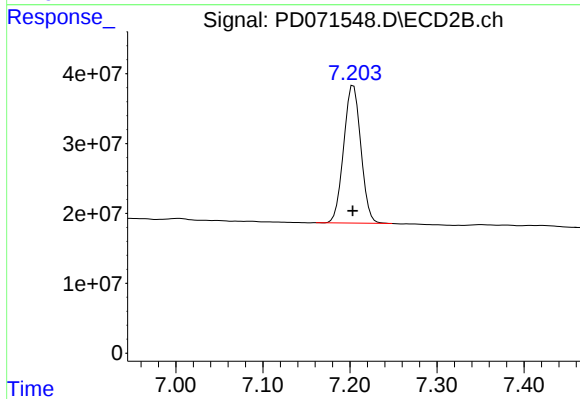

#19 Endosulfan Sulfate


R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 269778678
Conc: 22.01 ng/ml

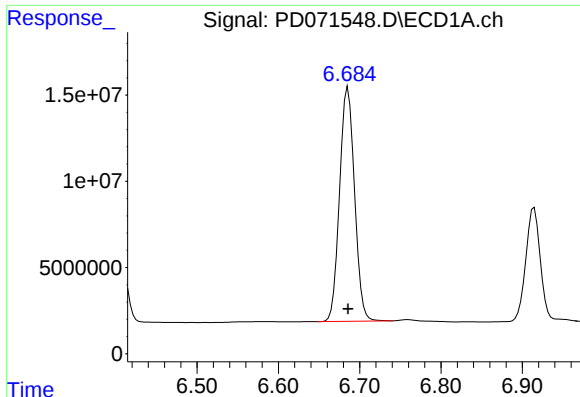

#20 Methoxychlor


R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 173218683
Conc: 109.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

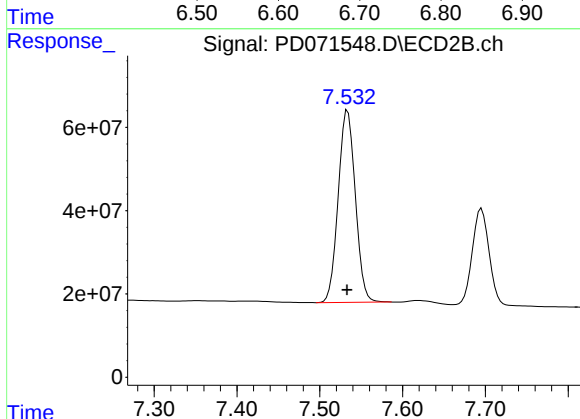


#20 Methoxychlor

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 663357934
Conc: 104.75 ng/ml

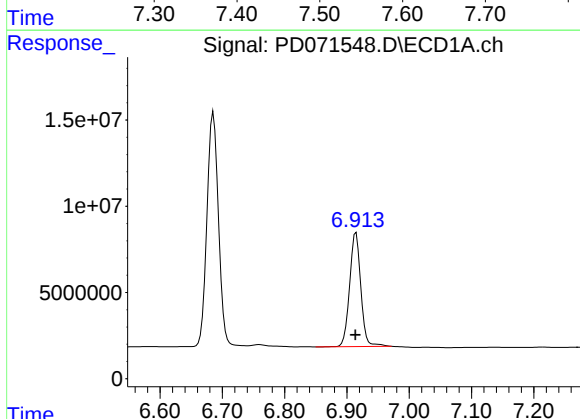


#21 Endrin ketone

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 83177807
Conc: 23.19 ng/ml

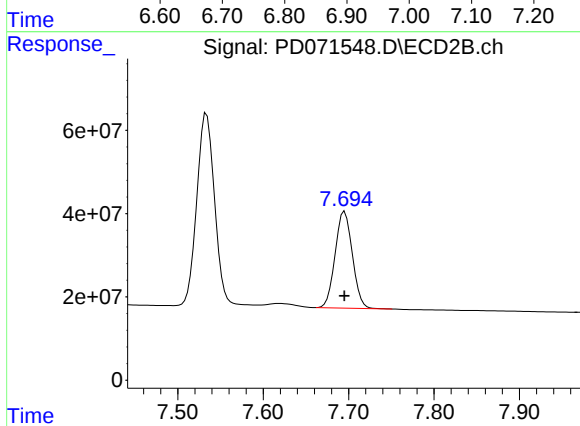

#21 Endrin ketone


R.T.: 7.695 min
Delta R.T.: 0.000 min
Response: 325279441
Conc: 24.27 ng/ml

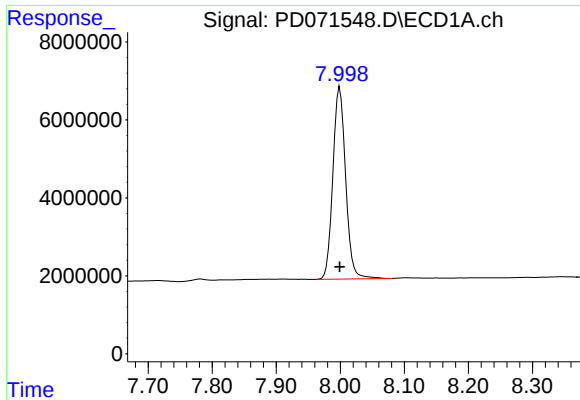

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 68412847
Conc: 23.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

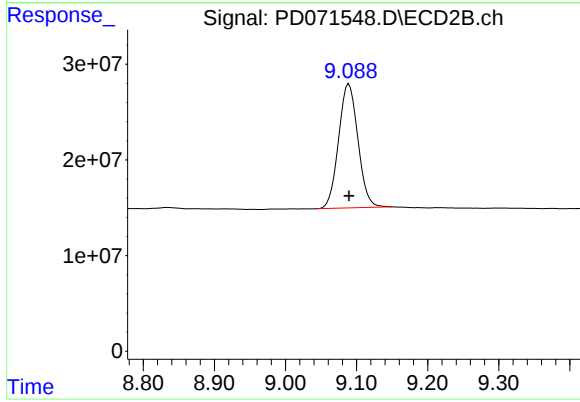

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 245522005
Conc: 24.06 ng/ml