

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
 Data File : PD071554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 19:00
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:50:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 03:50:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	353.9E6	2894.2E6	99.244	95.820
28)	SA Decachlor...	7.999	9.090	305.9E6	1006.4E6	97.818	95.964
Target Compounds							
23)	Chlordane-1	3.818	4.727	116.2E6	888.2E6	989.753	943.593
24)	Chlordane-2	4.401	5.259	129.3E6	642.5E6	966.444	939.773
25)	Chlordane-3	5.038	5.971	415.3E6	2275.3E6	1002.624	968.944
26)	Chlordane-4	5.103	6.049	379.0E6	2694.7E6	990.597	974.185
27)	Chlordane-5	6.006	6.911	143.9E6	465.6E6	994.555	921.595



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
Data File : PD071554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 19:00
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:50:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 03:50:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

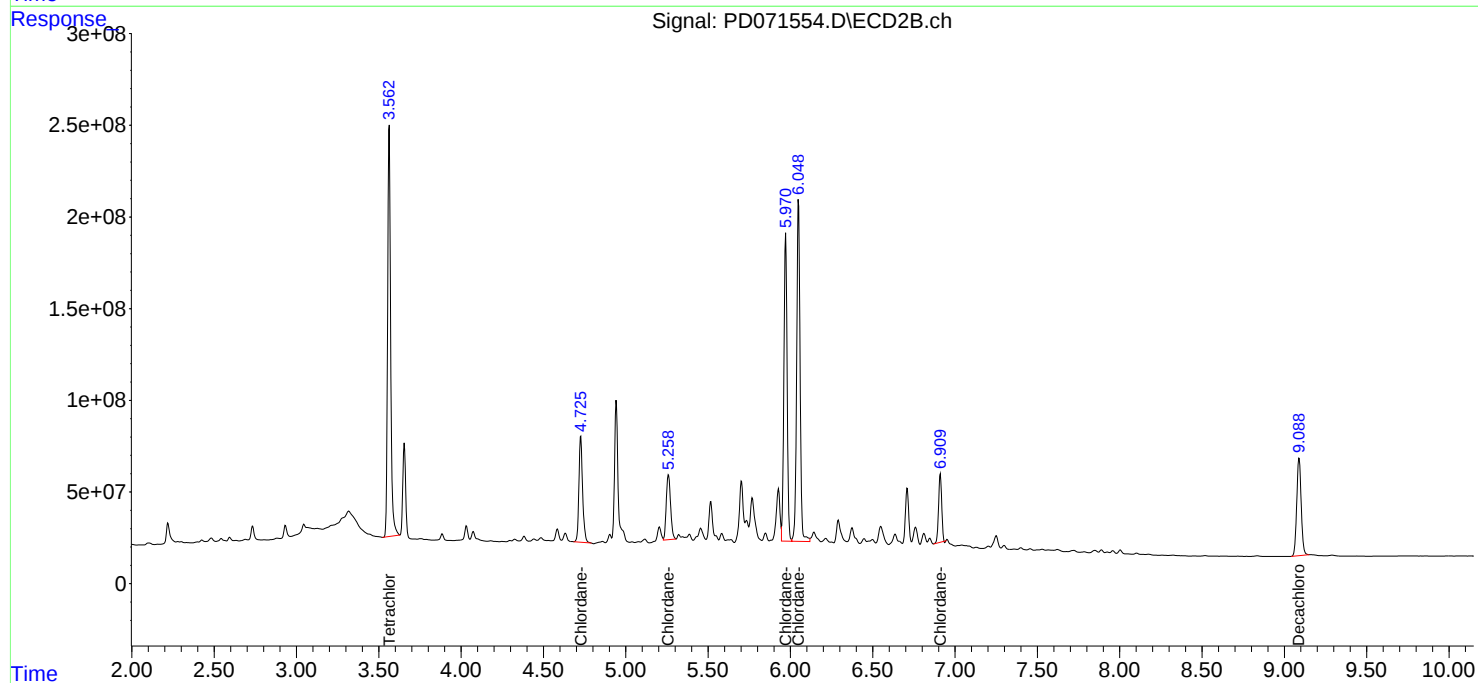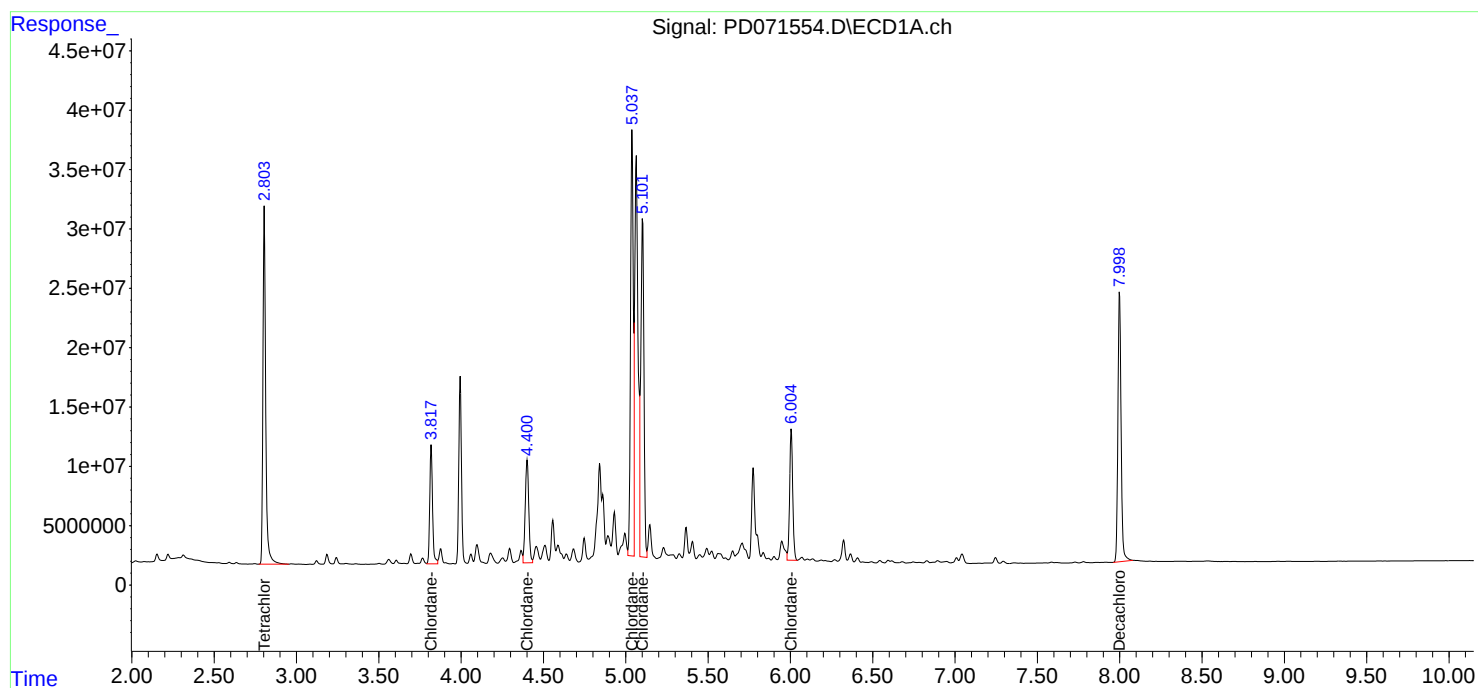


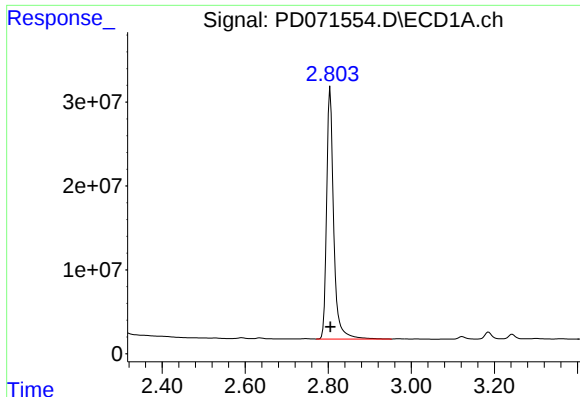

#1 Tetrachloro-m-xylene


R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 353871065
Conc: 99.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

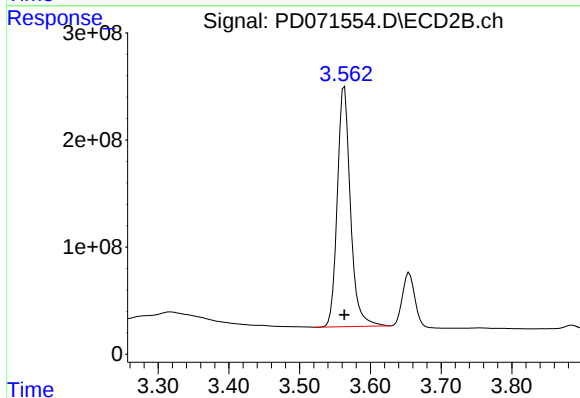


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 2894180661
Conc: 95.82 ng/ml

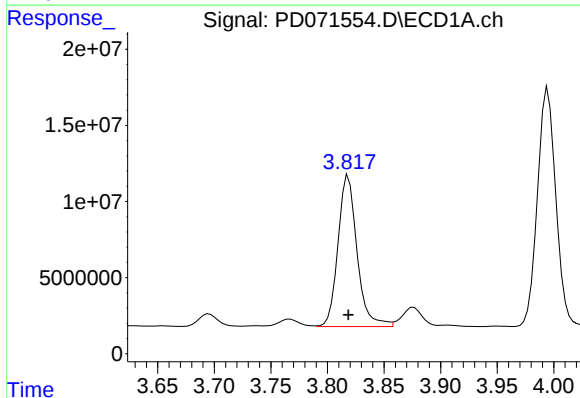


#23 Chlordane-1

R.T.: 3.818 min
Delta R.T.: 0.000 min
Response: 116222875
Conc: 989.75 ng/ml

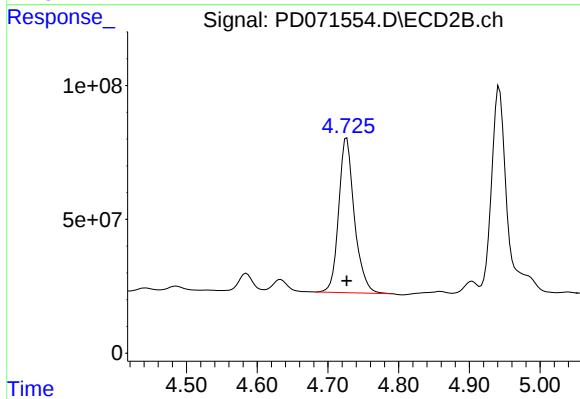

#23 Chlordane-1


R.T.: 4.727 min
Delta R.T.: 0.000 min
Response: 888160788
Conc: 943.59 ng/ml

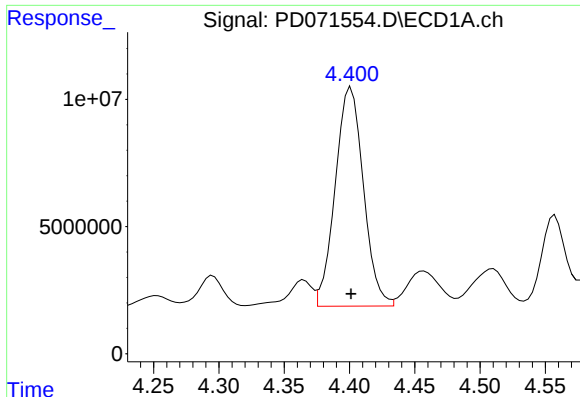

#24 Chlordane-2


R.T.: 4.401 min
Delta R.T.: 0.000 min
Response: 129288806
Conc: 966.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

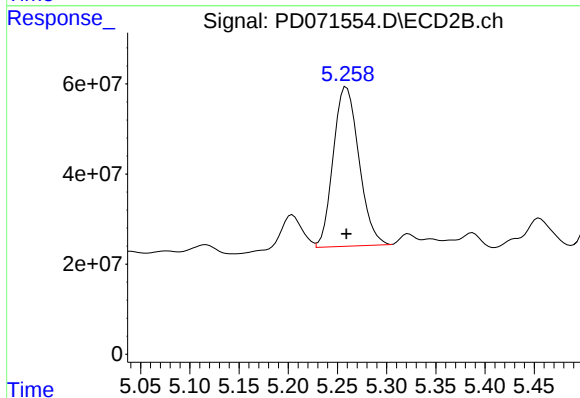


#24 Chlordane-2

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 642538353
Conc: 939.77 ng/ml

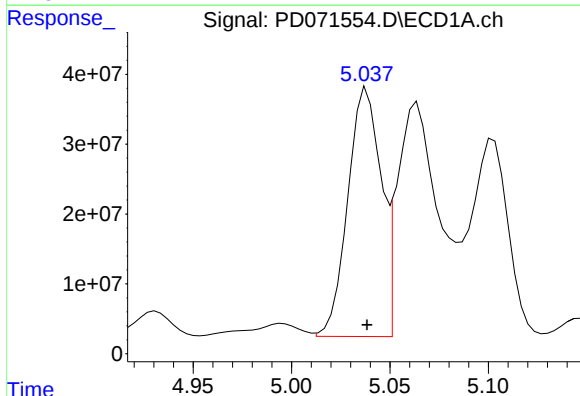


#25 Chlordane-3

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 415322544
Conc: 1002.62 ng/ml

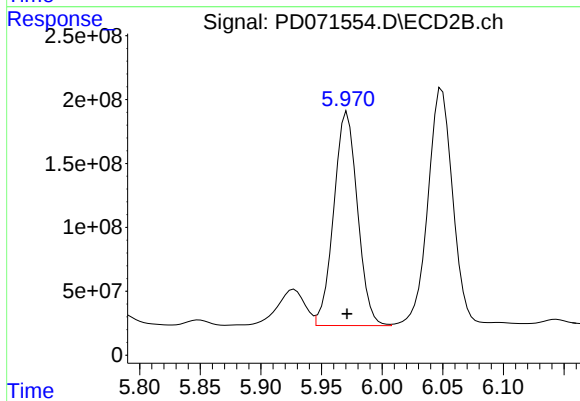

#25 Chlordane-3


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 2275322832
Conc: 968.94 ng/ml

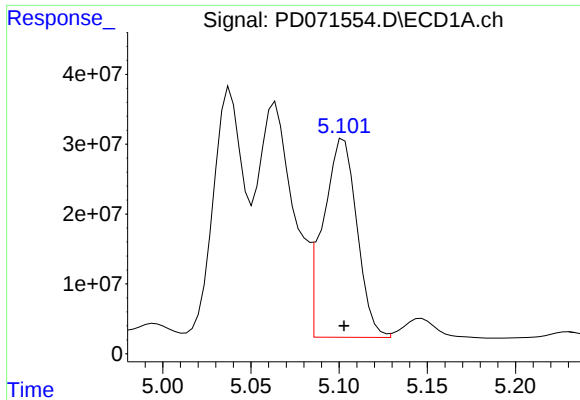

#26 Chlordane-4


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 379036372
Conc: 990.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

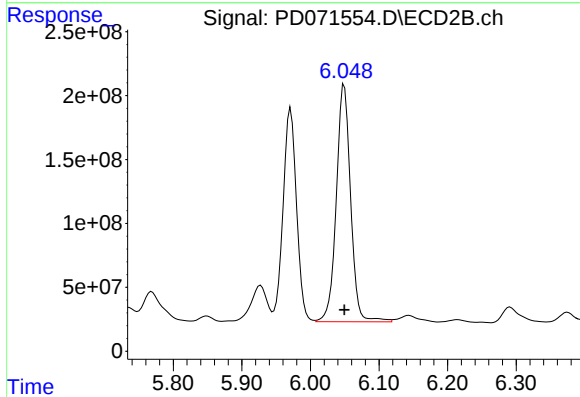


#26 Chlordane-4

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 2694731402
Conc: 974.18 ng/ml

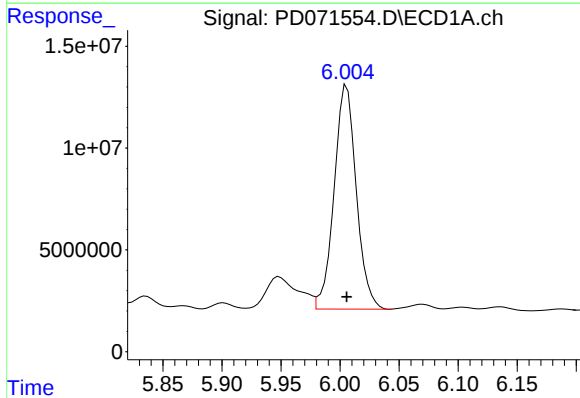


#27 Chlordane-5

R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 143866032
Conc: 994.56 ng/ml

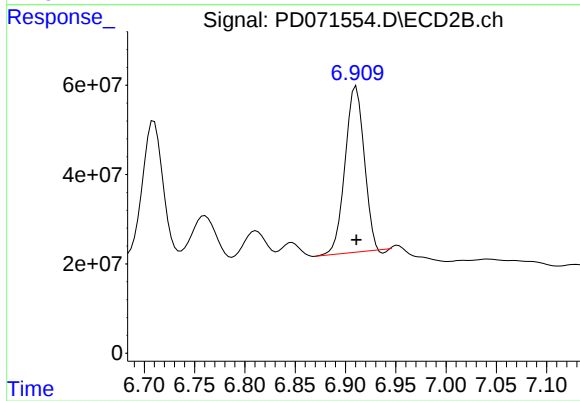

#27 Chlordane-5


R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 465577886
Conc: 921.60 ng/ml

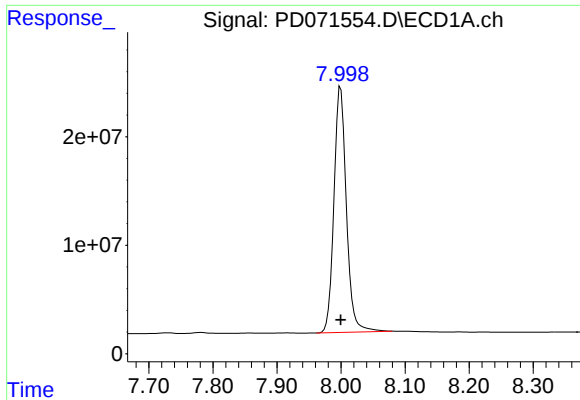

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 305936673
Conc: 97.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

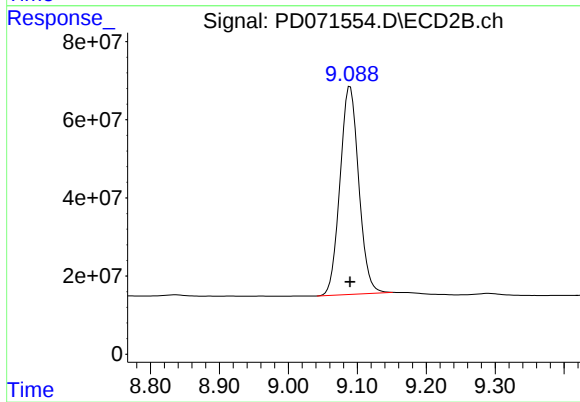

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 1006402944
Conc: 95.96 ng/ml