

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
 Data File : PD071555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 19:13
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:52:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 03:52:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	269.5E6	2245.0E6	75.380	74.550
28)	SA Decachlor...	7.999	9.090	233.9E6	780.5E6	74.867	74.616
Target Compounds							
23)	Chlordane-1	3.819	4.726	88401110	695.4E6	751.880	742.487
24)	Chlordane-2	4.402	5.259	100.1E6	508.1E6	748.858	745.432
25)	Chlordane-3	5.039	5.971	312.0E6	1757.7E6	752.179	748.997
26)	Chlordane-4	5.103	6.049	292.8E6	2060.6E6	760.045	746.625
27)	Chlordane-5	6.006	6.910	108.3E6	392.1E6	749.117	767.213



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
Data File : PD071555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 19:13
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:52:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 03:52:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

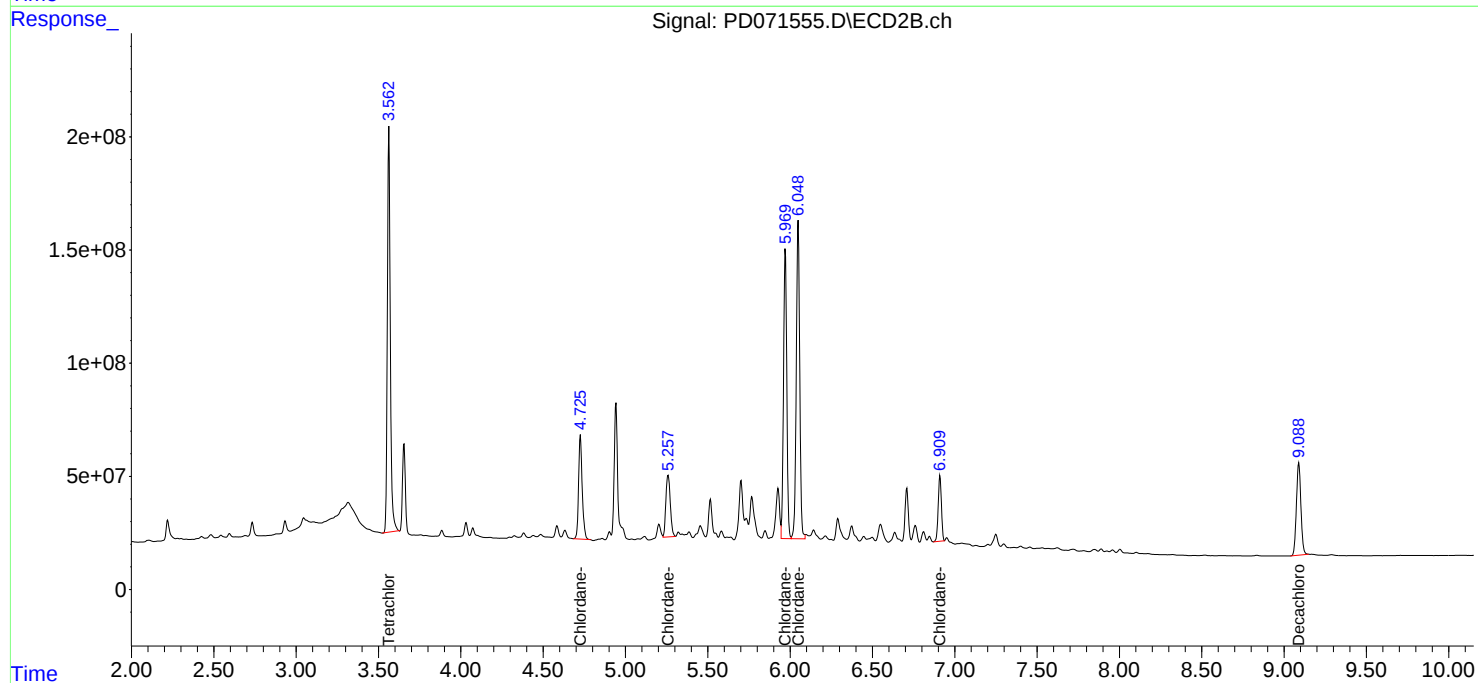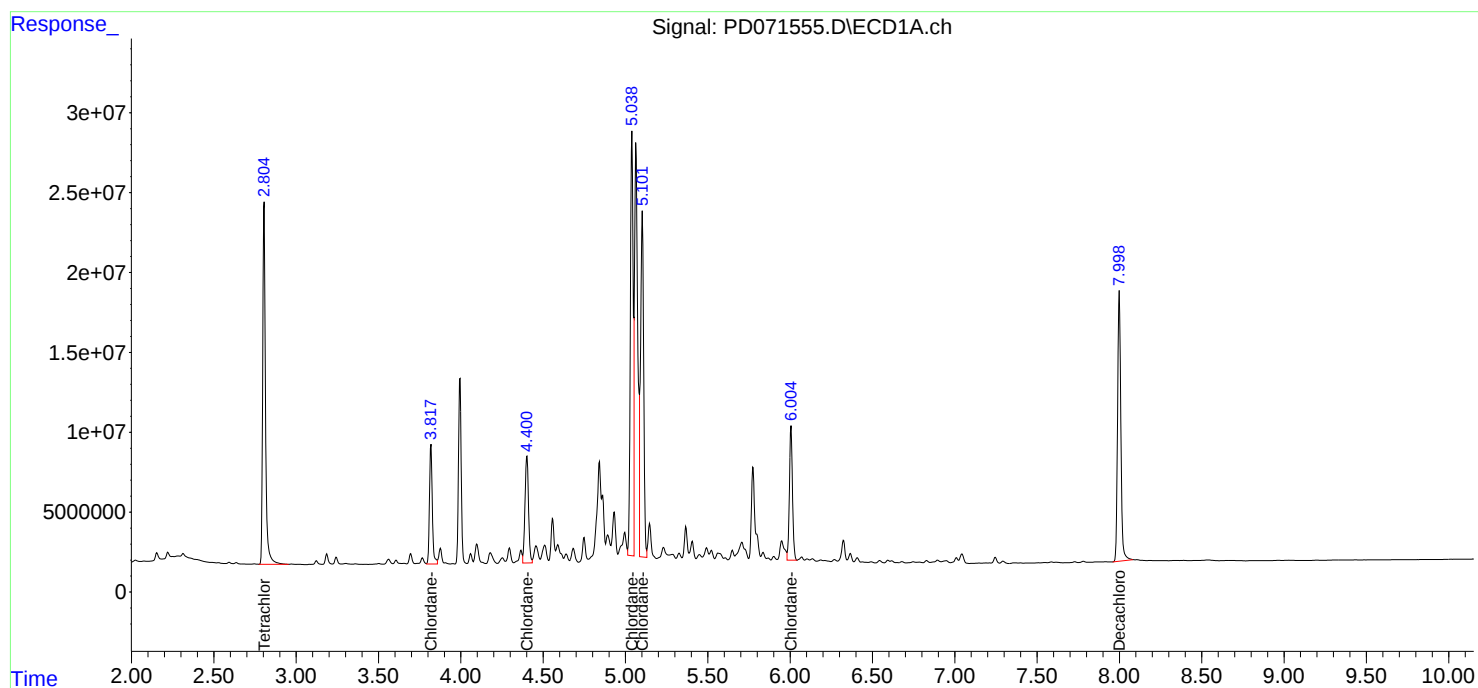


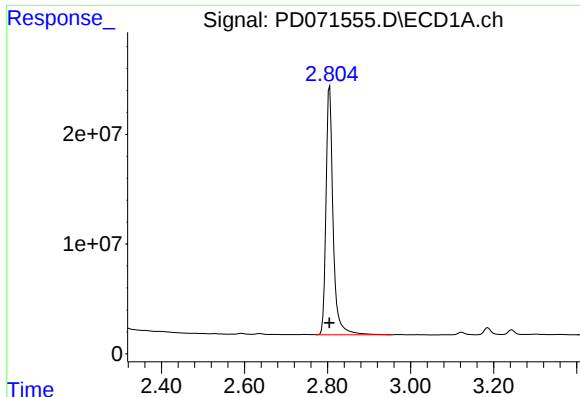

#1 Tetrachloro-m-xylene


R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 269461176
Conc: 75.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

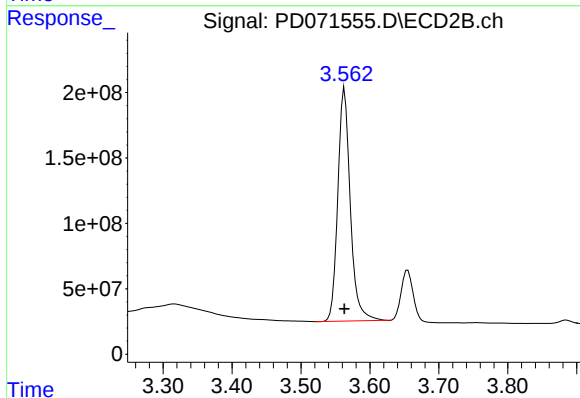


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 2245015088
Conc: 74.55 ng/ml

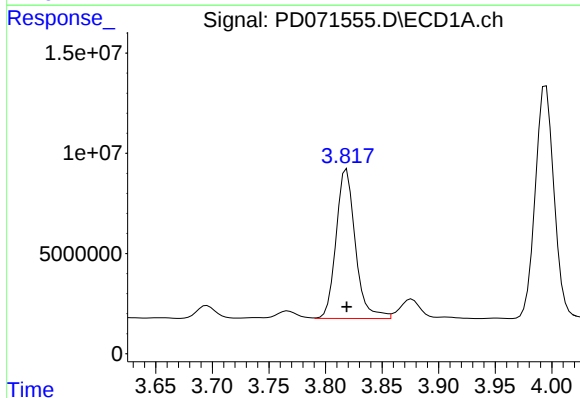


#23 Chlordane-1

R.T.: 3.819 min
Delta R.T.: 0.000 min
Response: 88401110
Conc: 751.88 ng/ml

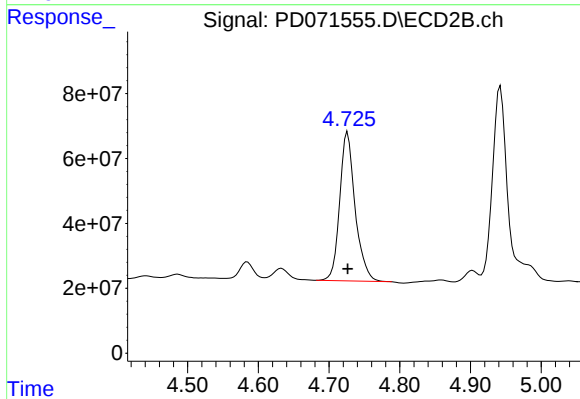

#23 Chlordane-1


R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 695386295
Conc: 742.49 ng/ml

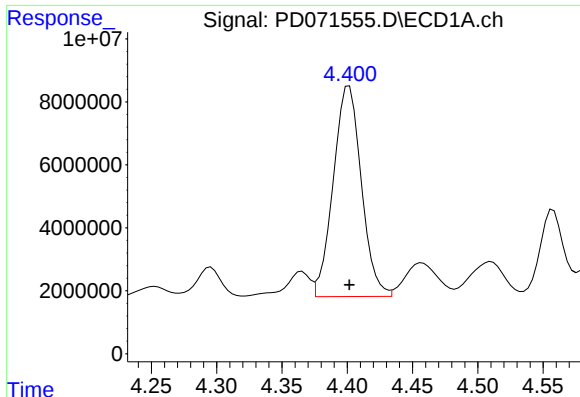

#24 Chlordane-2


R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 100104432
Conc: 748.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

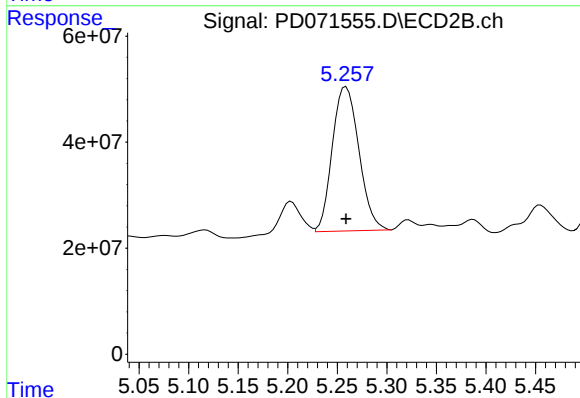


#24 Chlordane-2

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 508116765
Conc: 745.43 ng/ml

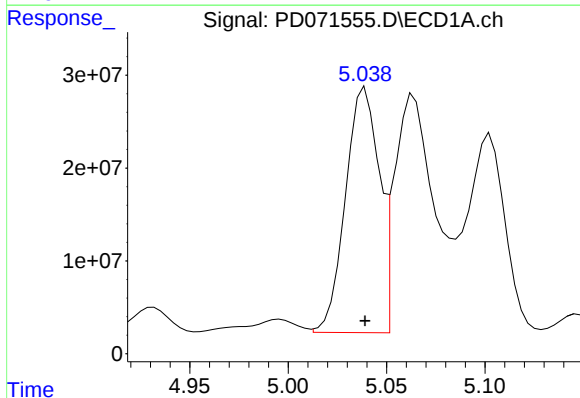


#25 Chlordane-3

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 312032576
Conc: 752.18 ng/ml

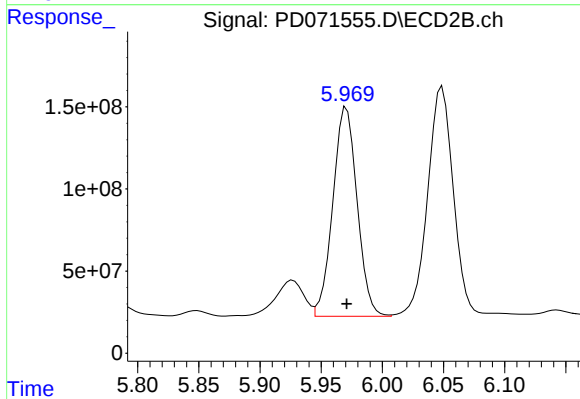

#25 Chlordane-3


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 1757654498
Conc: 749.00 ng/ml

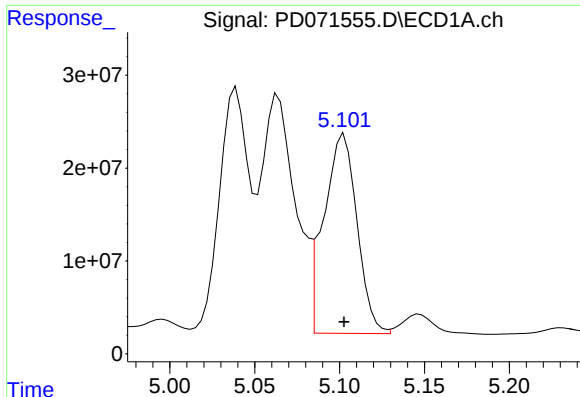

#26 Chlordane-4


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 292779833
Conc: 760.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

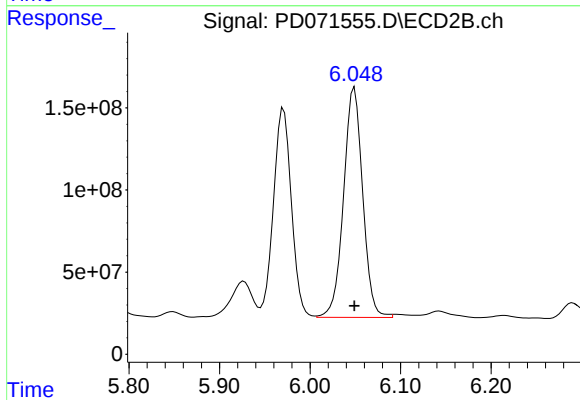


#26 Chlordane-4

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 2060631318
Conc: 746.62 ng/ml

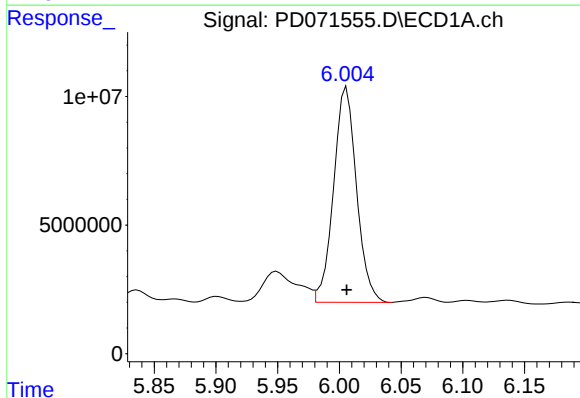


#27 Chlordane-5

R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 108298710
Conc: 749.12 ng/ml

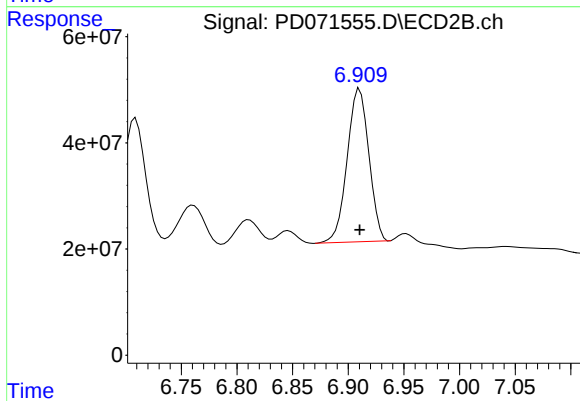

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 392084988
Conc: 767.21 ng/ml

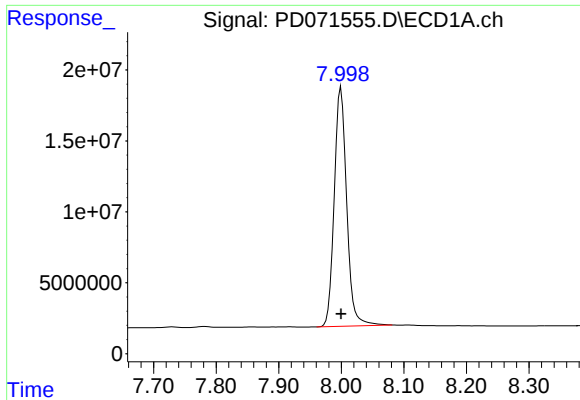

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 233948458
Conc: 74.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

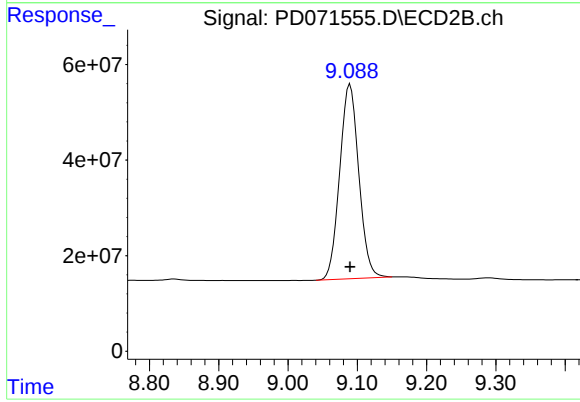

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 780522608
Conc: 74.62 ng/ml