

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
 Data File : PD071556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 19:27
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:48:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 03:47:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	179.6E6	1573.3E6	50.000	50.000
28)	SA Decachlor...	7.999	9.089	159.8E6	545.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.818	4.726	59314717	497.2E6	500.000	500.000
24)	Chlordane-2	4.401	5.259	69133508	362.4E6	500.000	500.000
25)	Chlordane-3	5.039	5.971	206.6E6	1210.6E6	500.000	500.000
26)	Chlordane-4	5.103	6.049	193.1E6	1418.8E6	500.000	500.000
27)	Chlordane-5	6.006	6.911	72720611	272.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
Data File : PD071556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 19:27
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:48:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 03:47:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

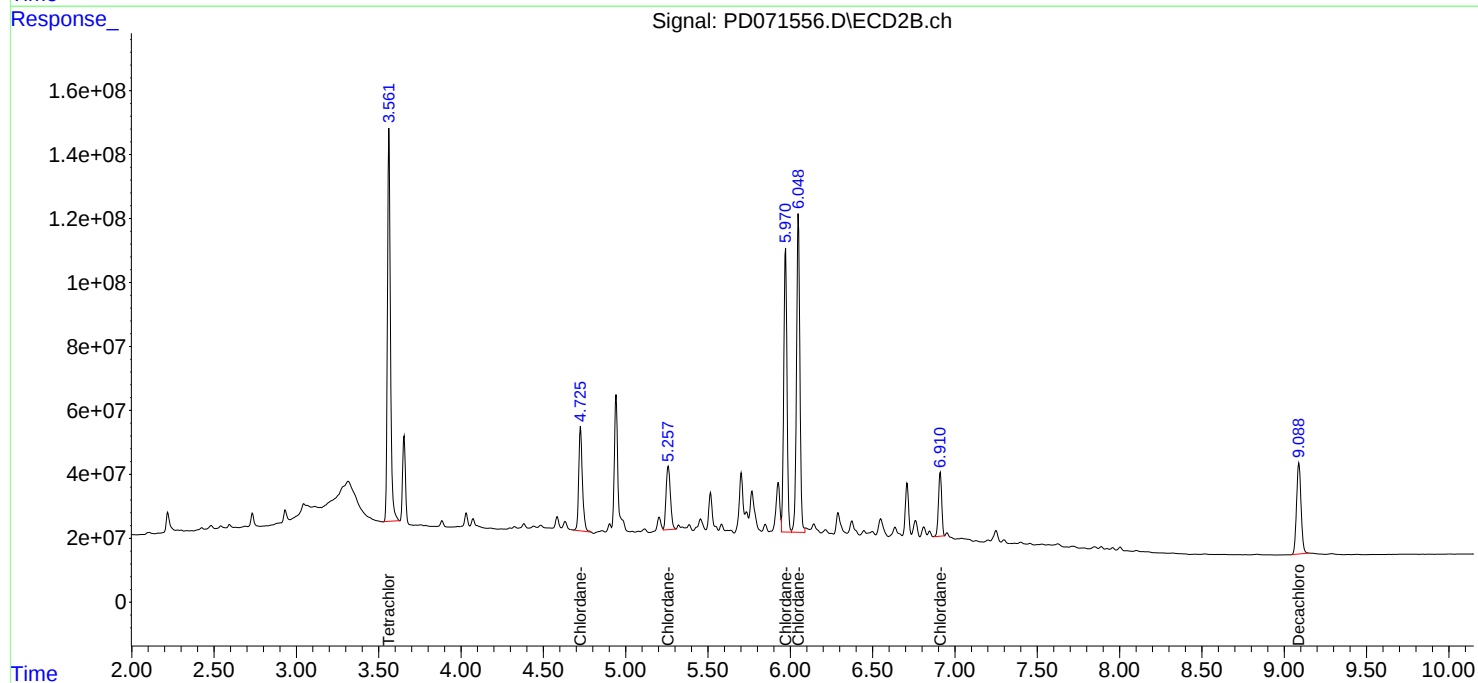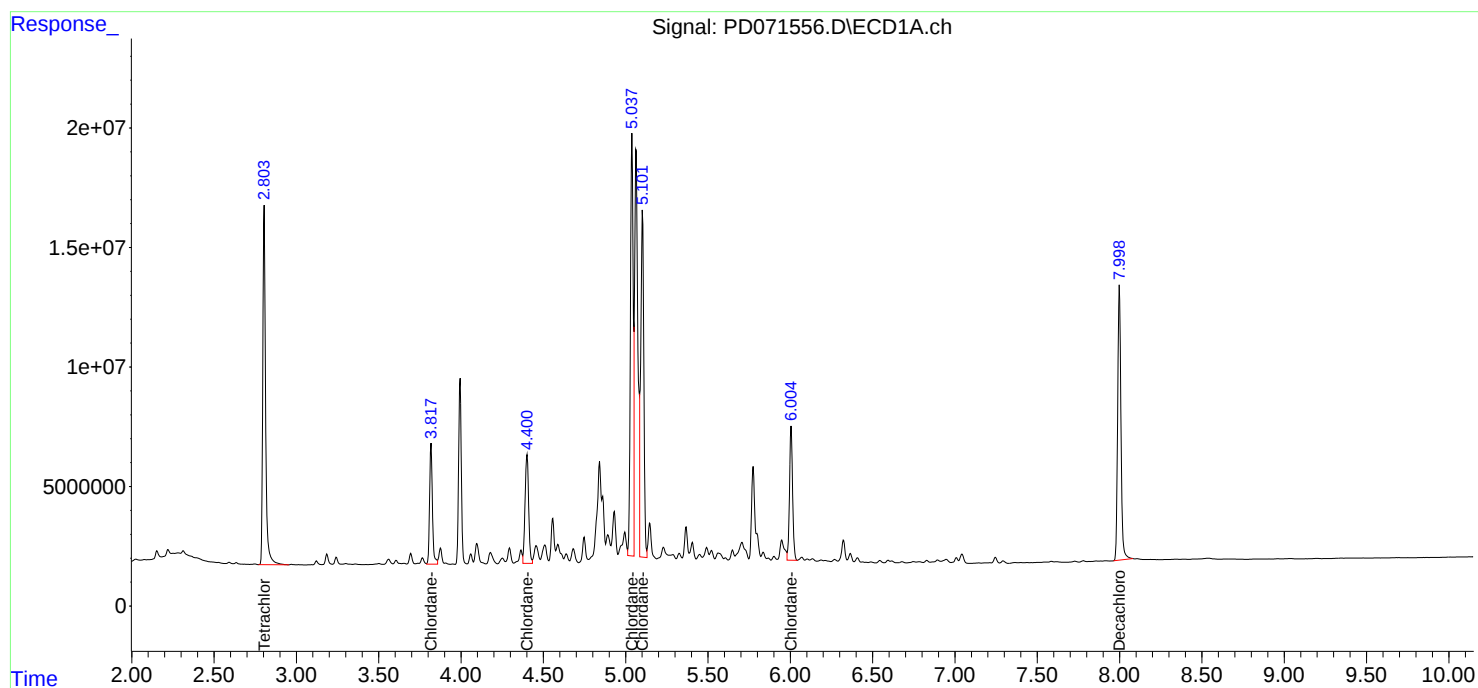


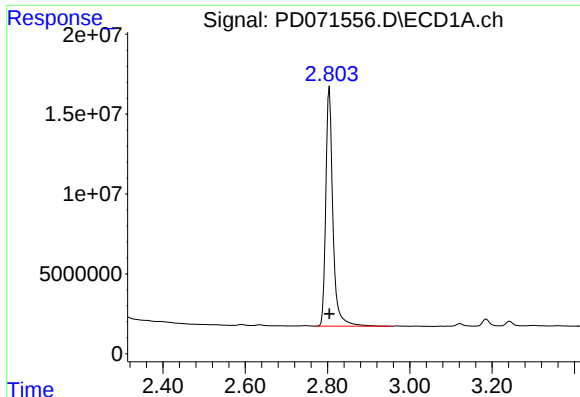

#1 Tetrachloro-m-xylene


R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 179629717
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

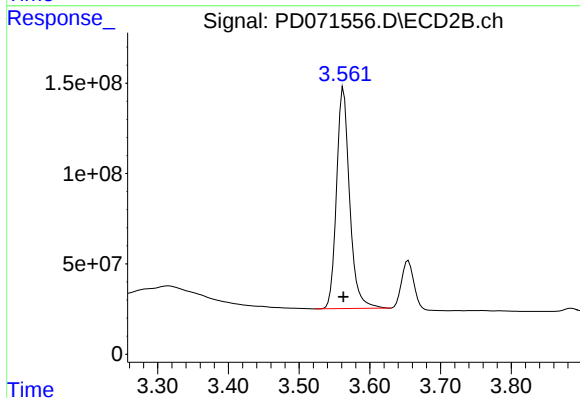


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 1573336630
Conc: 50.00 ng/ml

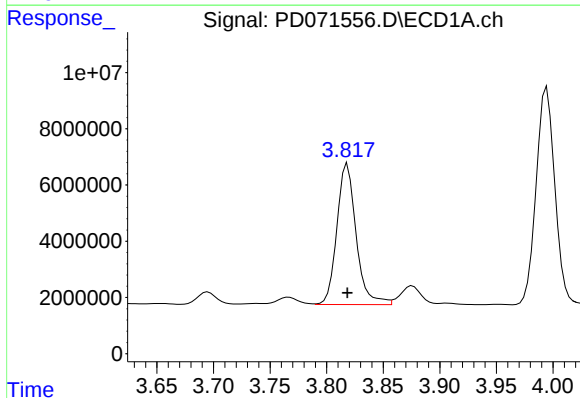


#23 Chlordane-1

R.T.: 3.818 min
Delta R.T.: 0.000 min
Response: 59314717
Conc: 500.00 ng/ml

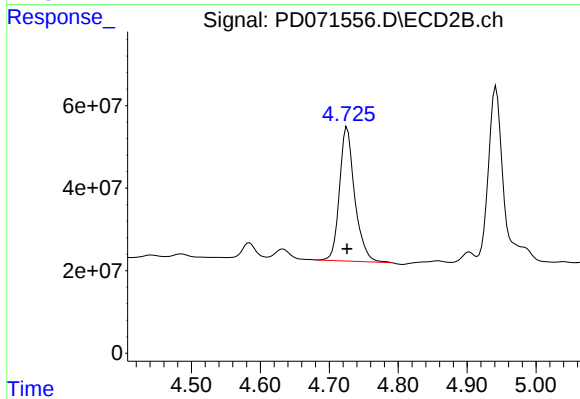

#23 Chlordane-1


R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 497174124
Conc: 500.00 ng/ml

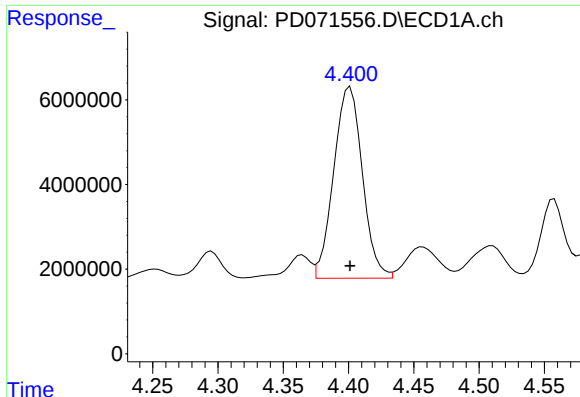

#24 Chlordane-2


R.T.: 4.401 min
Delta R.T.: 0.000 min
Response: 69133508
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

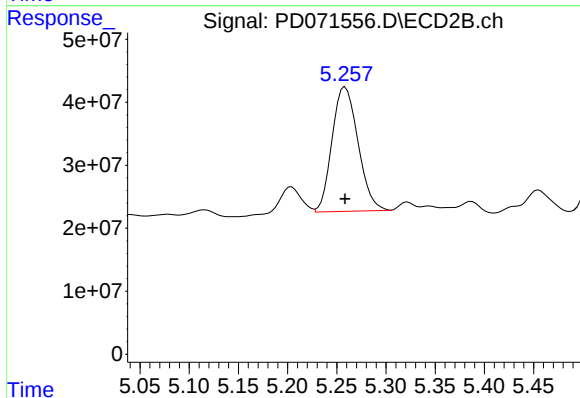


#24 Chlordane-2

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 362447346
Conc: 500.00 ng/ml

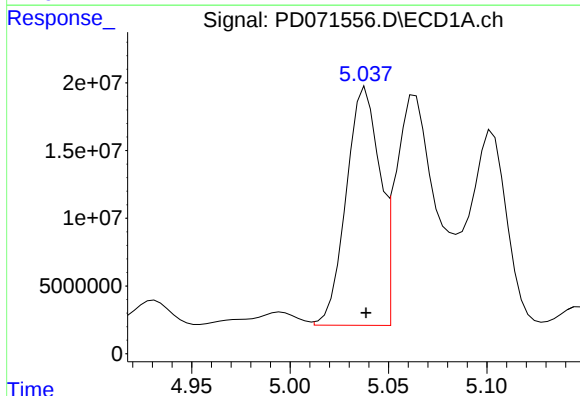


#25 Chlordane-3

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 206574337
Conc: 500.00 ng/ml

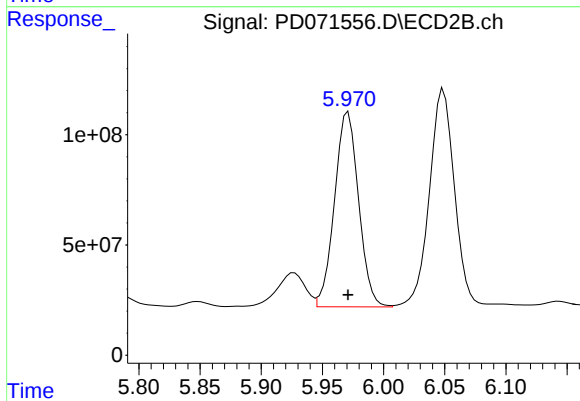

#25 Chlordane-3


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 1210587484
Conc: 500.00 ng/ml

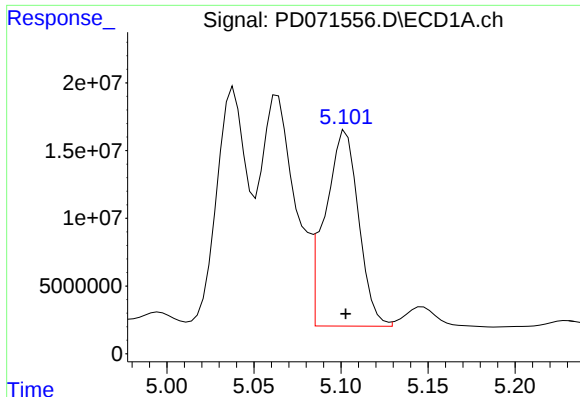

#26 Chlordane-4


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 193115918
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

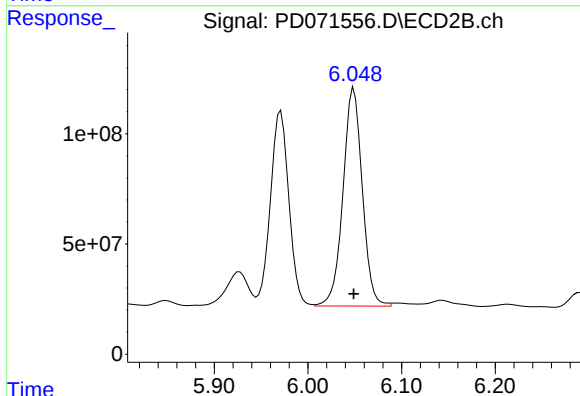


#26 Chlordane-4

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 1418774114
Conc: 500.00 ng/ml

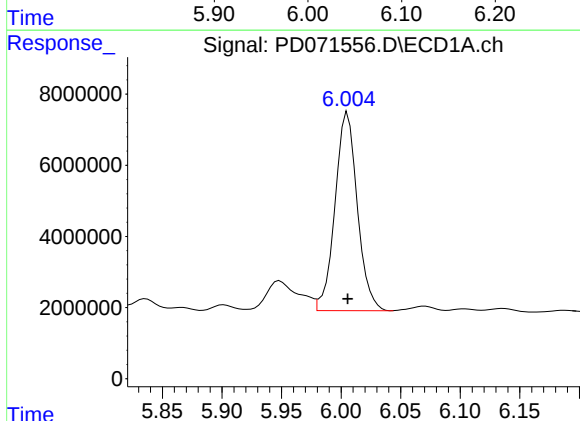


#27 Chlordane-5

R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 72720611
Conc: 500.00 ng/ml

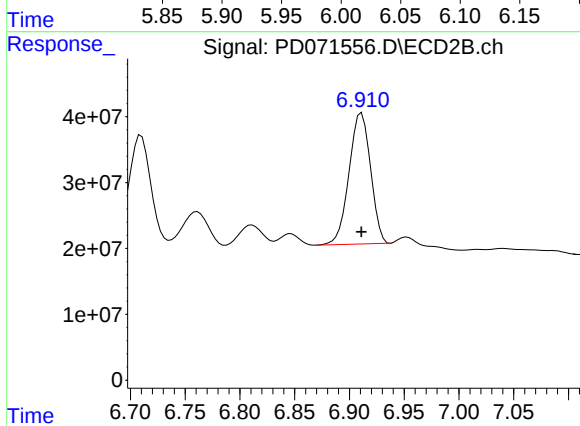

#27 Chlordane-5


R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 272397907
Conc: 500.00 ng/ml

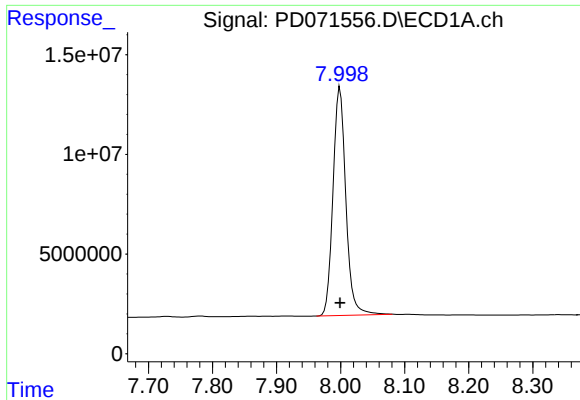

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 159793360
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

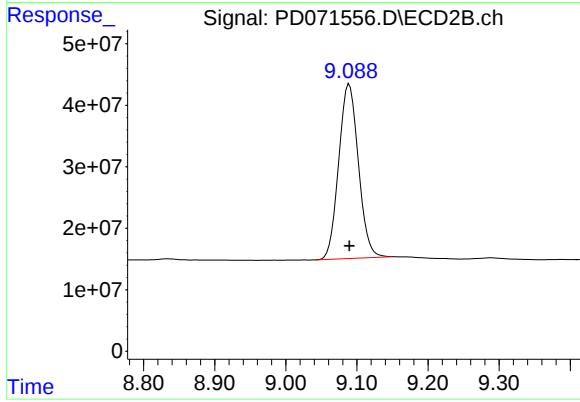

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 545527514
Conc: 50.00 ng/ml