

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
 Data File : PD071557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 19:40
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:55:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 03:55:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	86055816	812.9E6	24.299	26.466
28)	SA Decachlor...	7.999	9.089	80964959	284.8E6	25.676	26.636
Target Compounds							
23)	Chlordane-1	3.818	4.726	29166718	260.8E6	248.551	270.756
24)	Chlordane-2	4.401	5.259	35349211	193.9E6	260.675	274.984
25)	Chlordane-3	5.039	5.971	98186933	621.2E6	239.881	260.869
26)	Chlordane-4	5.102	6.049	91186363	729.5E6	239.903	260.587
27)	Chlordane-5	6.005	6.910	35103611	138.1E6	244.573	264.916



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081522\
Data File : PD071557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 19:40
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:55:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 03:55:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

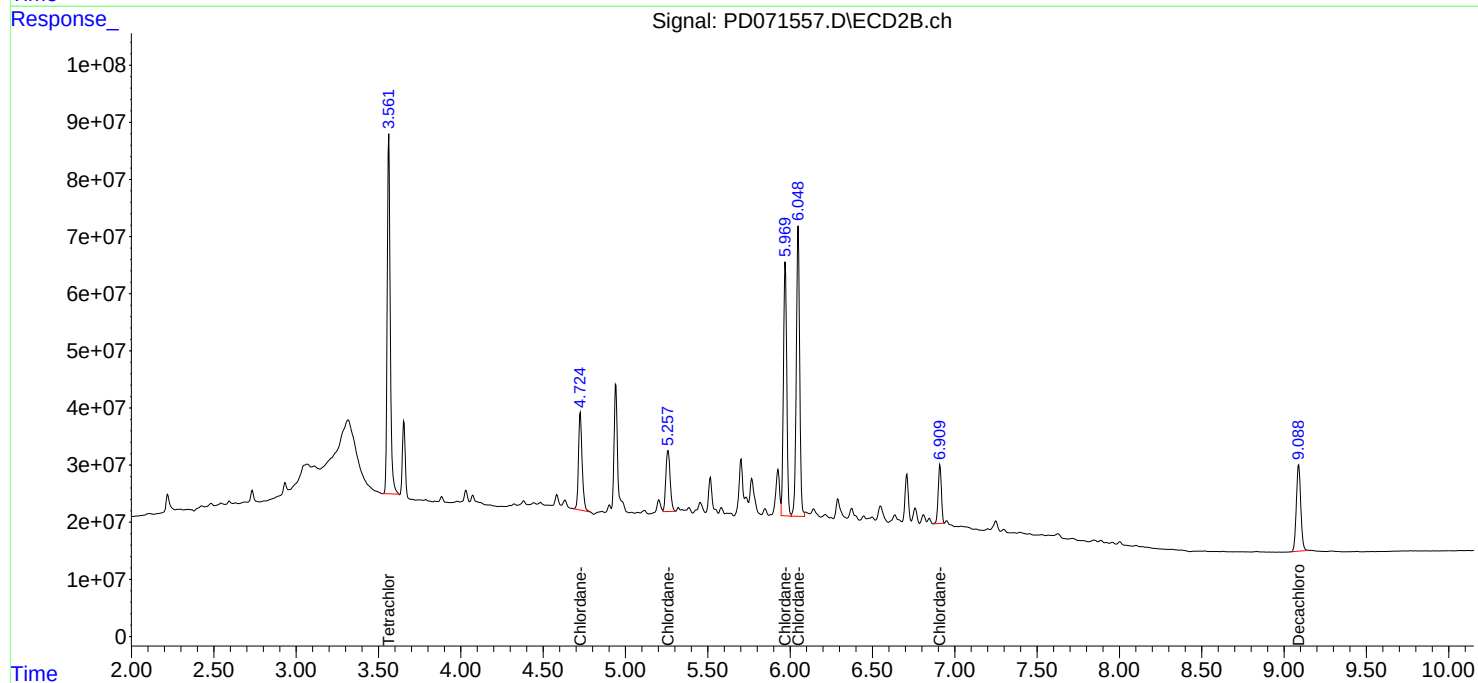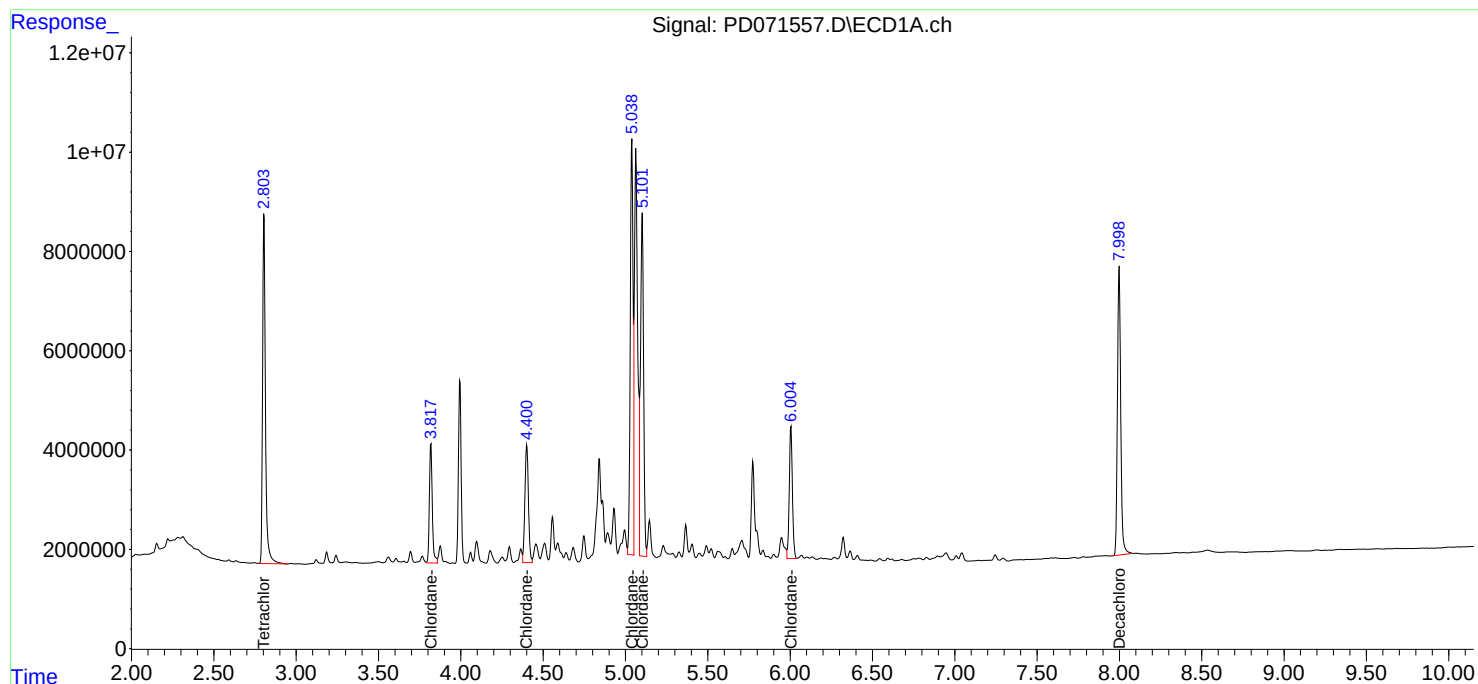


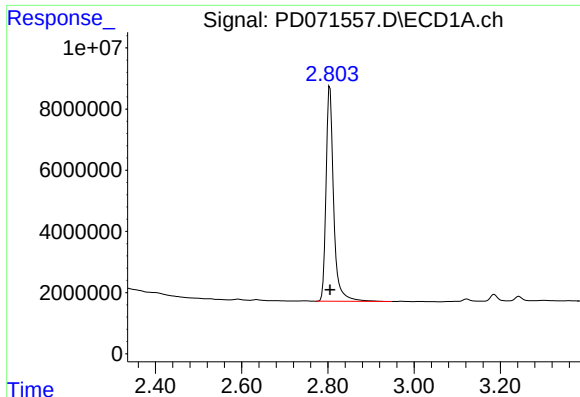

#1 Tetrachloro-m-xylene


R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 86055816
Conc: 24.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

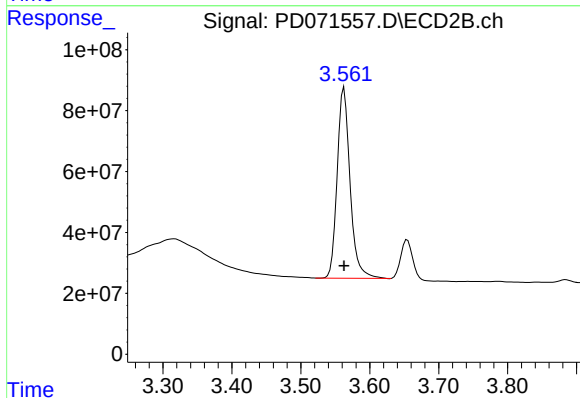


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 812885412
Conc: 26.47 ng/ml

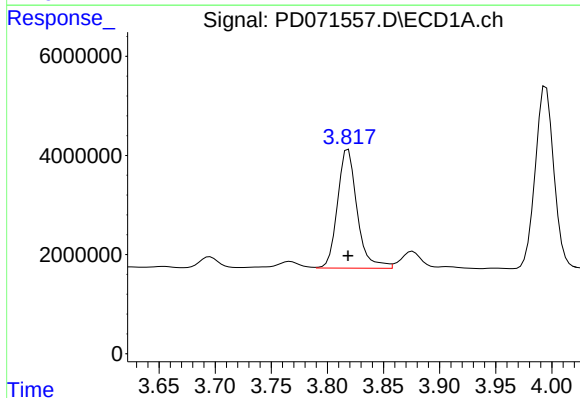


#23 Chlordane-1

R.T.: 3.818 min
Delta R.T.: 0.000 min
Response: 29166718
Conc: 248.55 ng/ml

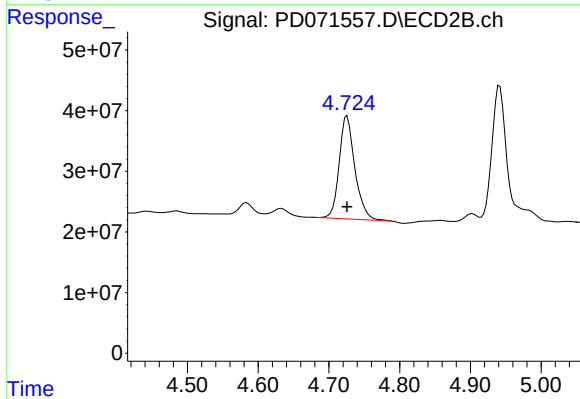

#23 Chlordane-1


R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 260797459
Conc: 270.76 ng/ml

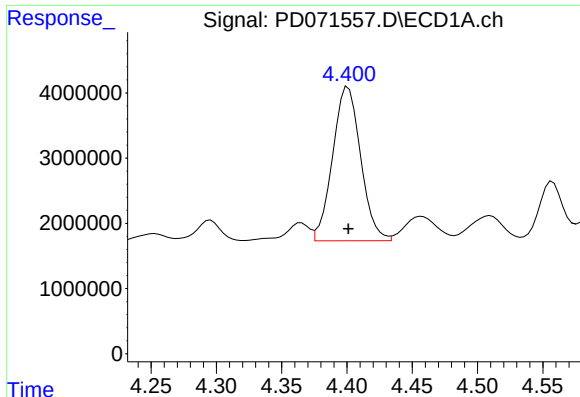

#24 Chlordane-2


R.T.: 4.401 min
Delta R.T.: 0.000 min
Response: 35349211
Conc: 260.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

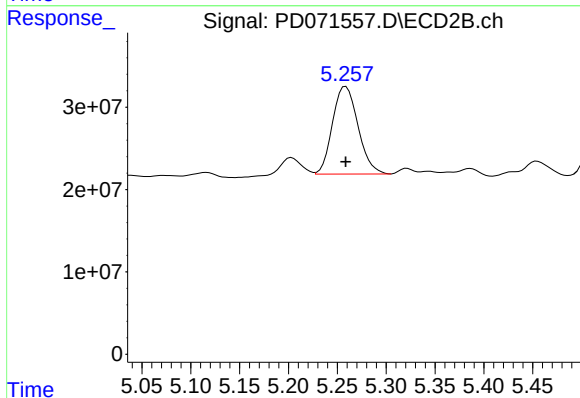


#24 Chlordane-2

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 193899281
Conc: 274.98 ng/ml

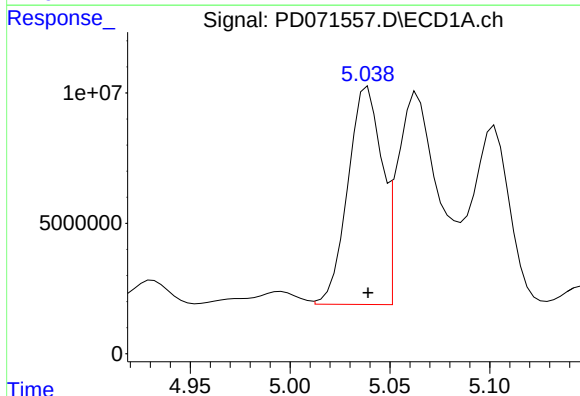


#25 Chlordane-3

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 98186933
Conc: 239.88 ng/ml

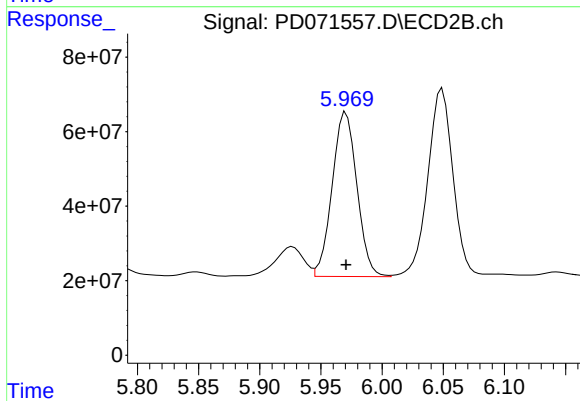

#25 Chlordane-3


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 621177686
Conc: 260.87 ng/ml

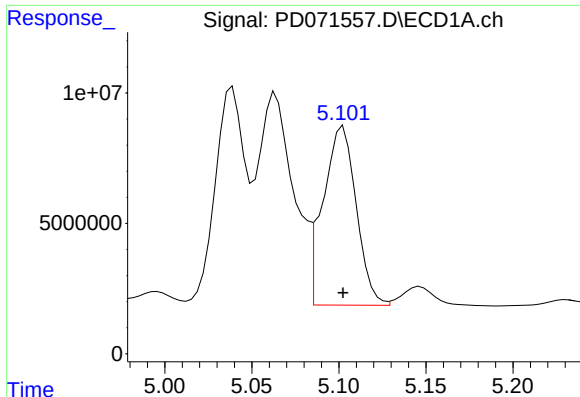

#26 Chlordane-4


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 91186363
Conc: 239.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

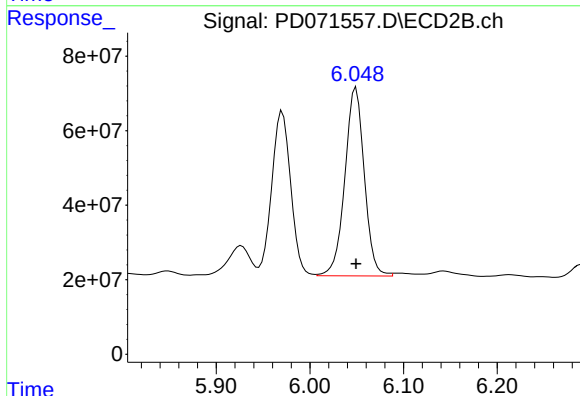


#26 Chlordane-4

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 729500518
Conc: 260.59 ng/ml

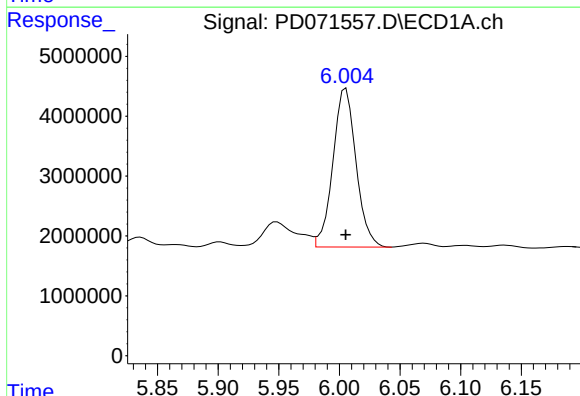


#27 Chlordane-5

R.T.: 6.005 min
Delta R.T.: 0.000 min
Response: 35103611
Conc: 244.57 ng/ml

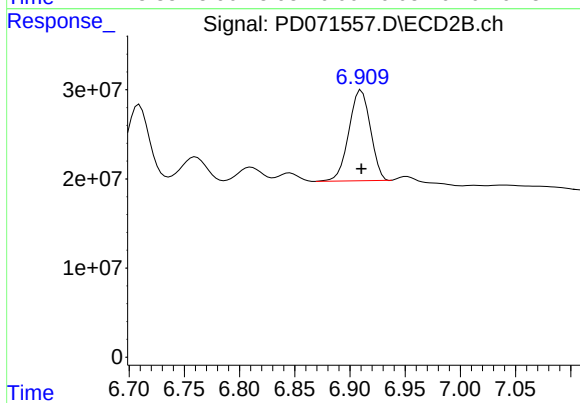

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 138133118
Conc: 264.92 ng/ml

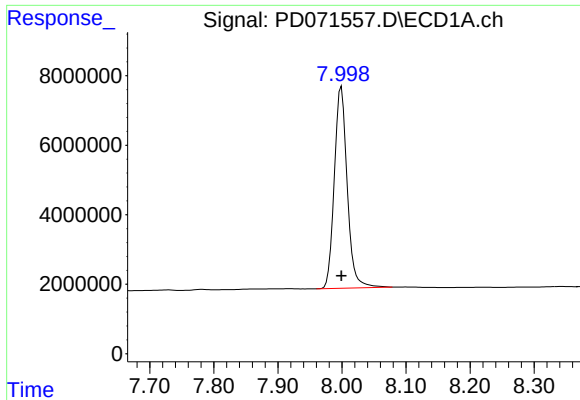

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 80964959
Conc: 25.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

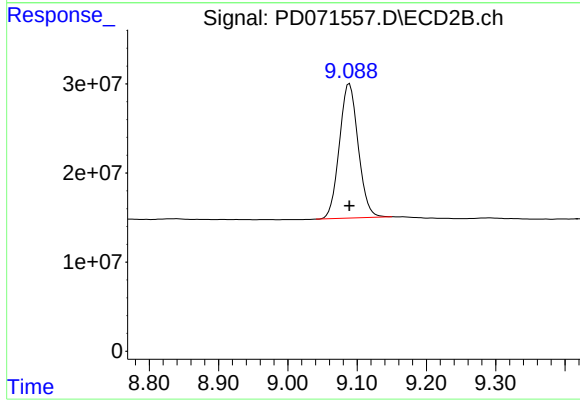

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 284833344
Conc: 26.64 ng/ml