

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081523\
 Data File : PD077192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2023 14:14
 Operator : AR\AJ
 Sample : PIBLK231
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:07:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.761	46100236	25917697	20.999	20.805
27)	SA Decachlor...	9.088	7.904	122.0E6	62070725	47.950	49.795
Target Compounds							
4)	MA Heptachlor	0.000	3.896f	0	245267	N.D.	0.142
5)	MB Aldrin	0.000	4.218	0	1273695	N.D.	0.736
6)	B beta-BHC	0.000	3.896	0	245267	N.D.	0.300
7)	B delta-BHC	4.769	0.000	5901187	0	1.780	N.D. #
8)	B Heptachlo...	5.690	4.739	3147241	454069	0.986	0.278 #
10)	B trans-Chl...	5.986	0.000	2150609	0	0.696	N.D. #
11)	B cis-Chlor...	5.986f	0.000	2150609	0	0.672	N.D. #
14)	MA Endrin	0.000	5.644	0	209591	N.D.	0.151
15)	B Endosulfa...	6.812	5.879f	2181923	87912	0.772	<MDL #
18)	B Endrin al...	0.000	6.114	0	506089	N.D.	0.466
23)	Toxaphene-2	0.000	5.644	0	209591	N.D.	23.958


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081523\
Data File : PD077192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2023 14:14
Operator : AR\AJ
Sample : PIBLK231
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:07:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

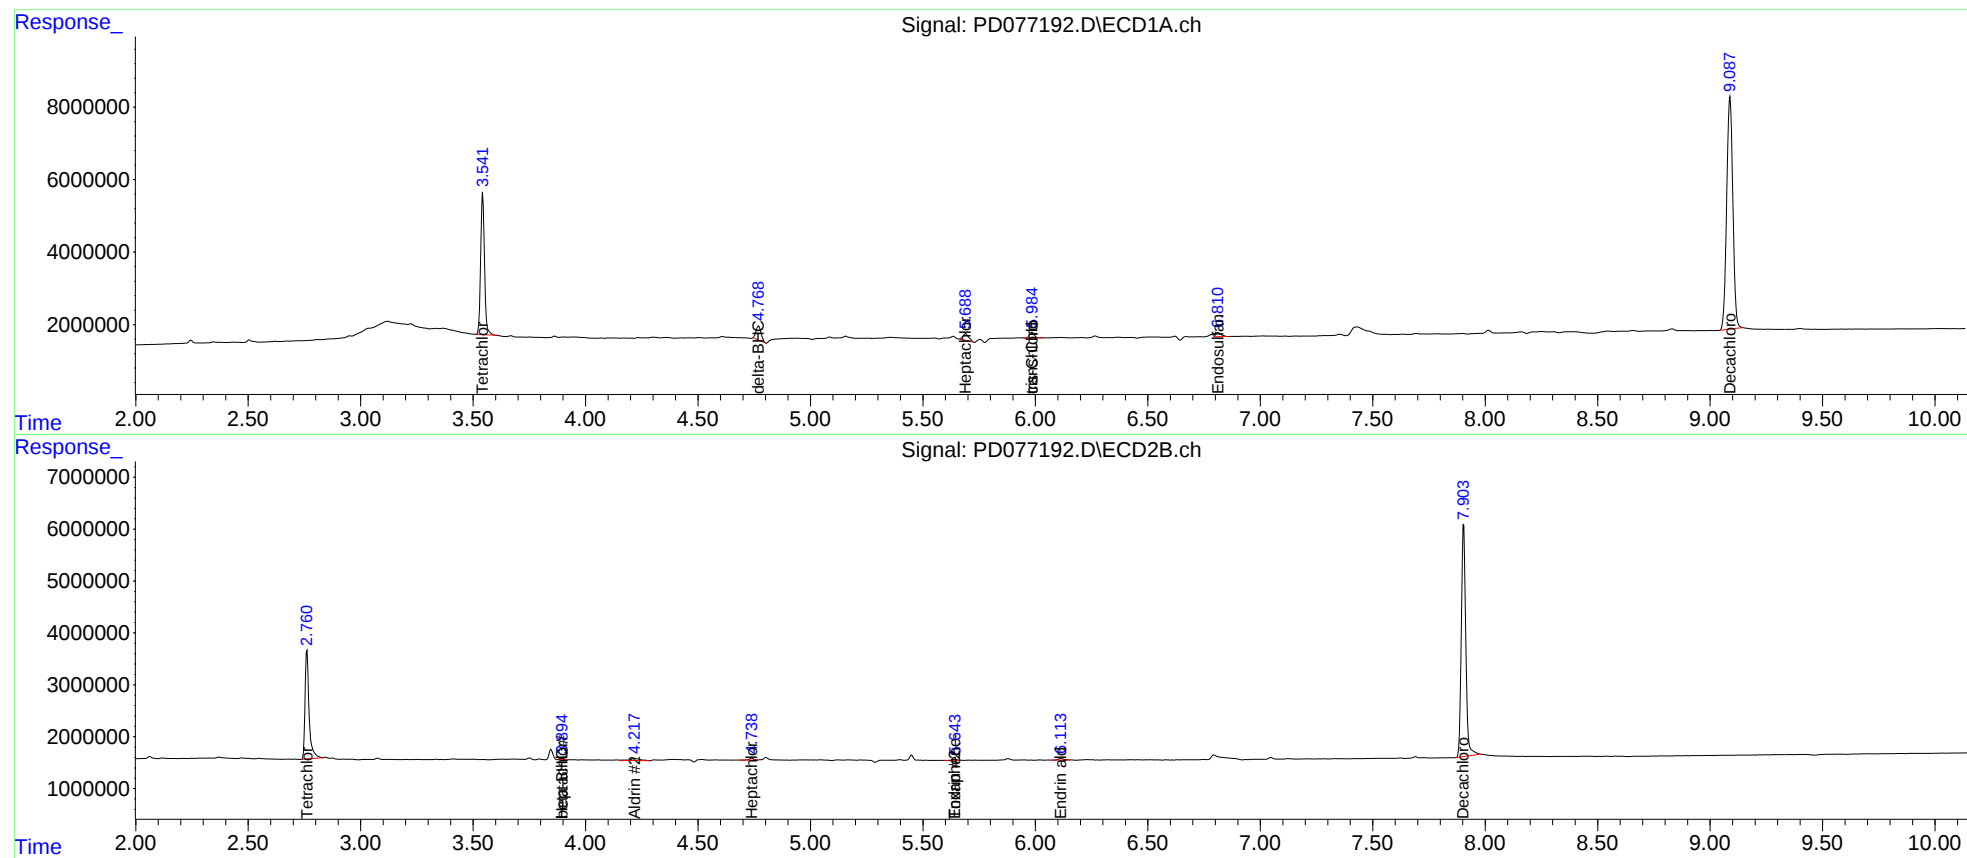

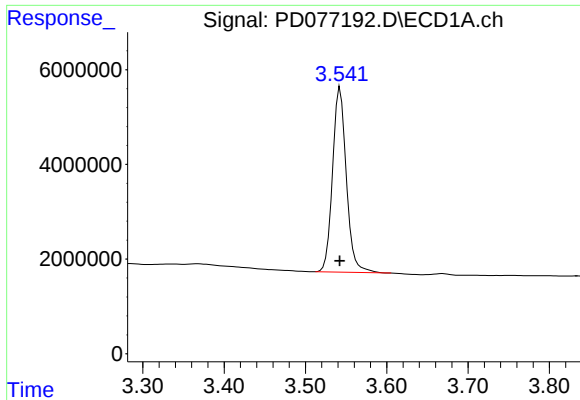


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 46100236
Conc: 21.00 ng/ml

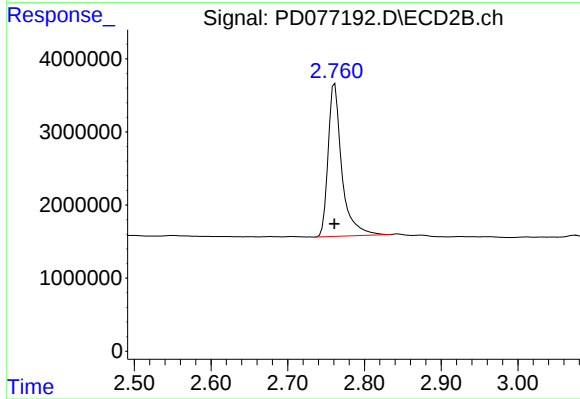


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 25917697
Conc: 20.80 ng/ml

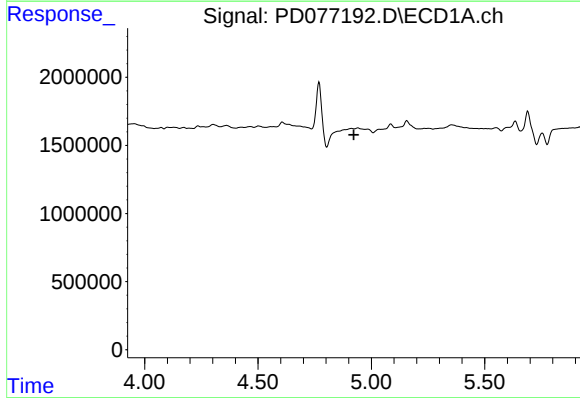


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

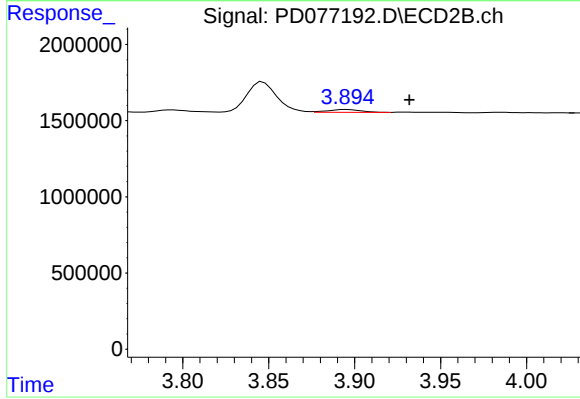


#4 Heptachlor

R.T.: 3.896 min
Delta R.T.: -0.036 min
Response: 245267
Conc: 0.14 ng/ml

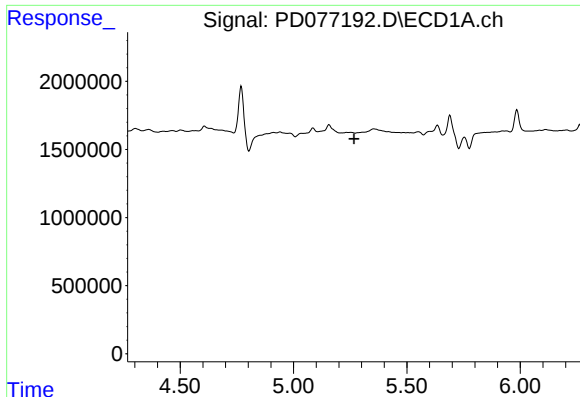


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

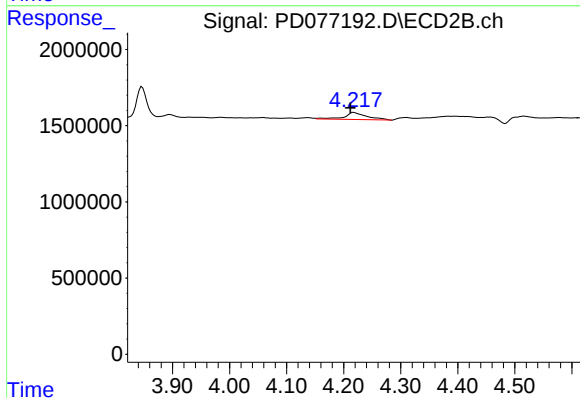


#5 Aldrin

R.T.: 4.218 min
Delta R.T.: 0.006 min
Response: 1273695
Conc: 0.74 ng/ml

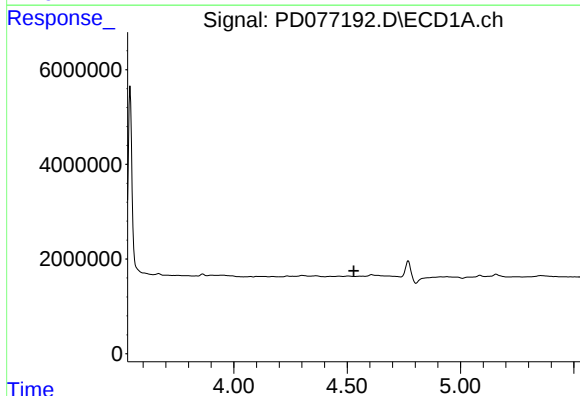


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

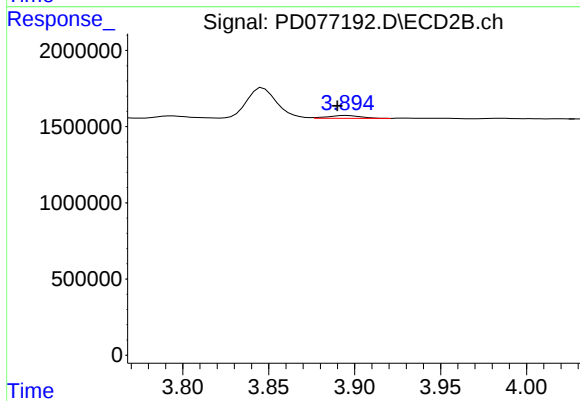


#6 beta-BHC

R.T.: 3.896 min
Delta R.T.: 0.006 min
Response: 245267
Conc: 0.30 ng/ml

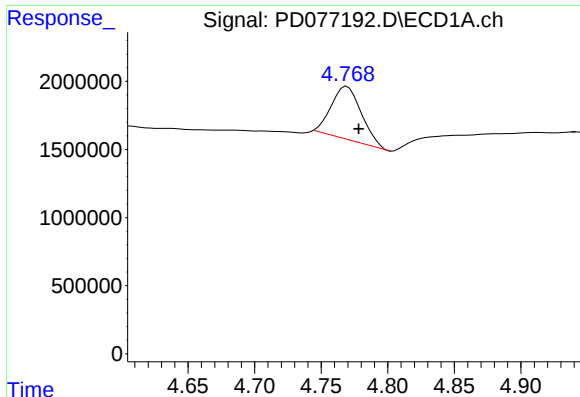


#7 delta-BHC

R.T.: 4.769 min
Delta R.T.: -0.009 min
Response: 5901187
Conc: 1.78 ng/ml

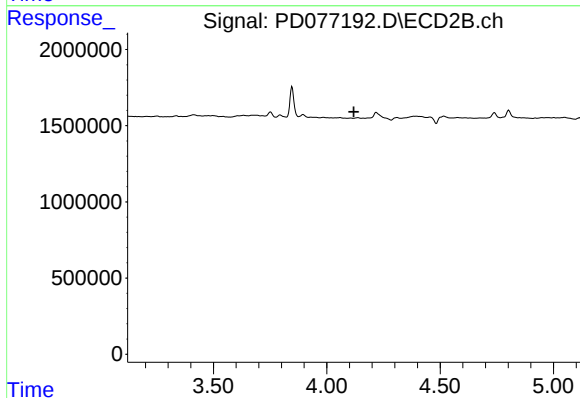


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.119 min
Response: 0
Conc: N.D.

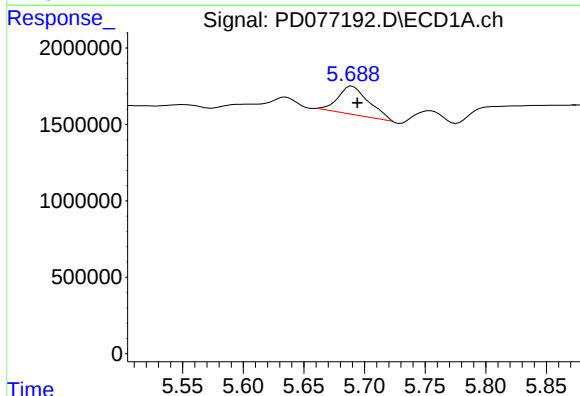


#8 Heptachlor epoxide

R.T.: 5.690 min
Delta R.T.: -0.004 min
Response: 3147241
Conc: 0.99 ng/ml

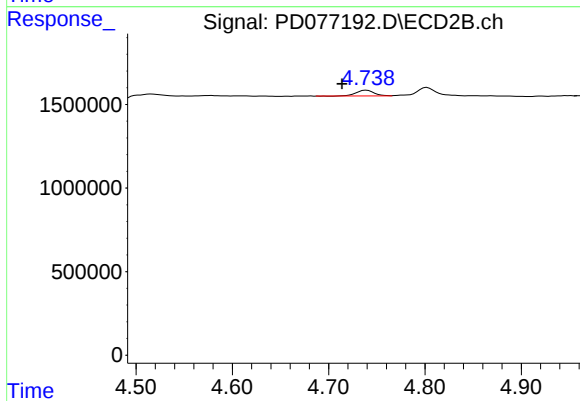


#8 Heptachlor epoxide

R.T.: 4.739 min
Delta R.T.: 0.025 min
Response: 454069
Conc: 0.28 ng/ml

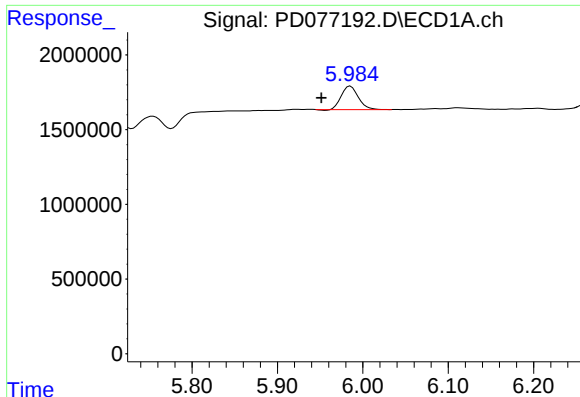


#10 trans-Chlordane

R.T.: 5.986 min
Delta R.T.: 0.034 min
Response: 2150609
Conc: 0.70 ng/ml

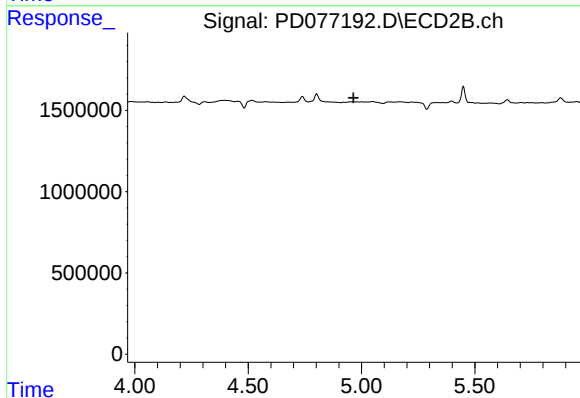


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.965 min
Response: 0
Conc: N.D.

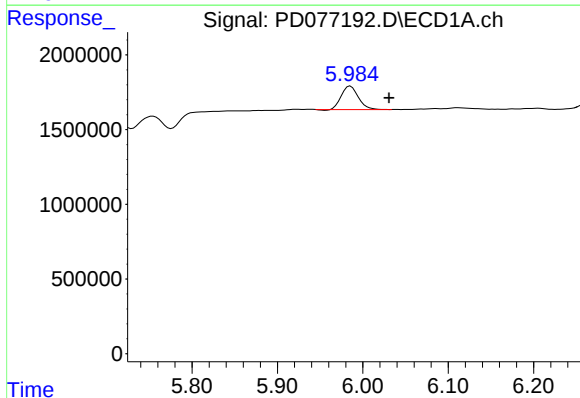


#11 cis-Chlordane

R.T.: 5.986 min
Delta R.T.: -0.045 min
Response: 2150609
Conc: 0.67 ng/ml

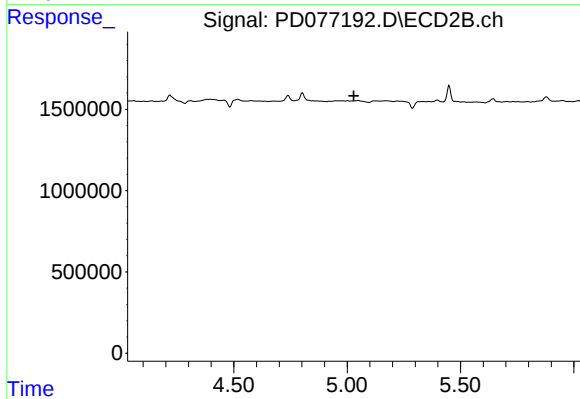


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.029 min
Response: 0
Conc: N.D.

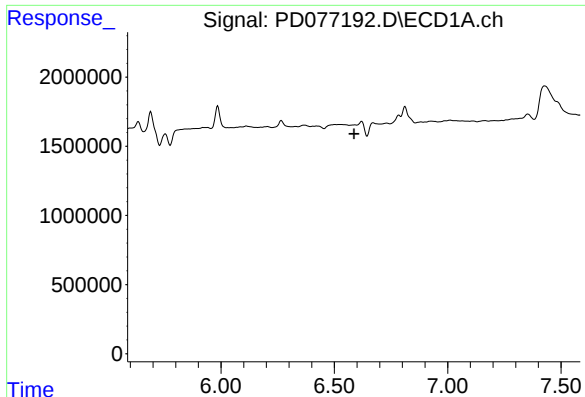


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

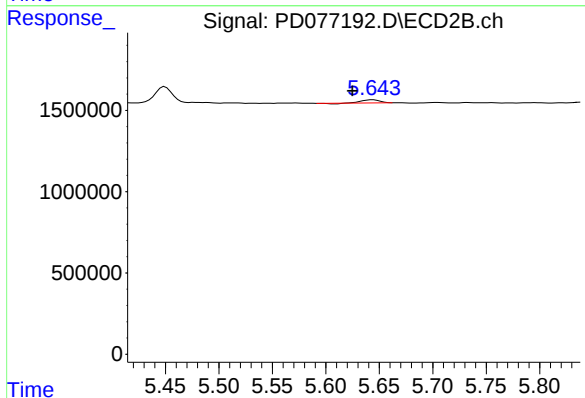


#14 Endrin

R.T.: 5.644 min
Delta R.T.: 0.019 min
Response: 209591
Conc: 0.15 ng/ml

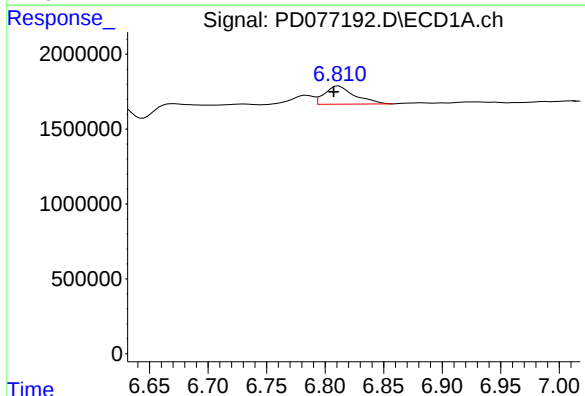


#15 Endosulfan II

R.T.: 6.812 min
Delta R.T.: 0.004 min
Response: 2181923
Conc: 0.77 ng/ml

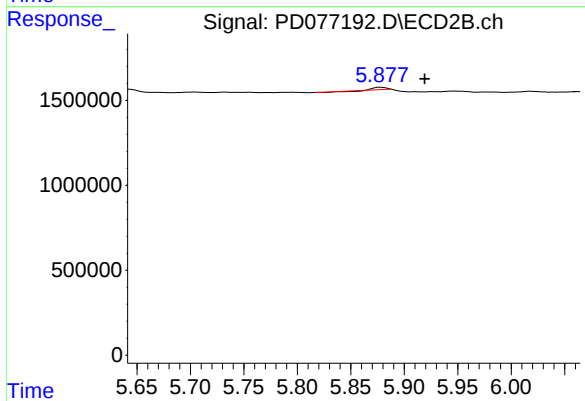


#15 Endosulfan II

R.T.: 5.879 min
Delta R.T.: -0.041 min
Response: 87912
Conc: N.D.

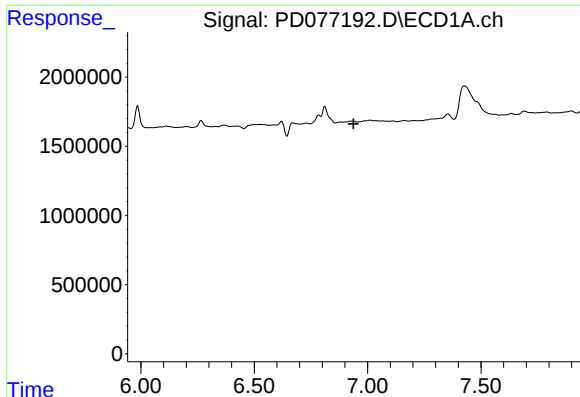


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.938 min
Response: 0
Conc: N.D.

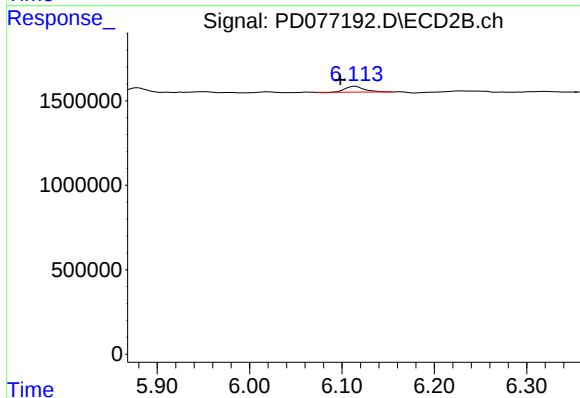


#18 Endrin aldehyde

R.T.: 6.114 min
Delta R.T.: 0.016 min
Response: 506089
Conc: 0.47 ng/ml

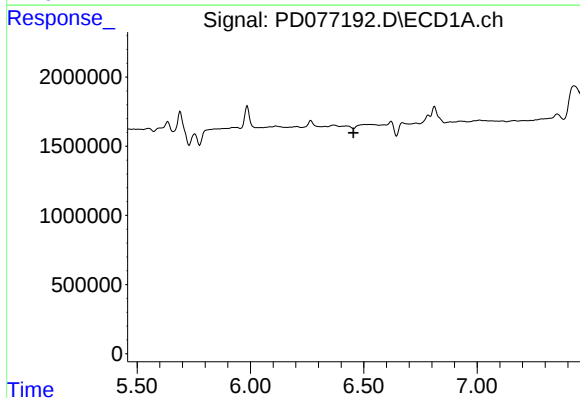


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

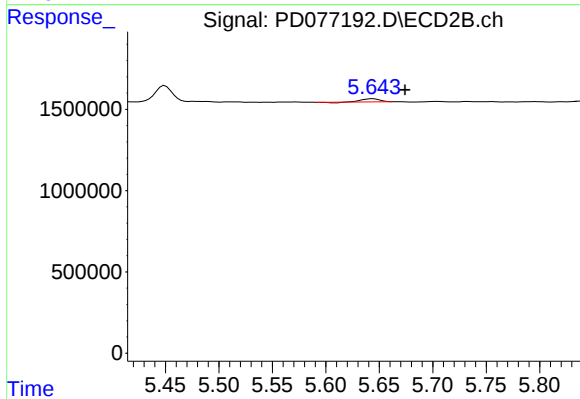


#23 Toxaphene-2

R.T.: 5.644 min
Delta R.T.: -0.030 min
Response: 209591
Conc: 23.96 ng/ml

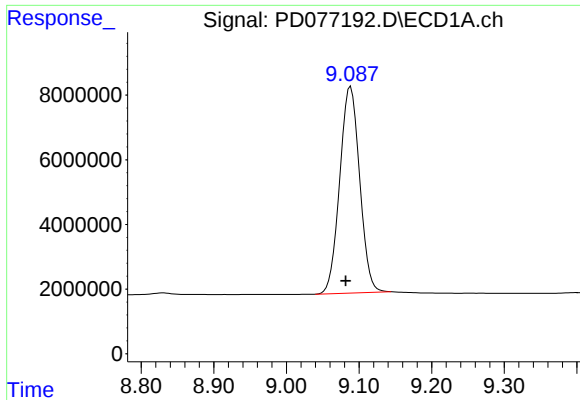

#27 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.006 min
Response: 122013780
Conc: 47.95 ng/ml

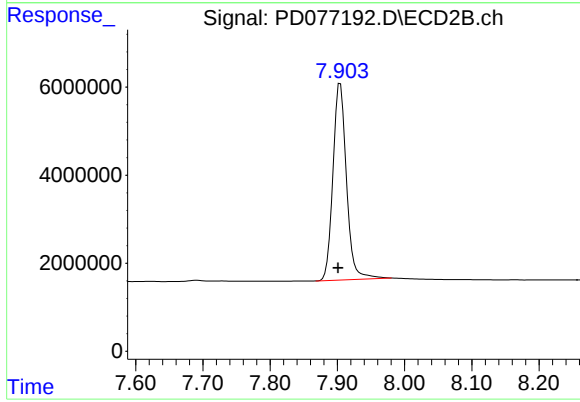

#27 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.003 min
Response: 62070725
Conc: 49.79 ng/ml