

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 10:23
 Operator : AR\AJ
 Sample : PB162720BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:38:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.588	2.925	16137417	102.0E6	19.248	19.383
2)	SA Decachlor...	9.121	8.138	43034197	103.8E6	24.742	27.632
Target Compounds							
9)	A Endosulfan I	6.118	0.000	1186567	0	0.745	N.D. #
11)	B cis-Chlor...	6.118f	0.000	1186567	0	0.690	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 10:23
Operator : AR\AJ
Sample : PB162720BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:38:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

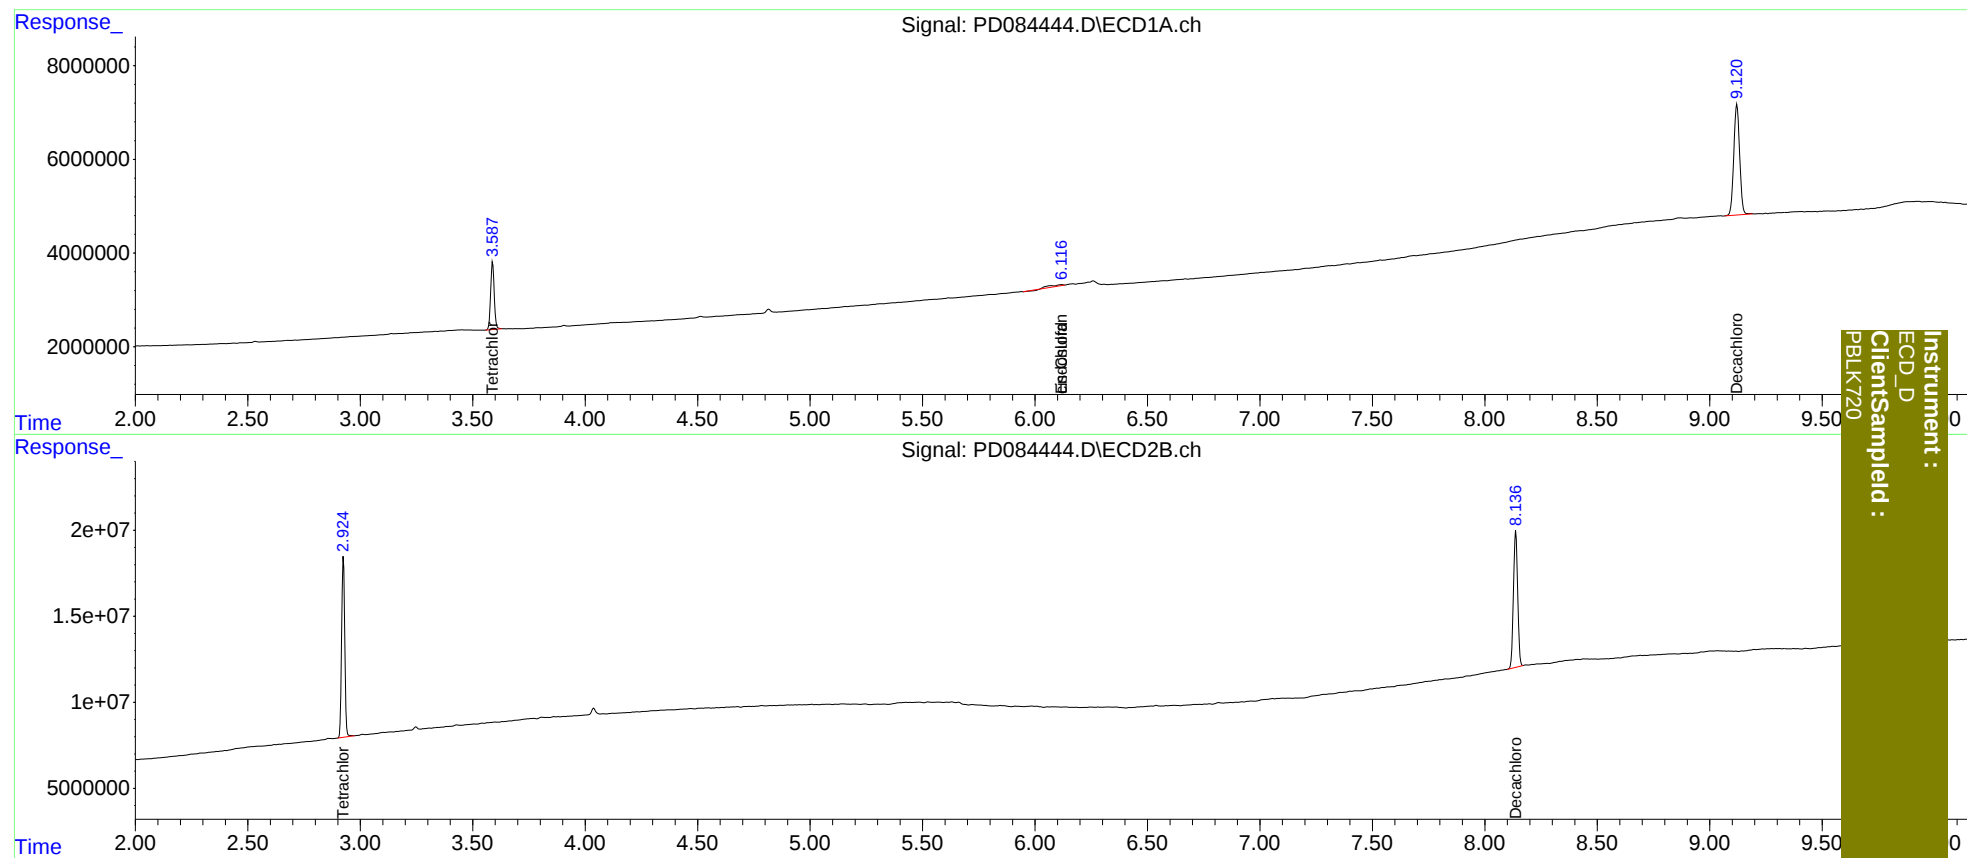


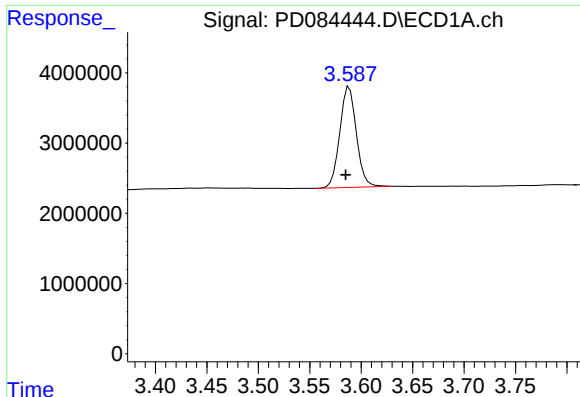

#1 Tetrachloro-m-xylene


R.T.: 3.588 min
Delta R.T.: 0.003 min
Response: 16137417
Conc: 19.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK720

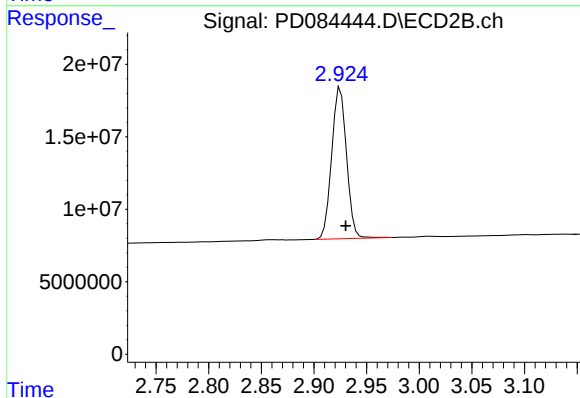


#1 Tetrachloro-m-xylene

R.T.: 2.925 min
Delta R.T.: -0.005 min
Response: 102035719
Conc: 19.38 ng/ml

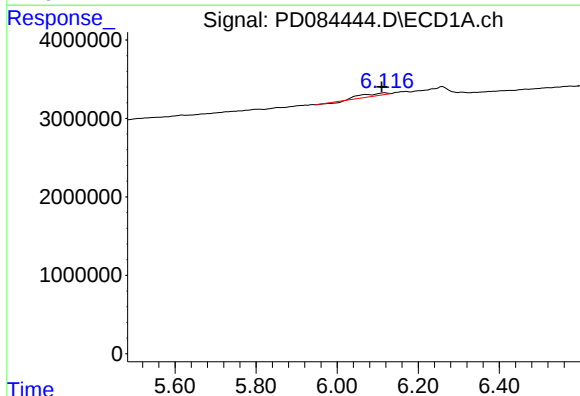


#9 Endosulfan I

R.T.: 6.118 min
Delta R.T.: 0.007 min
Response: 1186567
Conc: 0.74 ng/ml

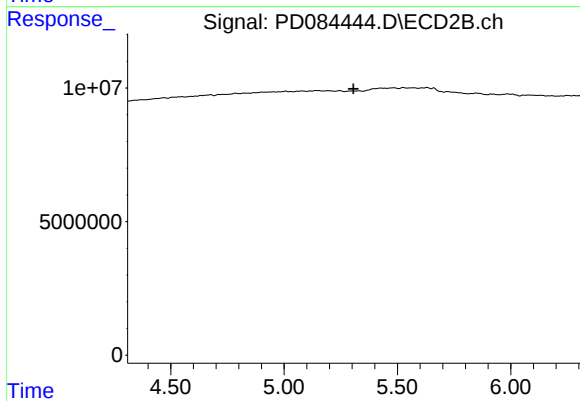

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

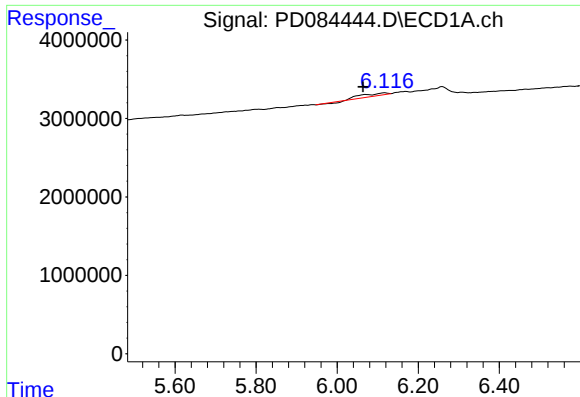

#11 cis-Chlordane


R.T.: 6.118 min
Delta R.T.: 0.054 min
Response: 1186567
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK720

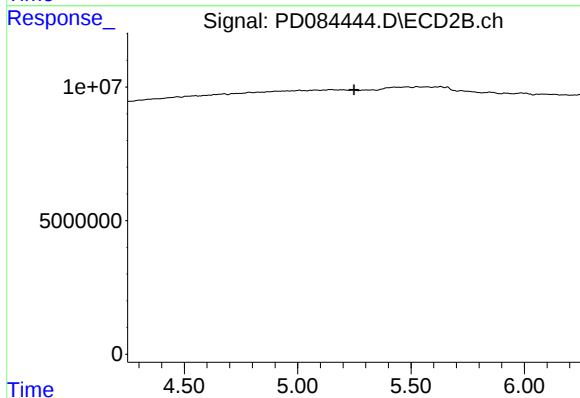


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

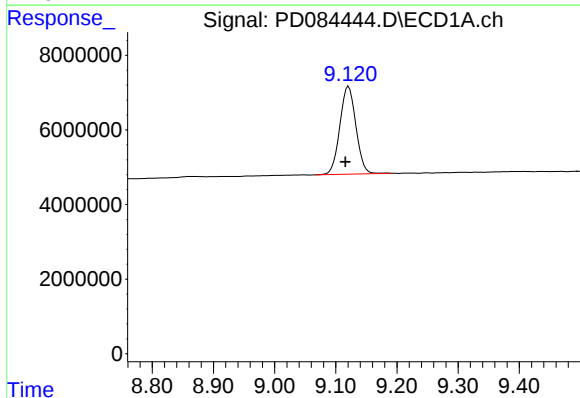

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.005 min
Response: 43034197
Conc: 24.74 ng/ml

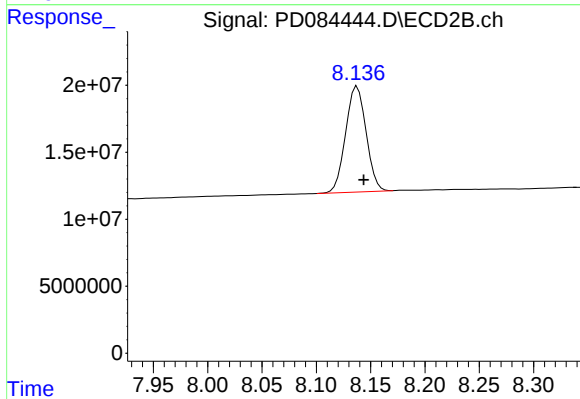

#27 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.006 min
Response: 103838393
Conc: 27.63 ng/ml