

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 13:29
 Operator : AR\AJ
 Sample : PIBLK062
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:43:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.586	2.924	20082326	126.0E6	23.954	23.935
27)	SA Decachlor...	9.117	8.136	38571403	86924790	22.176	23.131
Target Compounds							
7)	B delta-BHC	4.812	0.000	1443288	0	0.836	N.D. #
8)	B Heptachlo...	5.717	0.000	1342707	0	0.790	N.D. #
9)	A Endosulfan I	6.105	0.000	17060888	0	10.710	N.D. #
11)	B cis-Chlor...	6.105f	0.000	17060888	0	9.915	N.D. #
25)	Toxaphene-4	0.000	7.283	0	213.4E6	N.D.	2664.994
26)	Toxaphene-5	8.006f	7.416	13603330	95048172	548.315	1733.230 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 13:29
Operator : AR\AJ
Sample : PIBLK062
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:43:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

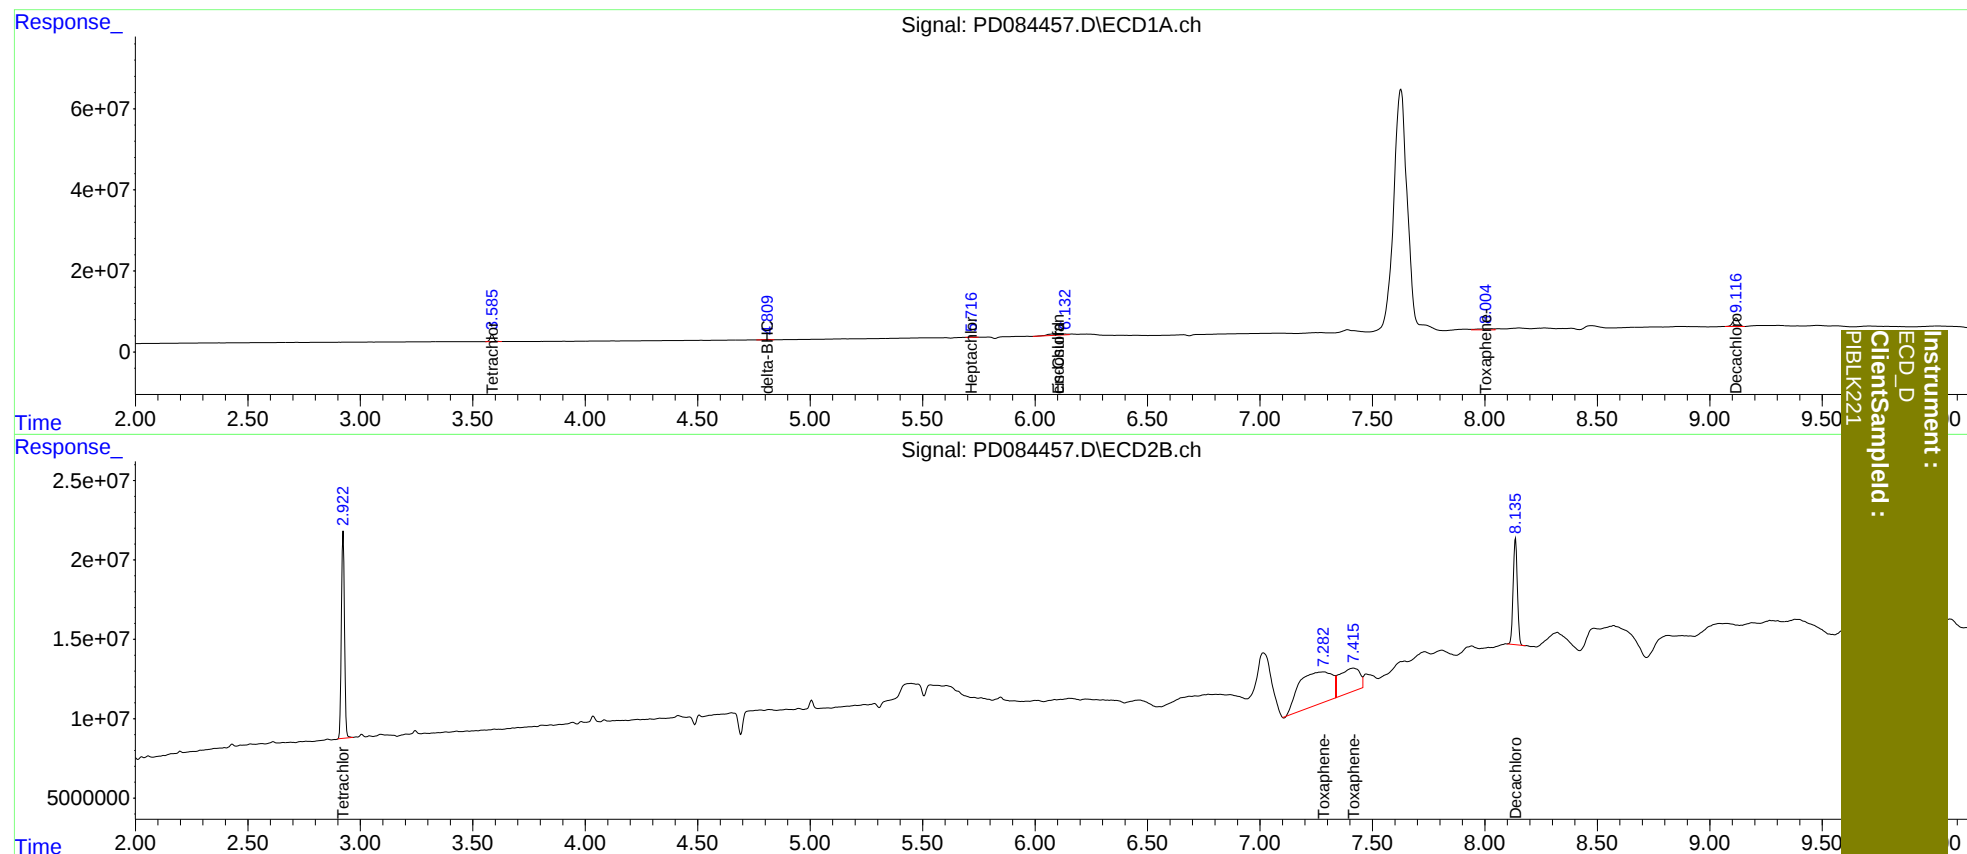


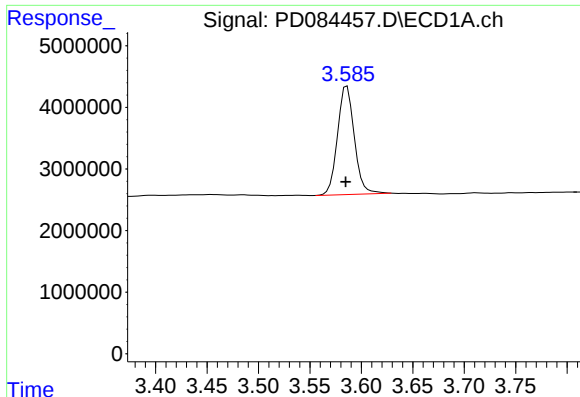

#1 Tetrachloro-m-xylene


R.T.: 3.586 min
Delta R.T.: 0.001 min
Response: 20082326
Conc: 23.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK221

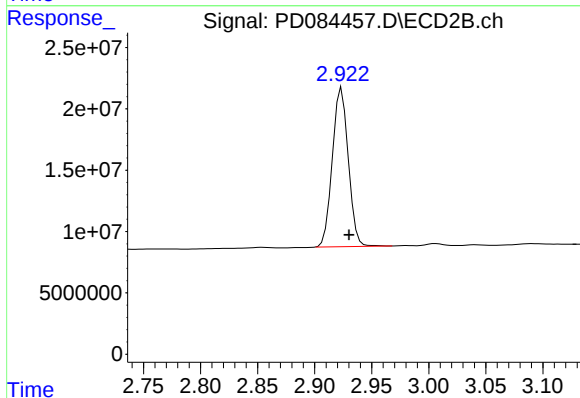


#1 Tetrachloro-m-xylene

R.T.: 2.924 min
Delta R.T.: -0.007 min
Response: 125999762
Conc: 23.94 ng/ml

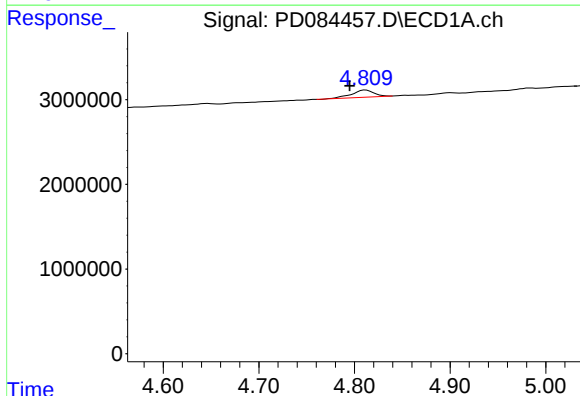


#7 delta-BHC

R.T.: 4.812 min
Delta R.T.: 0.017 min
Response: 1443288
Conc: 0.84 ng/ml

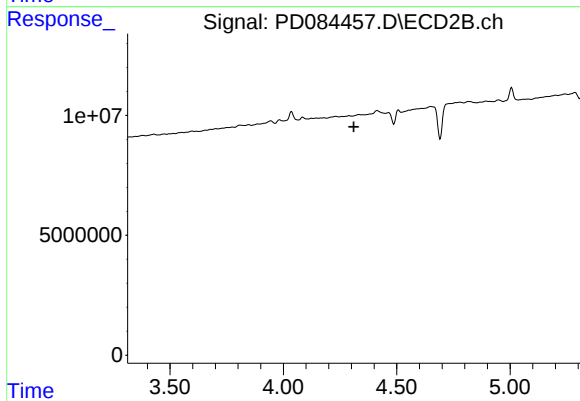

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.311 min
Response: 0
Conc: N.D.

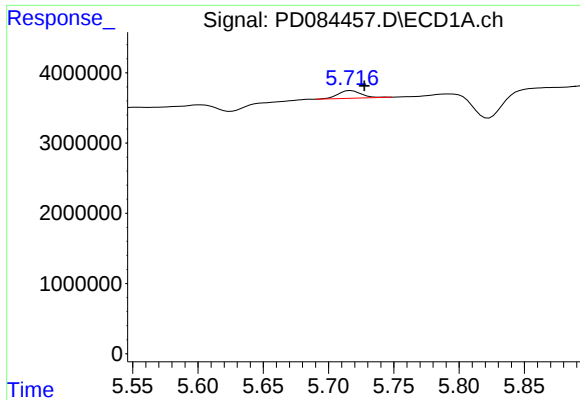

#8 Heptachlor epoxide


R.T.: 5.717 min
Delta R.T.: -0.010 min
Response: 1342707
Conc: 0.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK221

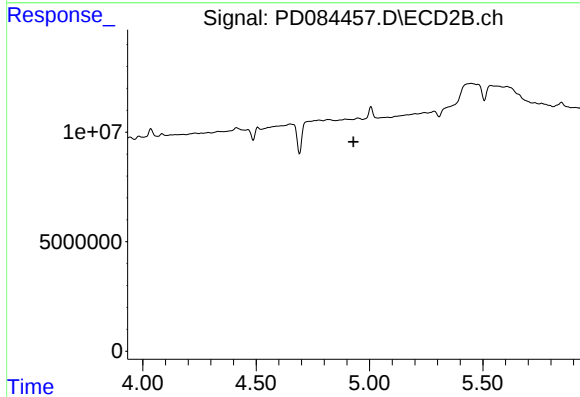


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.930 min
Response: 0
Conc: N.D.

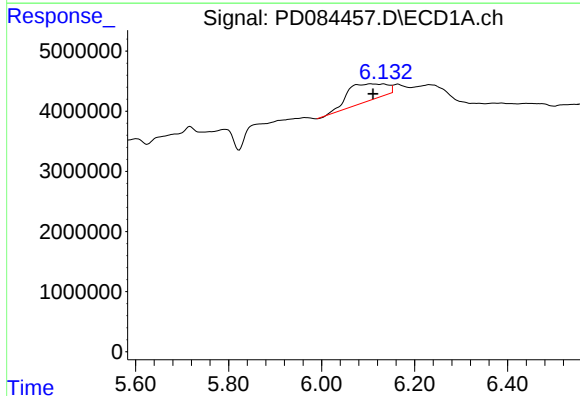


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: -0.005 min
Response: 17060888
Conc: 10.71 ng/ml

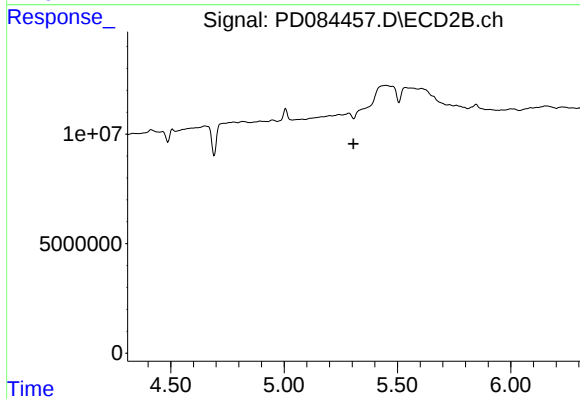

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

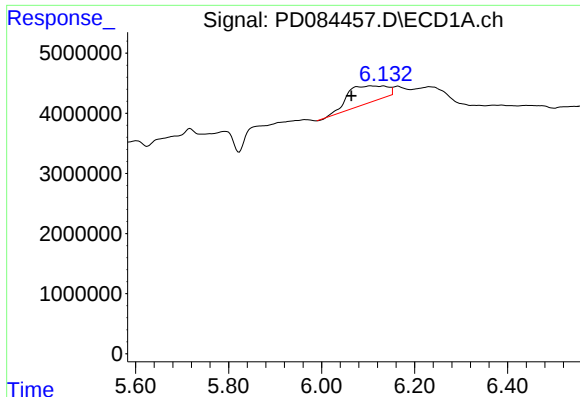

#11 cis-Chlordane


R.T.: 6.105 min
Delta R.T.: 0.041 min
Response: 17060888
Conc: 9.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK221

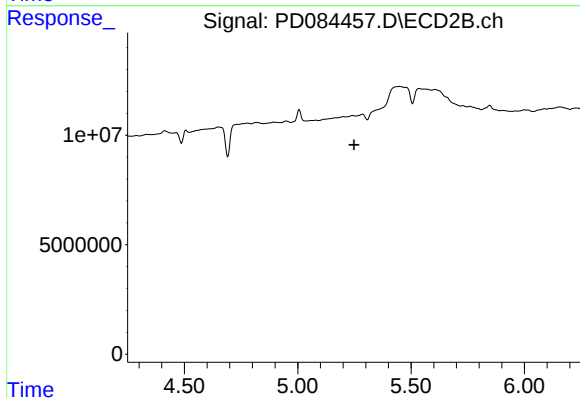


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

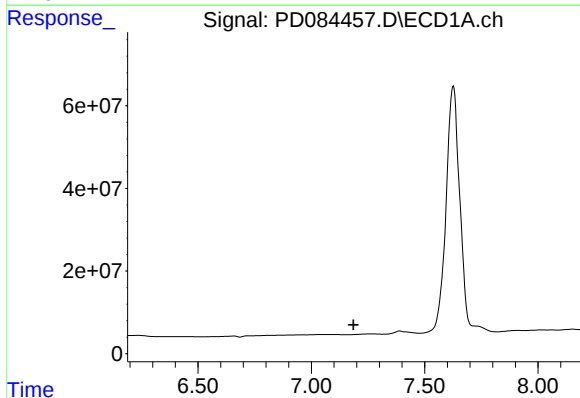


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

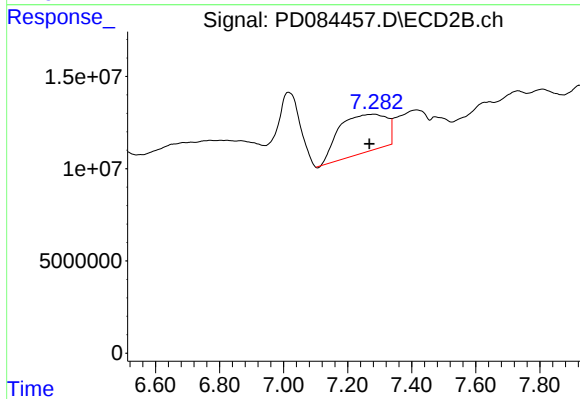

#25 Toxaphene-4


R.T.: 7.283 min
Delta R.T.: 0.016 min
Response: 213378063
Conc: 2664.99 ng/ml

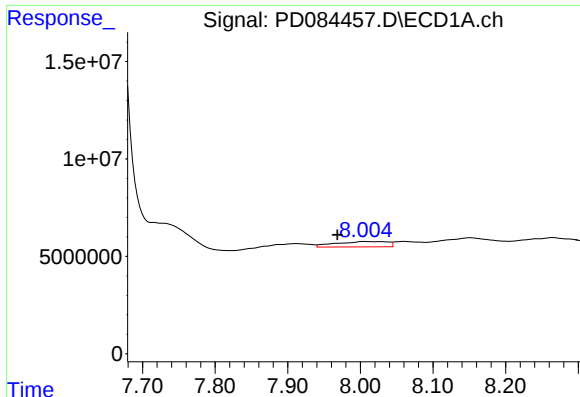

#26 Toxaphene-5


R.T.: 8.006 min
Delta R.T.: 0.037 min
Response: 13603330
Conc: 548.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK221

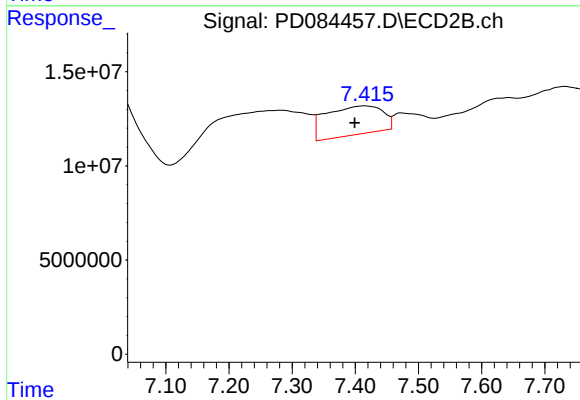


#26 Toxaphene-5

R.T.: 7.416 min
Delta R.T.: 0.016 min
Response: 95048172
Conc: 1733.23 ng/ml

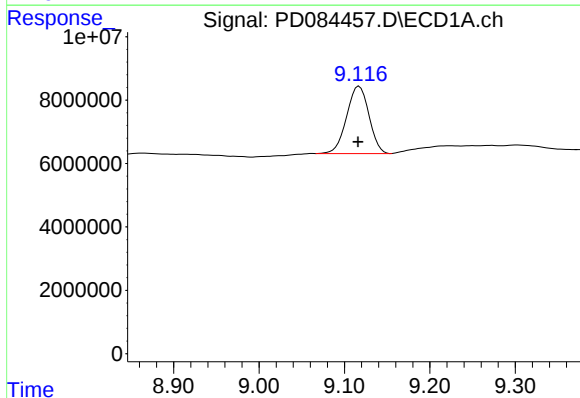

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.001 min
Response: 38571403
Conc: 22.18 ng/ml

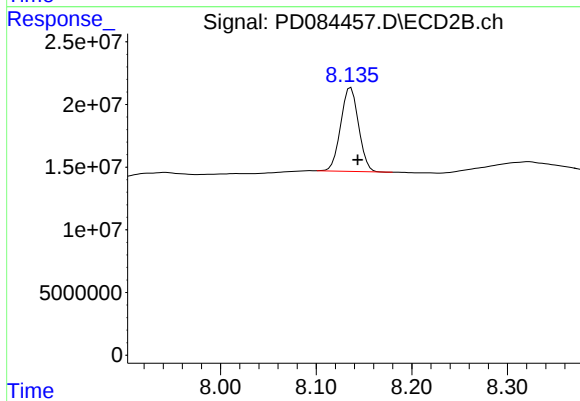

#27 Decachlorobiphenyl

R.T.: 8.136 min
Delta R.T.: -0.007 min
Response: 86924790
Conc: 23.13 ng/ml