

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 16:03
 Operator : AR\AJ
 Sample : P3481-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AD7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:44:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.587	2.924	8290417	56881476	9.889	10.805
27)	SA Decachlor...	9.120	8.137	15298712	36392920	8.796	9.684
Target Compounds							
9)	A Endosulfan I	6.064f	0.000	852941	0	0.535	N.D. #
10)	B trans-Chl...	6.029f	0.000	1999491	0	1.211	N.D. #
11)	B cis-Chlor...	6.064	0.000	852941	0	0.496	N.D. #
15)	B Endosulfa...	6.865f	0.000	805716	0	0.489	N.D. #
26)	Toxaphene-5	0.000	7.406	0	30245453	N.D.	551.534


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 16:03
Operator : AR\AJ
Sample : P3481-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:44:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

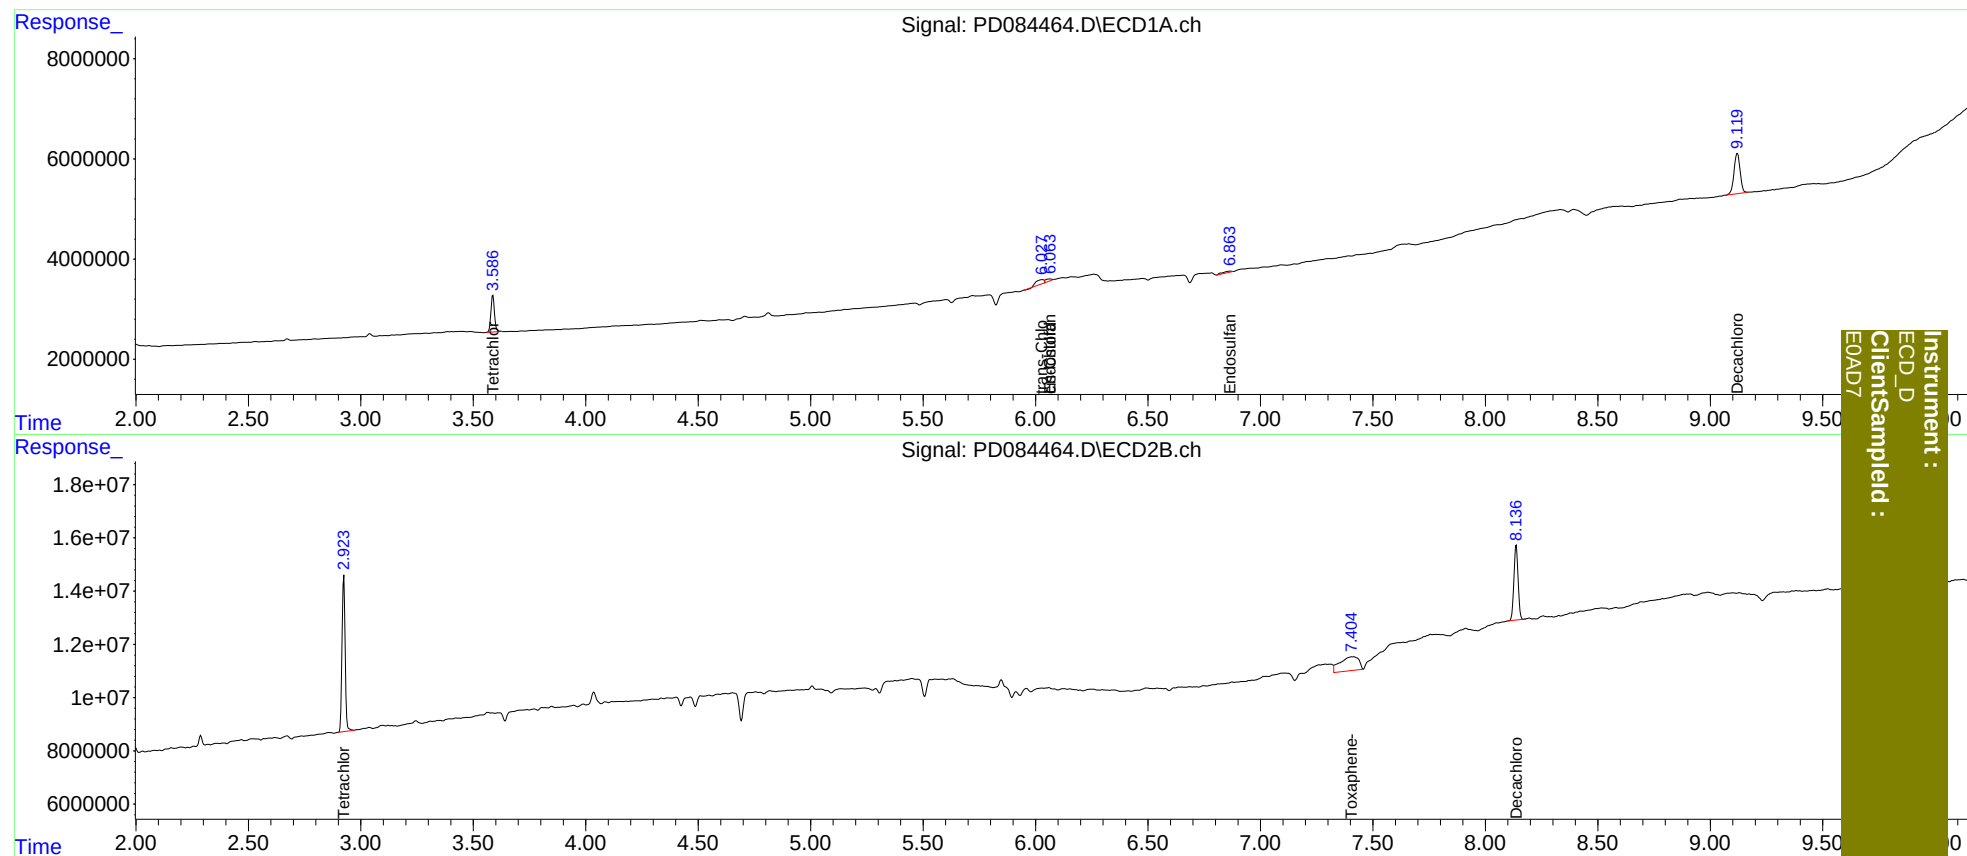


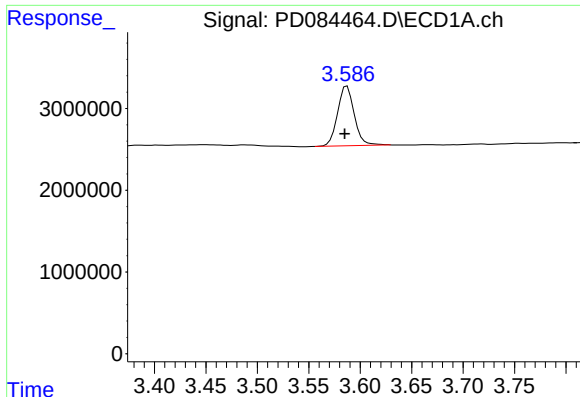

#1 Tetrachloro-m-xylene


R.T.: 3.587 min
Delta R.T.: 0.002 min
Response: 8290417
Conc: 9.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AD7

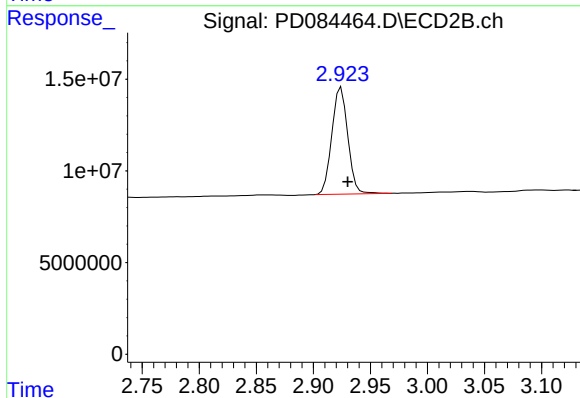


#1 Tetrachloro-m-xylene

R.T.: 2.924 min
Delta R.T.: -0.006 min
Response: 56881476
Conc: 10.81 ng/ml

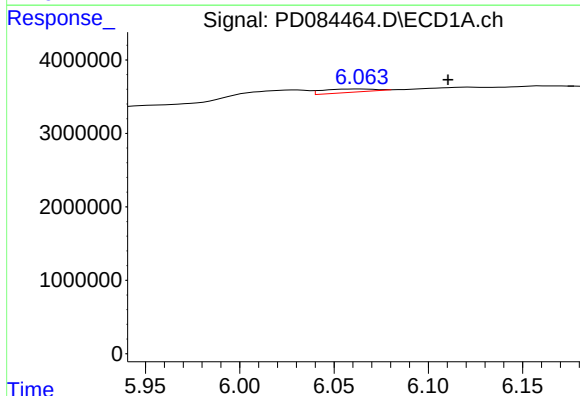


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: -0.046 min
Response: 852941
Conc: 0.54 ng/ml

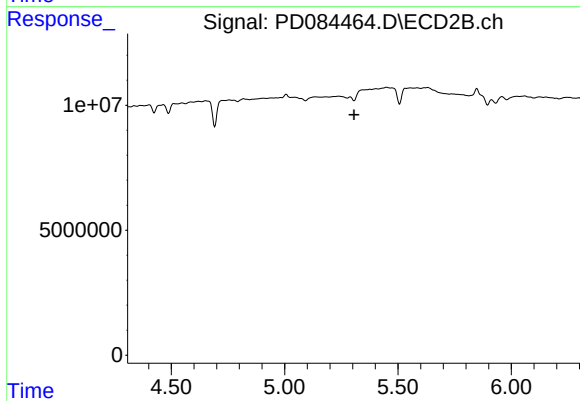

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.306 min
Response: 0
Conc: N.D.

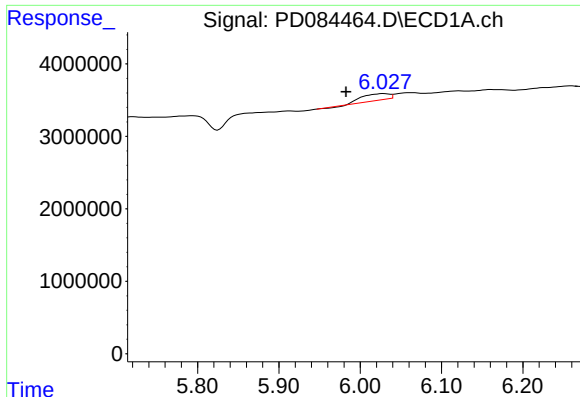

#10 trans-Chlordane


R.T.: 6.029 min
Delta R.T.: 0.047 min
Response: 1999491
Conc: 1.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AD7

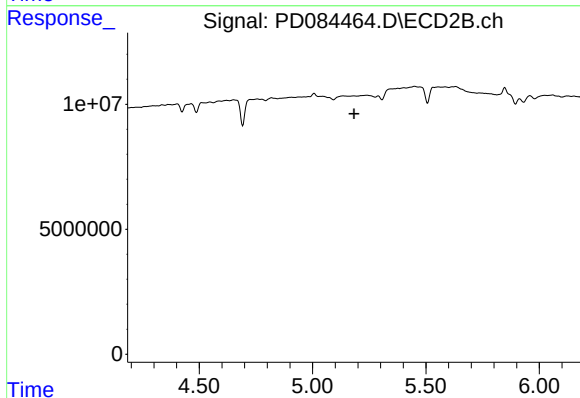


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

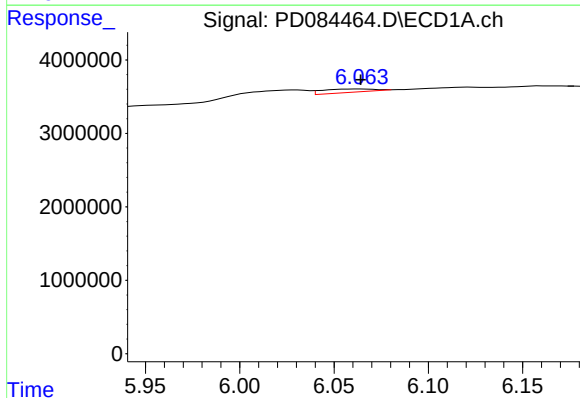


#11 cis-Chlordane

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 852941
Conc: 0.50 ng/ml

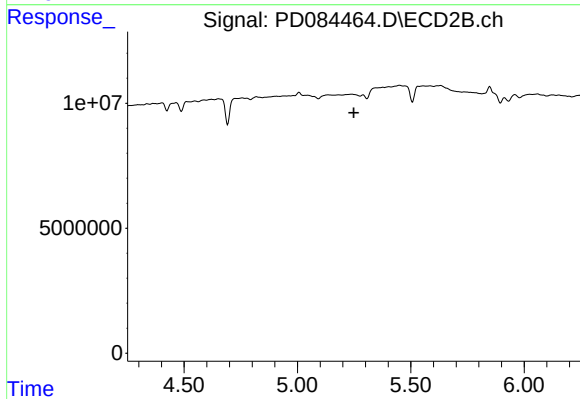

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

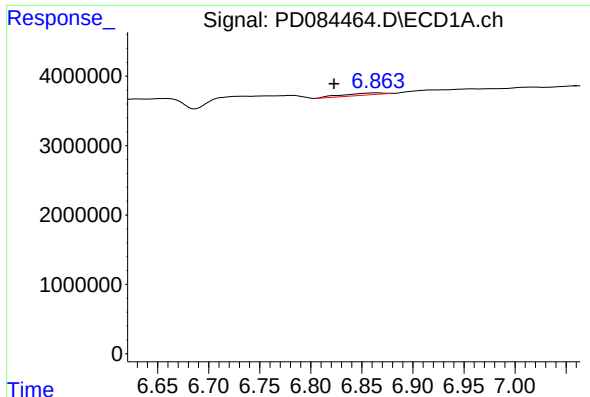

#15 Endosulfan II


R.T.: 6.865 min
Delta R.T.: 0.042 min
Response: 805716
Conc: 0.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AD7

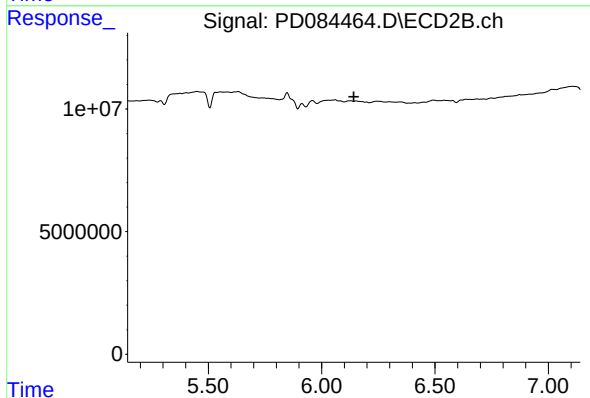


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.142 min
Response: 0
Conc: N.D.

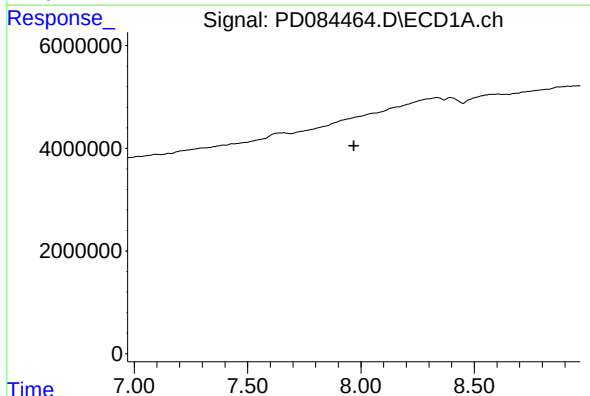


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.968 min
Response: 0
Conc: N.D.

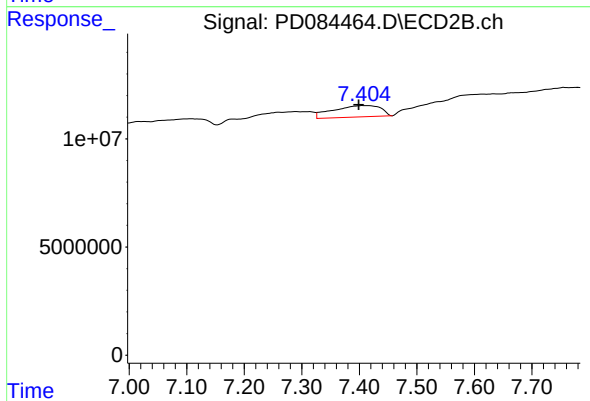

#26 Toxaphene-5


R.T.: 7.406 min
Delta R.T.: 0.007 min
Response: 30245453
Conc: 551.53 ng/ml

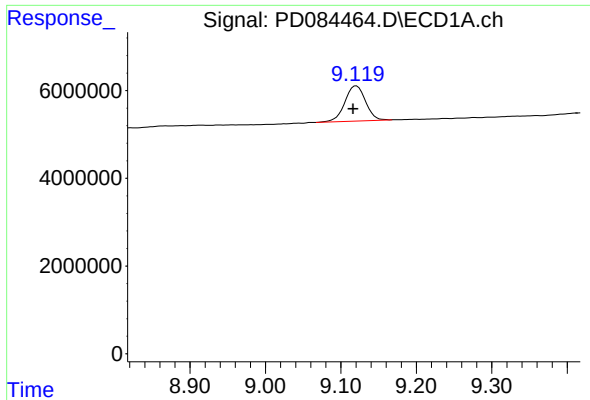

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.004 min
Response: 15298712
Conc: 8.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AD7

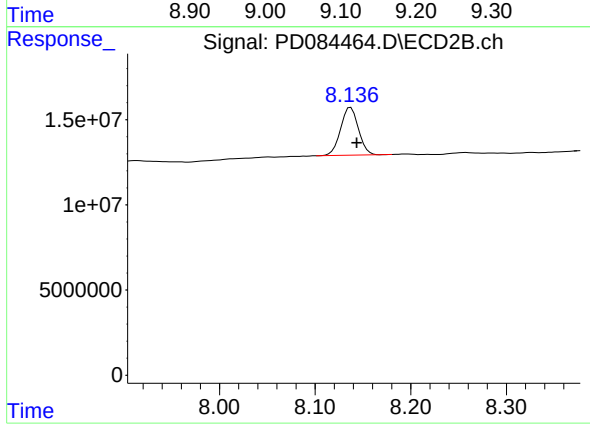

#27 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: -0.006 min
Response: 36392920
Conc: 9.68 ng/ml