

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 12:49
 Operator : AR\AJ
 Sample : P3555-11MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXV9MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:42:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.581	2.927	6009476	39996696	7.168m	7.598
2) SA Decachlor...	9.107	8.110	17557355	508.1E6	10.094m	135.207m#
Target Compounds						
2) A alpha-BHC	4.030	3.440	34951353	202.9E6	23.092	24.894
3) MA gamma-BHC...	4.360	3.776	37718178	187.9E6	24.217	24.378
4) MA Heptachlor	4.961	4.131	40614835	190.5E6	23.270	25.282m
5) MB Aldrin	5.303	4.420	41837652	164.3E6	23.706	22.413
6) B beta-BHC	4.543	4.069	16832420	85472356	23.297	23.766
7) B delta-BHC	4.793	4.307	52679079	197.8E6	30.505	23.584
8) B Heptachlo...	5.722	4.924	37111192	169.4E6	21.834	25.392
9) A Endosulfan I	6.106	5.300	38946802	145.9E6	24.449	24.596m
10) B trans-Chl...	5.975	5.177	37049312	136.8E6	22.438m	21.476m
11) B cis-Chlor...	6.059	5.244	40766736	149.0E6	23.691	23.679
12) B 4,4'-DDE	6.226	5.428	86424673	329.5E6	49.410	54.036
13) MA Dieldrin	6.379	5.567	85922792	317.9E6	47.824	51.678
14) MA Endrin	6.606	5.845	70092853	275.1E6	46.790	49.835
15) B Endosulfa...	6.818	6.135	56890261	229.6E6	34.504	44.224m#
16) A 4,4'-DDD	6.733	5.983	74684017	215.2E6	58.067m	43.871m
17) MA 4,4'-DDT	7.051	6.240	64666523	274.9E6	47.696	55.498
18) B Endrin al...	6.946	6.315	61374574	180.4E6	53.999	48.209
19) B Endosulfa...	7.180	6.558	75487898	6631.5E6	49.730	1420.363m#
20) A Methoxychlor	7.522	6.812	177.4E6	596.8E6	222.400	277.132
21) B Endrin ke...	7.642	7.050	5694.2E6	223.3E6	3438.361m	42.886 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 12:49
Operator : AR\AJ
Sample : P3555-11MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:42:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

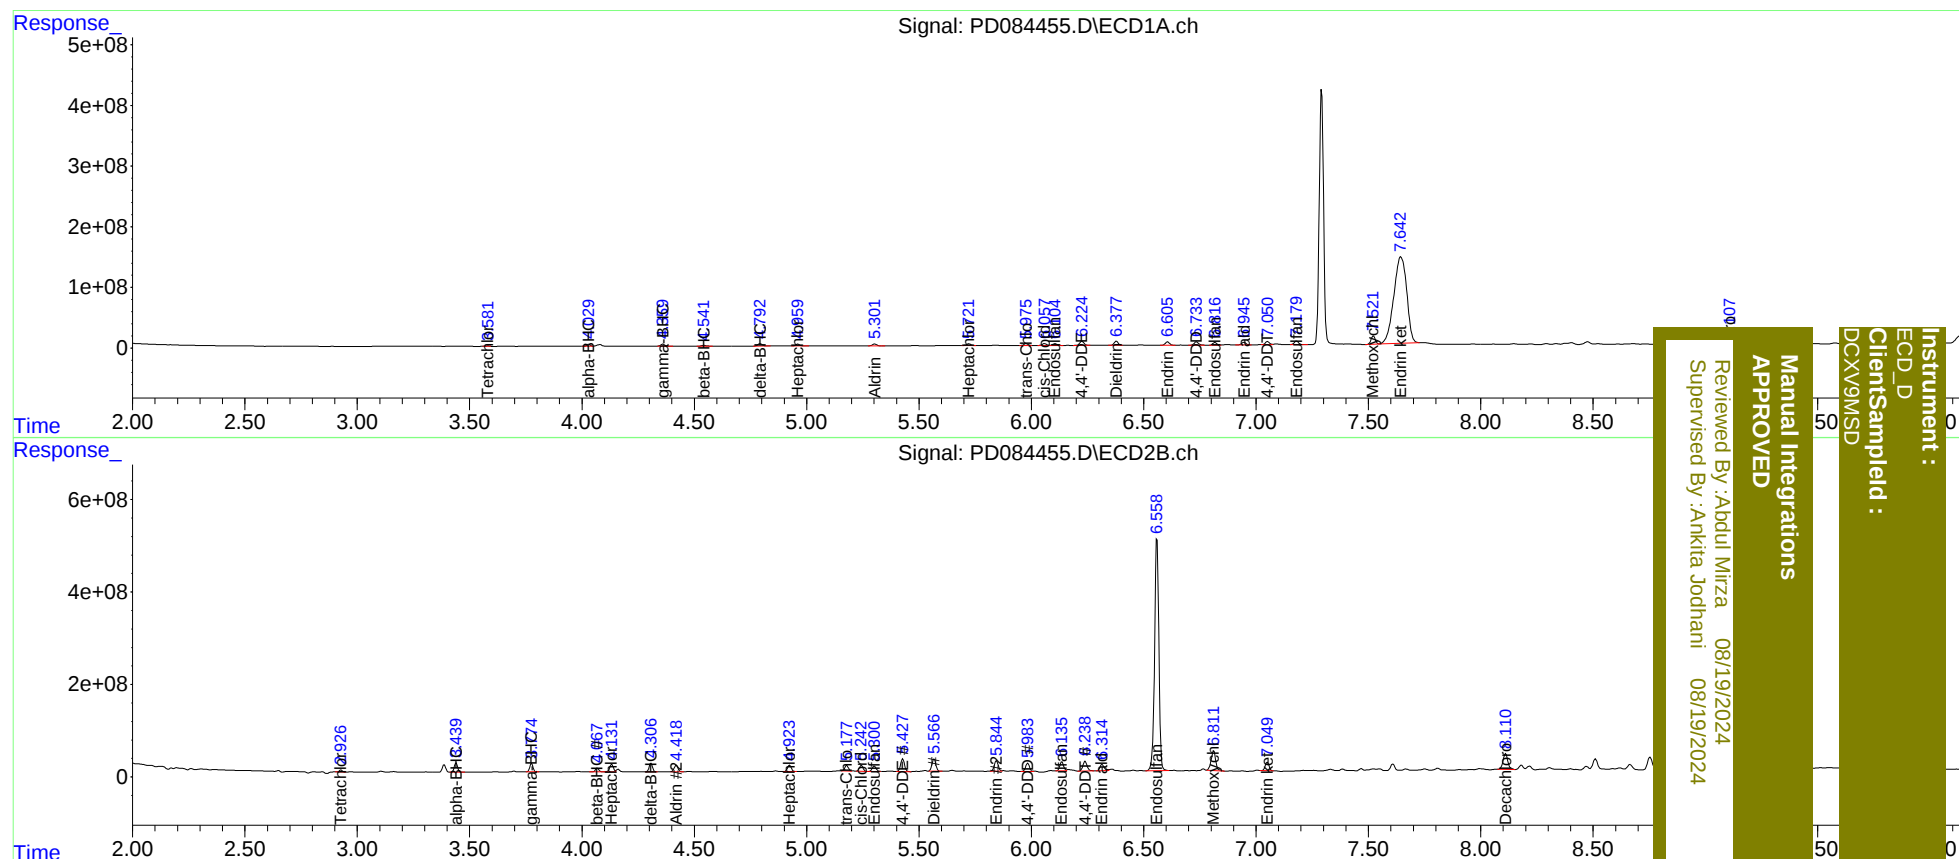

Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DCX/9MSD