

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 17:01
 Operator : AR\AJ
 Sample : P3481-09MS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AE4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/16/2024
 Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 08:11:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.925	11691218	76932026	13.945	14.614
2)	SA Decachlor...	9.114	8.136	21470006	49345931	12.344m	13.131
Target Compounds							
2)	A alpha-BHC	4.034	3.439	63525545	324.4E6	41.972	39.792
3)	MA gamma-BHC...	4.364	3.775	63898293	304.0E6	41.025	39.446
4)	MA Heptachlor	4.964	4.131	70330521	285.6E6	40.296	37.895m
5)	MB Aldrin	5.307	4.419	68908207	254.7E6	39.045	34.748
6)	B beta-BHC	4.546	4.068	20078044	105.2E6	27.789	29.248
7)	B delta-BHC	4.795	4.307	61547781	291.8E6	35.640	34.790
8)	B Heptachlo...	5.726	4.924	68098854	257.9E6	40.066	38.654
9)	A Endosulfan I	6.110	5.299	63098297	222.5E6	39.611	37.502m
10)	B trans-Chl...	5.980	5.178	64048320	244.0E6	38.790	38.295
11)	B cis-Chlor...	6.063	5.243	66334240	259.6E6	38.550	41.249
12)	B 4,4'-DDE	6.231	5.428	126.8E6	474.1E6	72.490	77.745
13)	MA Dieldrin	6.383	5.567	143.3E6	470.7E6	79.771	76.522
14)	MA Endrin	6.611	5.844	127.0E6	422.8E6	84.794	76.584
15)	B Endosulfa...	6.822	6.134	119.4E6	385.6E6	72.413	74.260m
16)	A 4,4'-DDD	6.739	5.984	119.9E6	364.7E6	93.188	74.342
17)	MA 4,4'-DDT	7.056	6.240	87858308	314.4E6	64.802	63.476
18)	B Endrin al...	6.950	6.315	91444418	254.5E6	80.455	68.013
19)	B Endosulfa...	7.185	6.540	118.2E6	335.4E6	77.881	71.829
20)	A Methoxychlor	7.526	6.813	270.7E6	710.2E6	339.410	329.781
21)	B Endrin ke...	7.666	7.051	129.5E6	359.4E6	78.227	69.017

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 17:01
Operator : AR\AJ
Sample : P3481-09MS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 08:11:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

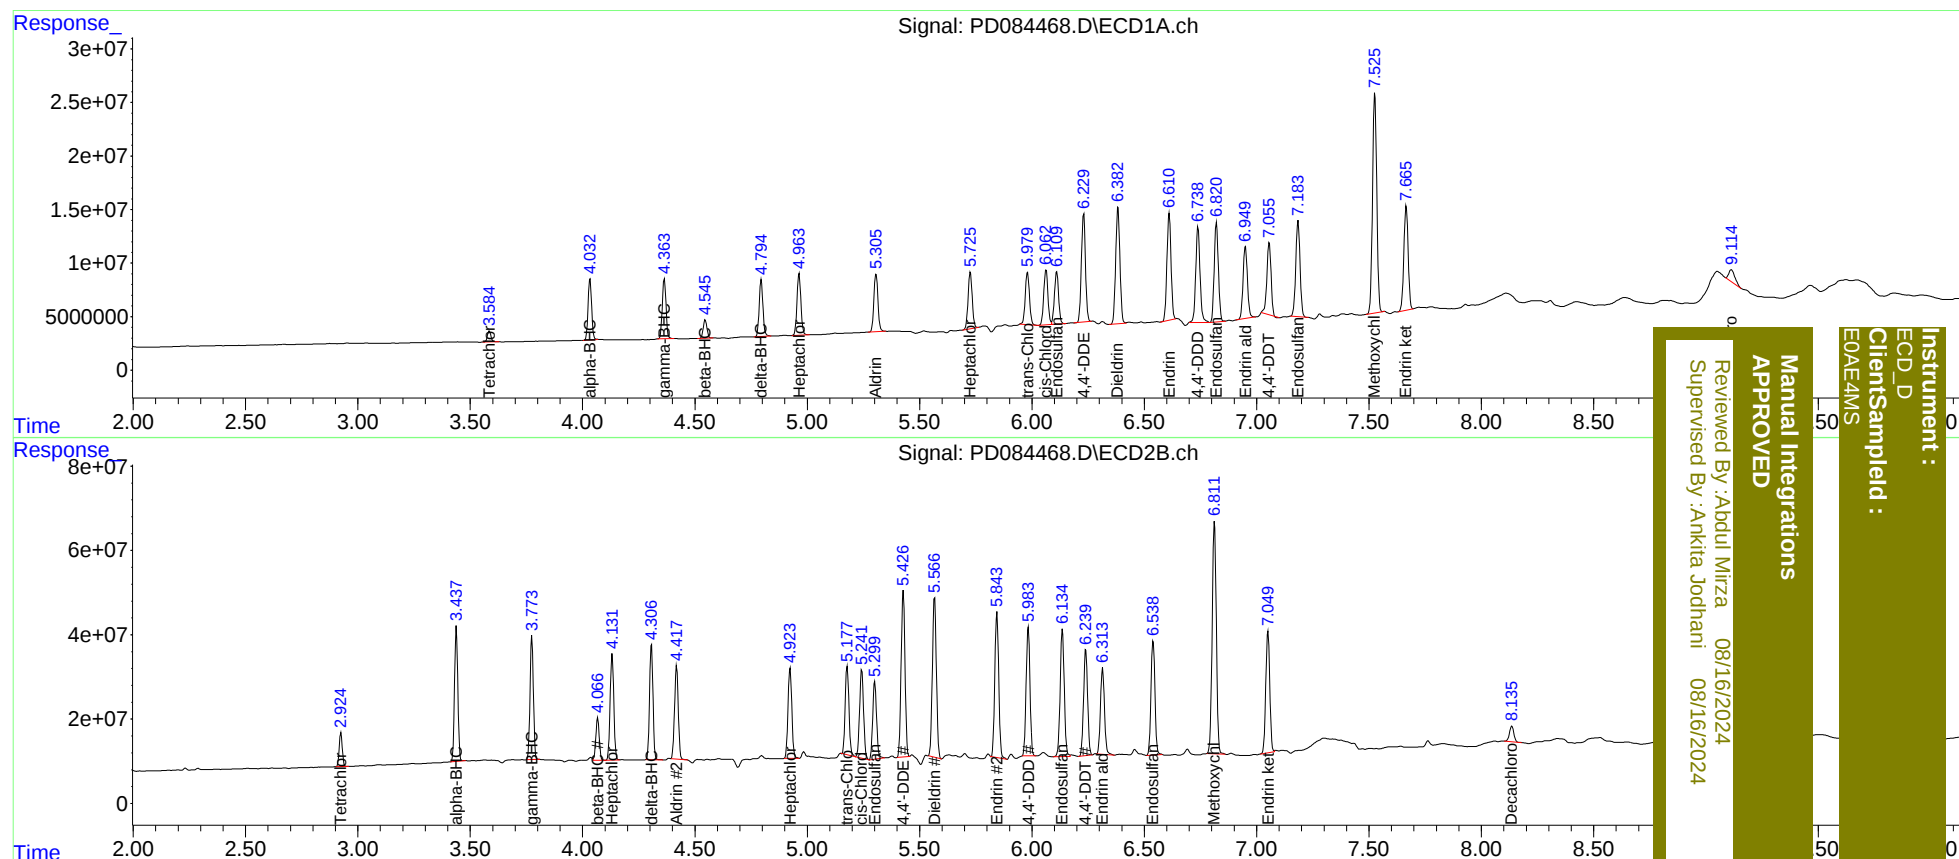

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 08/16/2024
Supervised By: Ankita Jodhani 08/16/2024

Instrument :
ECD_D
Client Sampled :
EOAE4MS