

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
 Data File : PD084469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 17:14
 Operator : AR\AJ
 Sample : P3481-10MSD
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AE4MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/16/2024
 Supervised By :Ankita Jodhani 08/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:45:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.927	11928152	78467296	14.228	14.906
27)	SA Decachlor...	9.113	8.136	25625537	52292727	14.733	13.915
Target Compounds							
2)	A alpha-BHC	4.031	3.440	62519403	321.1E6	41.307	39.392
3)	MA gamma-BHC...	4.361	3.776	62850976	298.7E6	40.353	38.755
4)	MA Heptachlor	4.962	4.132	69191655	271.3E6	39.643	35.994m
5)	MB Aldrin	5.303	4.420	69558230	241.4E6	39.414	32.936
6)	B beta-BHC	4.543	4.069	19736538	99337533	27.317	27.621
7)	B delta-BHC	4.792	4.308	60653000	277.4E6	35.122	33.071
8)	B Heptachlo...	5.723	4.925	66976470	256.1E6	39.406	38.382
9)	A Endosulfan I	6.105	5.300	60465386	231.1E6	37.958m	38.945m
10)	B trans-Chl...	5.977	5.179	62743146	240.7E6	38.000	37.772
11)	B cis-Chlor...	6.059	5.244	66176093	255.6E6	38.458	40.618
12)	B 4,4'-DDE	6.227	5.428	130.7E6	468.8E6	74.748	76.879
13)	MA Dieldrin	6.380	5.568	141.2E6	492.7E6	78.568	80.099
14)	MA Endrin	6.607	5.845	125.9E6	415.8E6	84.051	75.314
15)	B Endosulfa...	6.817	6.137	121.1E6	386.4E6	73.462	74.416
16)	A 4,4'-DDD	6.735	5.984	116.0E6	383.6E6	90.163	78.199
17)	MA 4,4'-DDT	7.052	6.240	82181003	323.3E6	60.615	65.274
18)	B Endrin al...	6.947	6.315	85153913	267.7E6	74.921	71.559
19)	B Endosulfa...	7.181	6.540	115.3E6	337.4E6	75.970	72.270
20)	A Methoxychlor	7.522	6.813	257.6E6	693.0E6	323.026	321.818
21)	B Endrin ke...	7.662	7.051	126.2E6	377.5E6	76.180	72.482

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081524\
Data File : PD084469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 17:14
Operator : AR\AJ
Sample : P3481-10MSD
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:45:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

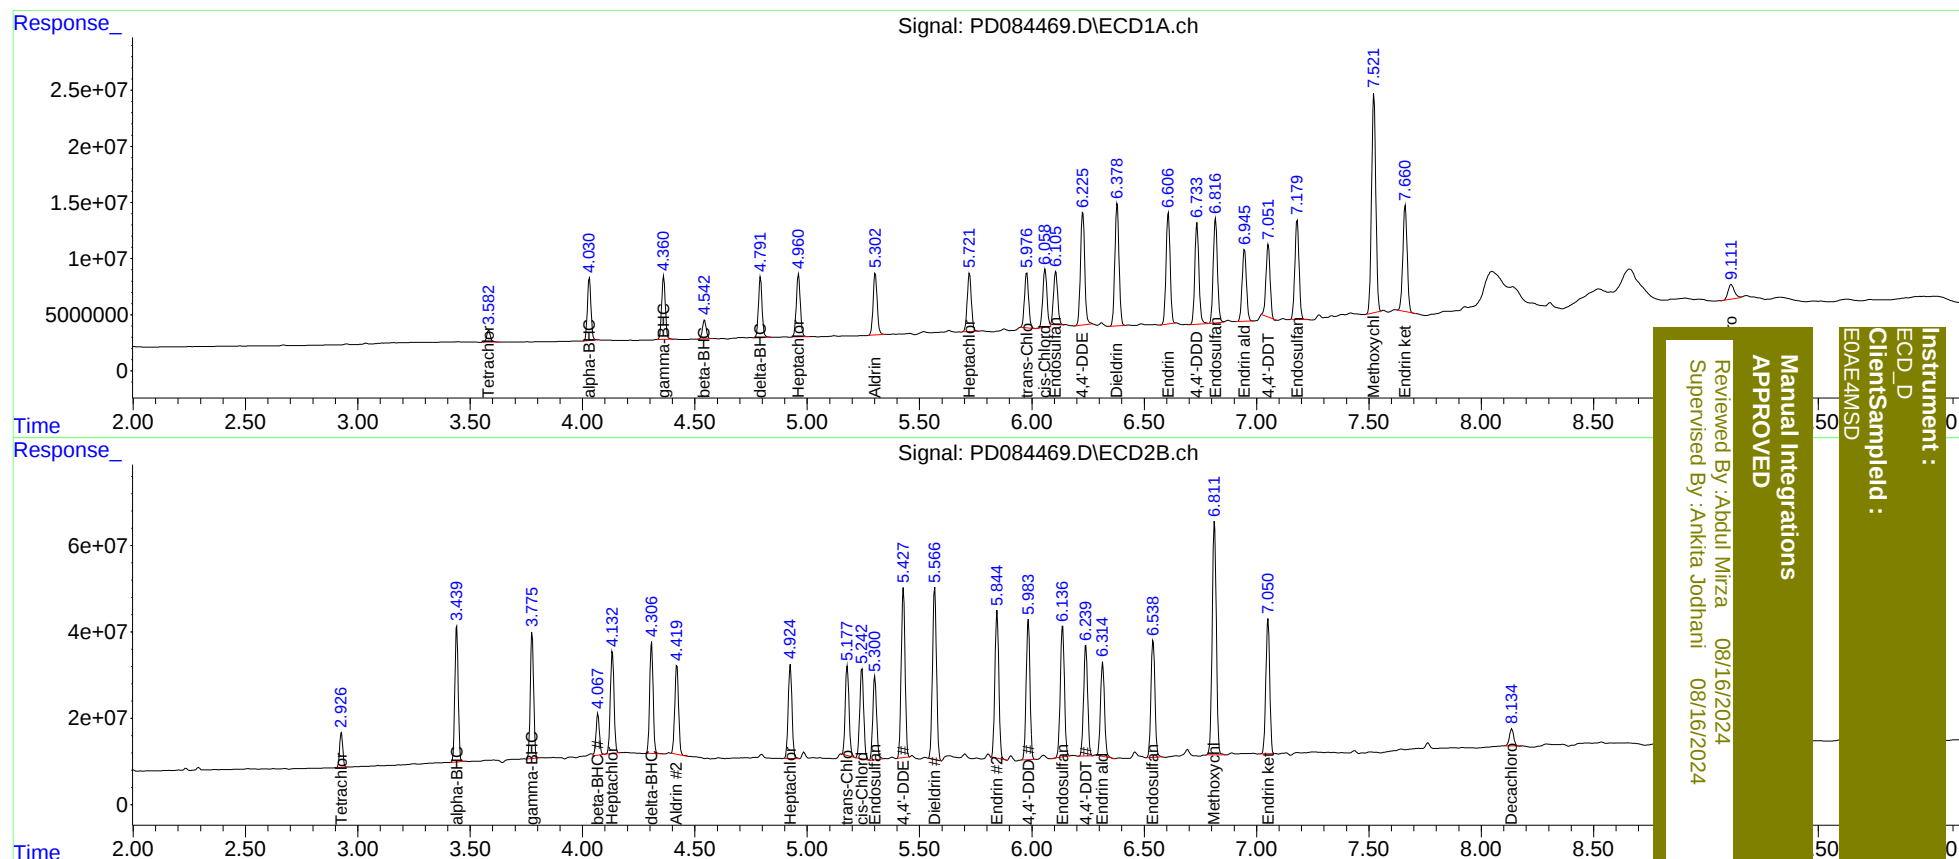

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 08/16/2024
Supervised By: Ankita Jodhani 08/16/2024

Instrument :
ECD_D
Client Sampled :
EOAE4MSD