

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081618\
 Data File : PD048985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Aug 2018 15:15
 Operator : AJ\SJ
 Sample : J4424-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:31:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 16 13:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.370	3.968	23623923	340.1E6	19.355	19.342
27) SA Decachlor...	8.066	8.992	46162917	524.6E6	32.060	32.409
Target Compounds						
4) MA Heptachlor	0.000	5.098f	0	3840326	N.D.	0.156
8) B Heptachlo...	0.000	5.850	0	2287740	N.D.	0.105
19) B Endosulfa...	0.000	7.190	0	5612726	N.D.	0.316


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081618\
Data File : PD048985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2018 15:15
Operator : AJ\SJ
Sample : J4424-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:31:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 16 13:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

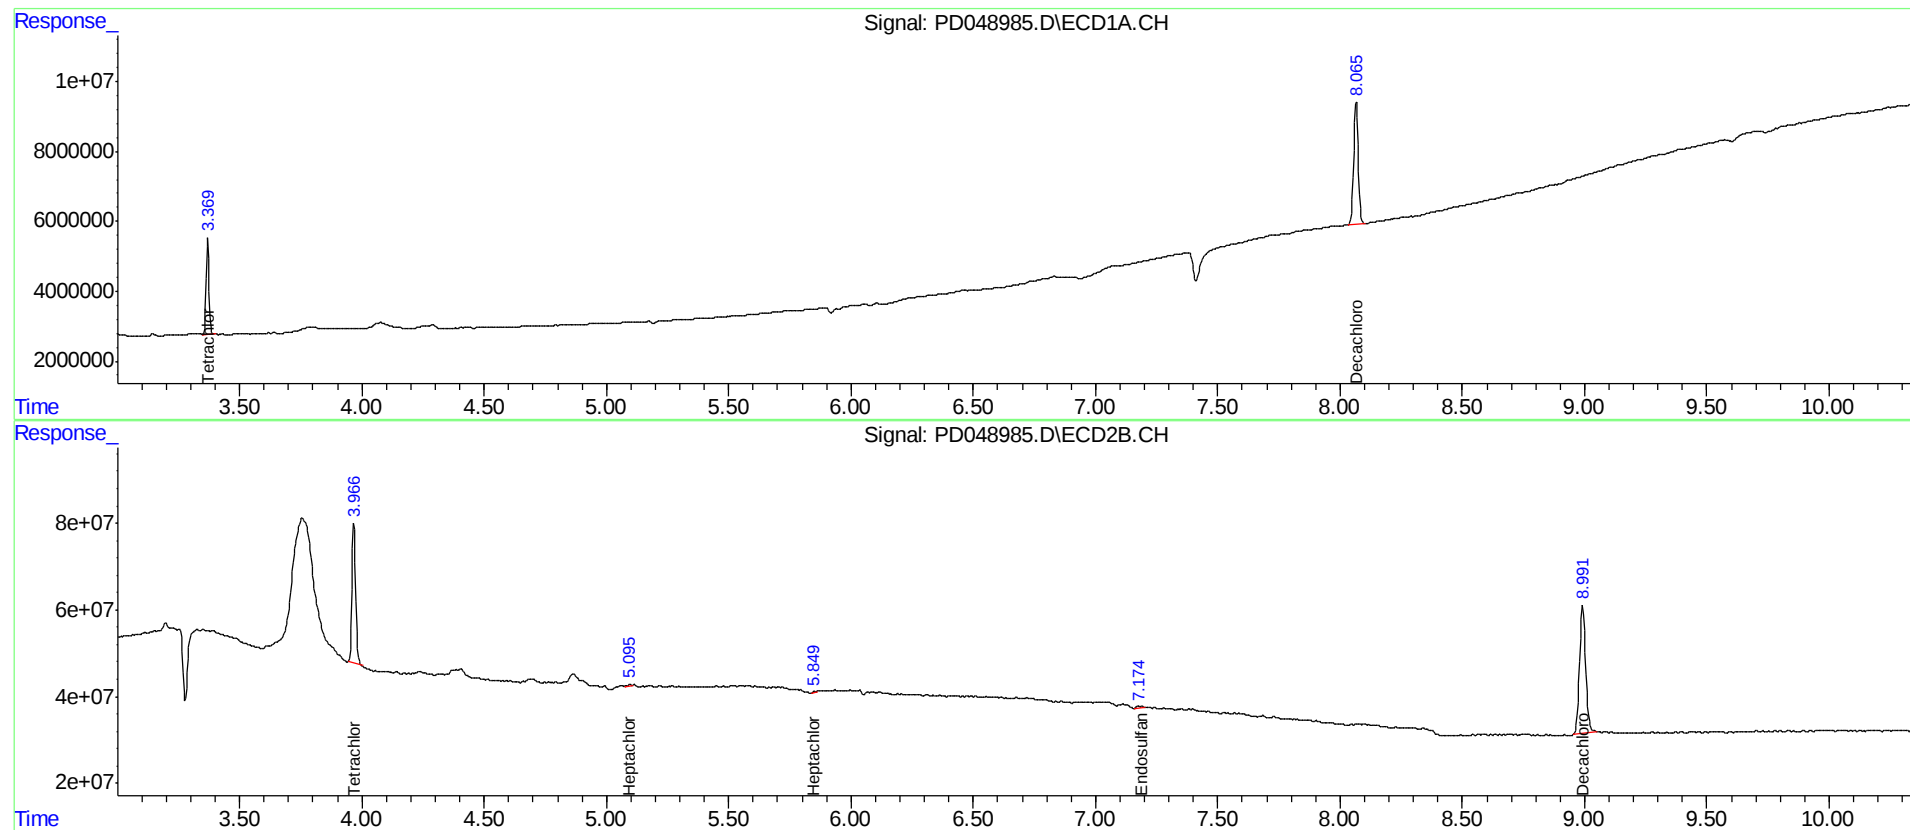


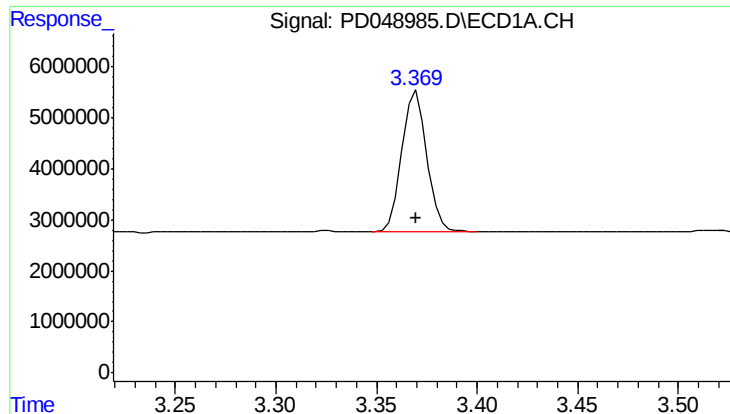

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 23623923
Conc: 19.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

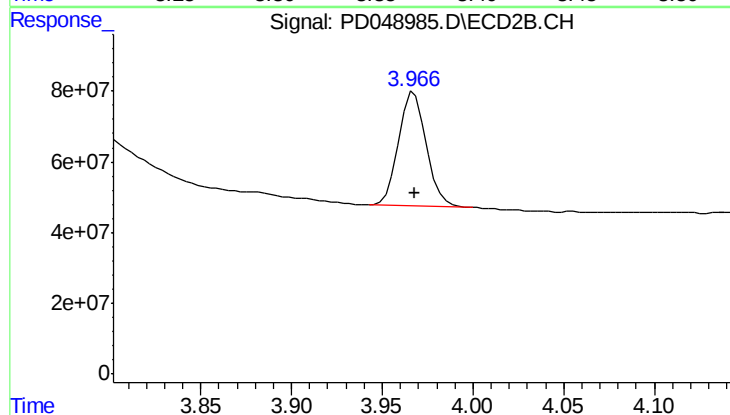


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 340078289
Conc: 19.34 ng/ml

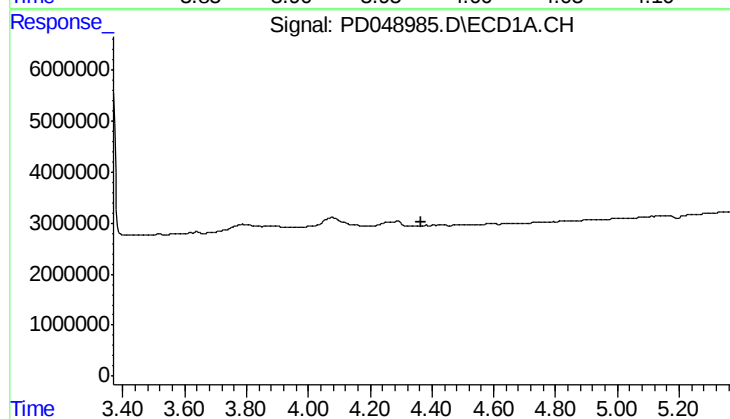


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.367 min
Response: 0
Conc: N.D.

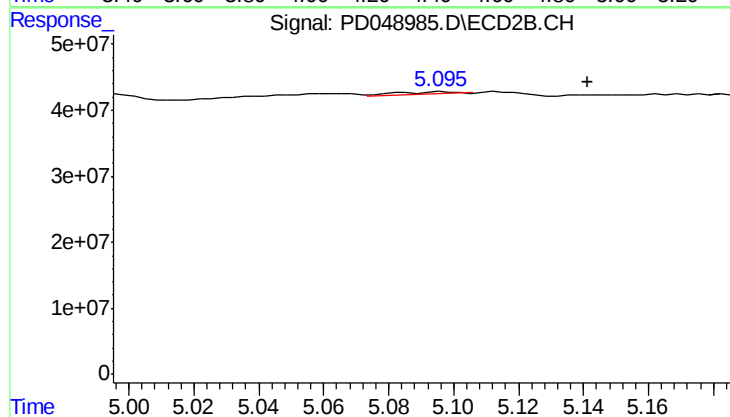

#4 Heptachlor


R.T.: 5.098 min
Delta R.T.: -0.044 min
Response: 3840326
Conc: 0.16 ng/ml

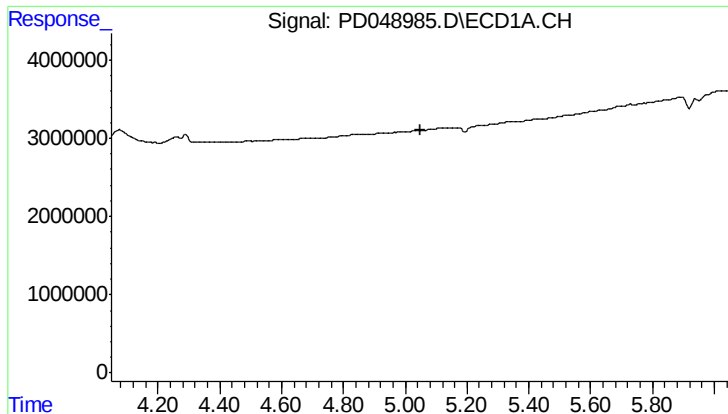

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

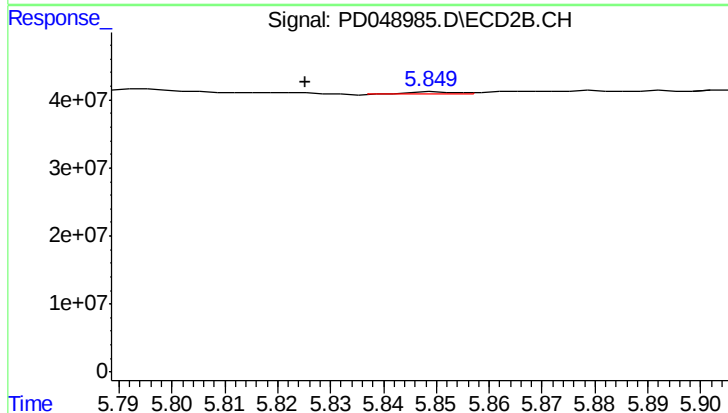


#8 Heptachlor epoxide

R.T.: 5.850 min
Delta R.T.: 0.025 min
Response: 2287740
Conc: 0.10 ng/ml

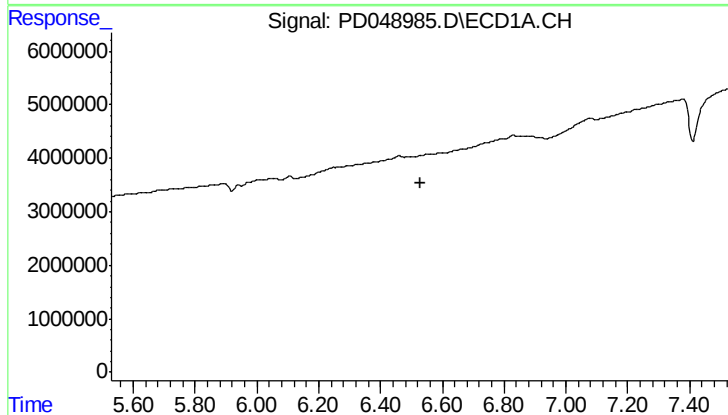


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.529 min
Response: 0
Conc: N.D.

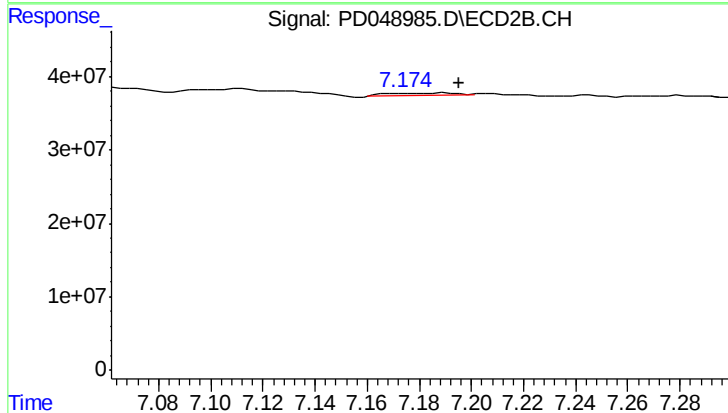

#19 Endosulfan Sulfate


R.T.: 7.190 min
Delta R.T.: -0.005 min
Response: 5612726
Conc: 0.32 ng/ml

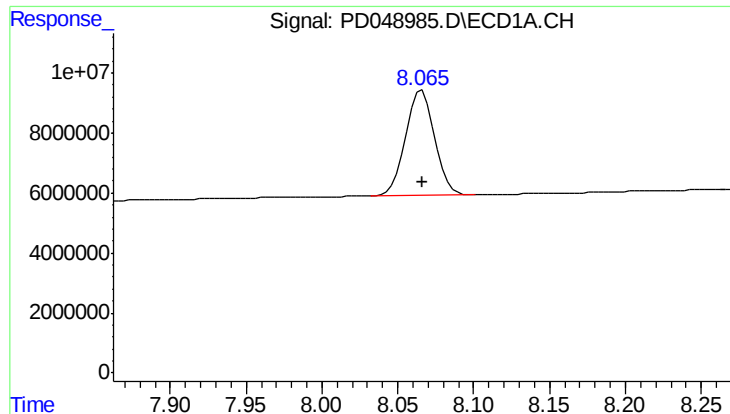

#27 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 46162917
Conc: 32.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

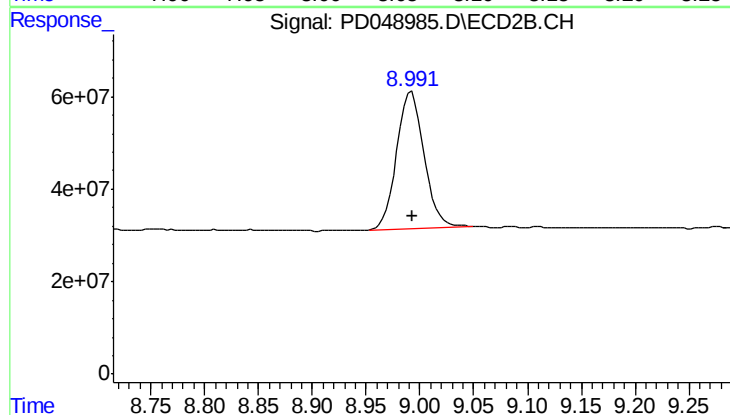

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 524642682
Conc: 32.41 ng/ml