

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081619\
 Data File : PD054322.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Aug 2019 15:07
 Operator : SG\AJ
 Sample : PIBLK36
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK37

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 18:02:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081619CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 16 15:23:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	14333490	20102744	20.647	20.592
2)	SA Decachlor...	8.005	9.024	28410794	39934470	41.120	41.046


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081619\
Data File : PD054322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2019 15:07
Operator : SG\AJ
Sample : PIBLK36
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 18:02:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081619CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 16 15:23:53 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

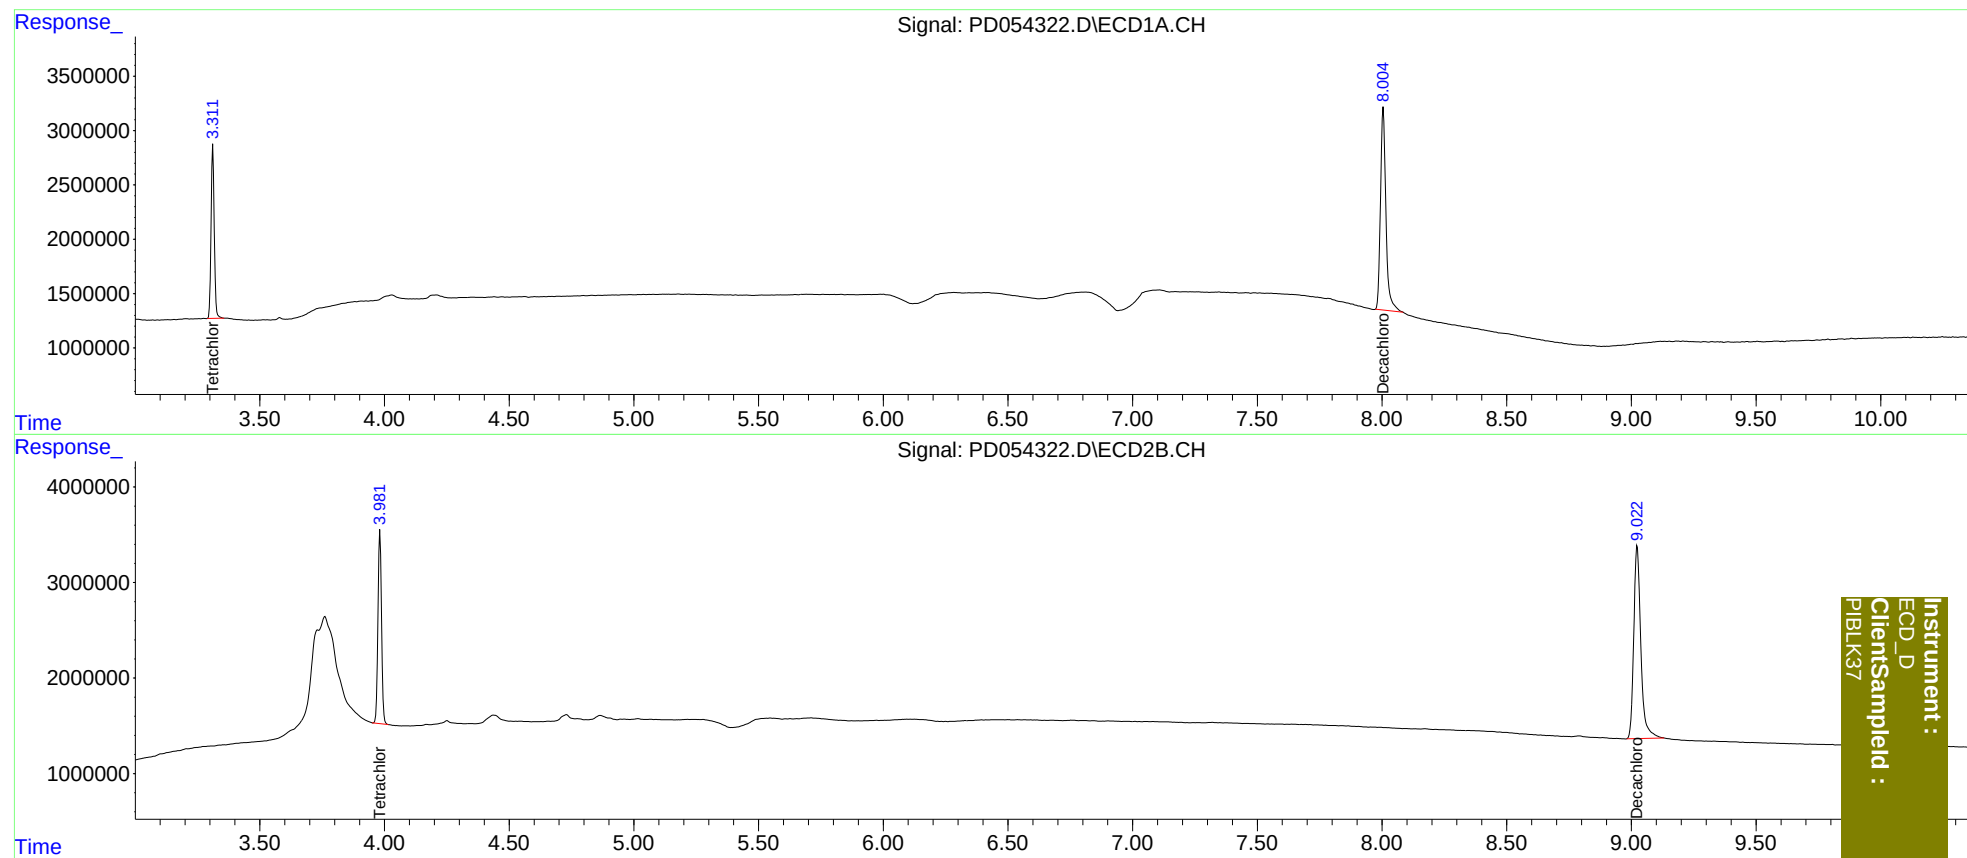


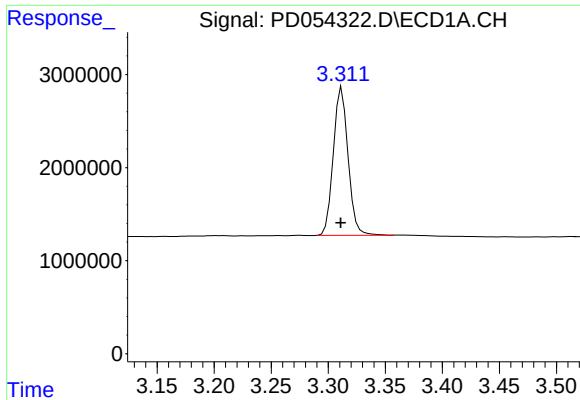

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.001 min
Response: 14333490
Conc: 20.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK37

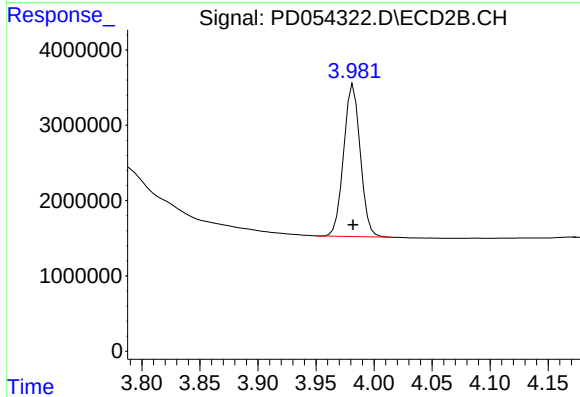


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 20102744
Conc: 20.59 ng/ml

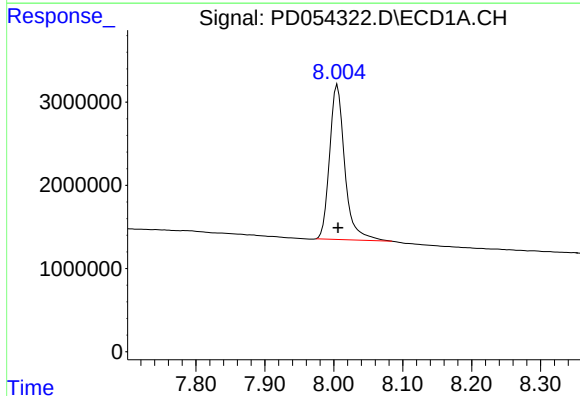

#27 Decachlorobiphenyl

R.T.: 8.005 min
Delta R.T.: 0.000 min
Response: 28410794
Conc: 41.12 ng/ml

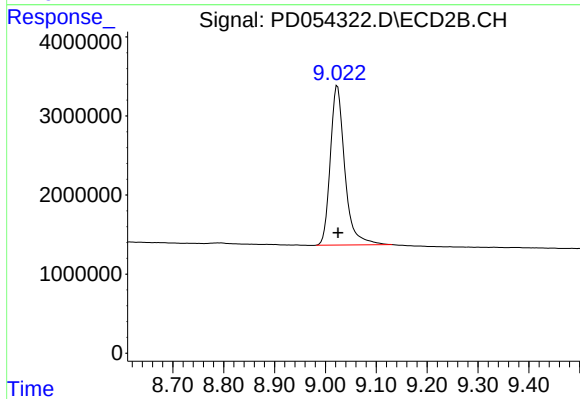

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.001 min
Response: 39934470
Conc: 41.05 ng/ml