

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081622\
 Data File : PD071588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2022 16:40
 Operator : AR\AJ
 Sample : N4216-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NB-08-081522

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/17/2022
 Supervised By :Ankita Jodhani 08/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:50:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 16 05:36:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.806	3.564	28702193	343.4E6	10.503	11.715
2) SA Decachlor...	8.000	9.091	33395917	136.2E6	11.498	13.348
Target Compounds						
11) B alpha-Chl...	5.102	6.048	1700361	18144616	0.444m	1.086m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081622\
Data File : PD071588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2022 16:40
Operator : AR\AJ
Sample : N4216-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
NB-08-081522


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/17/2022
Supervised By :Ankita Jodhani 08/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:50:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081522.M
Quant Title : GC Extractables
QLast Update : Tue Aug 16 05:36:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

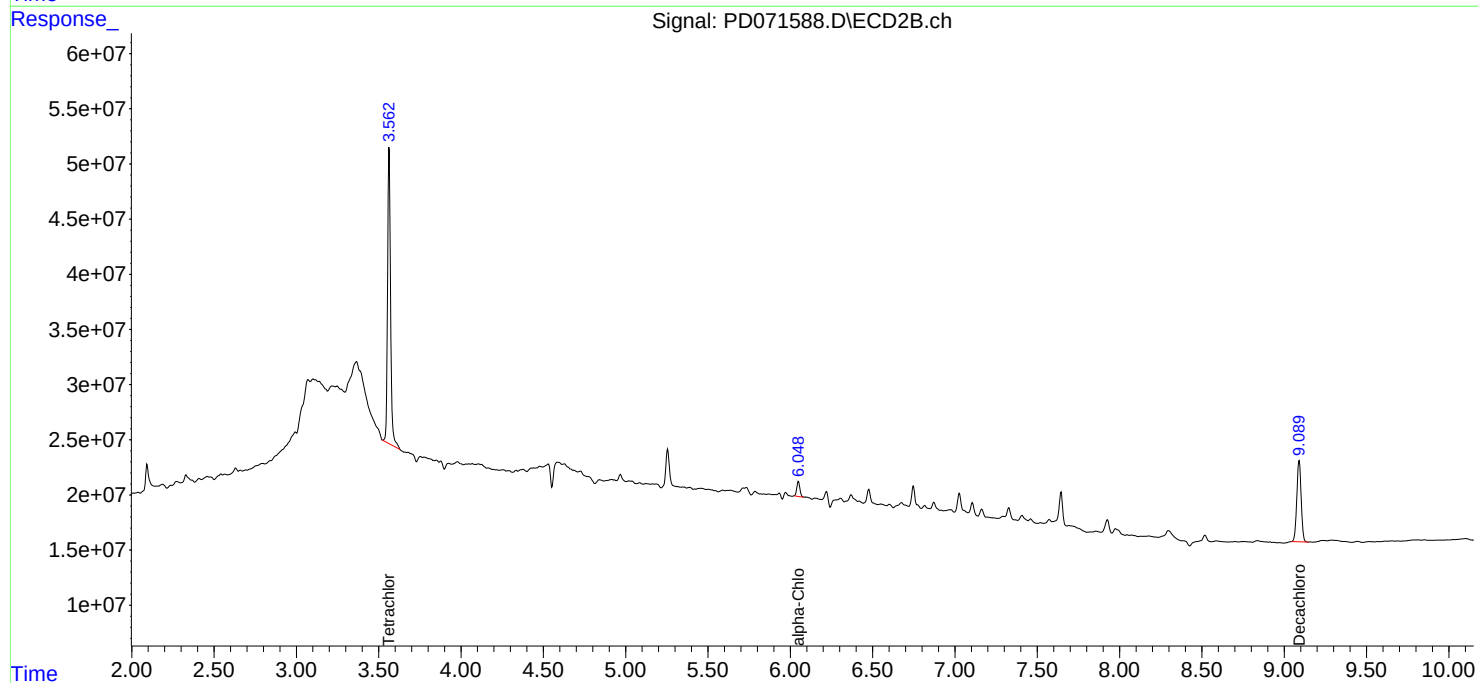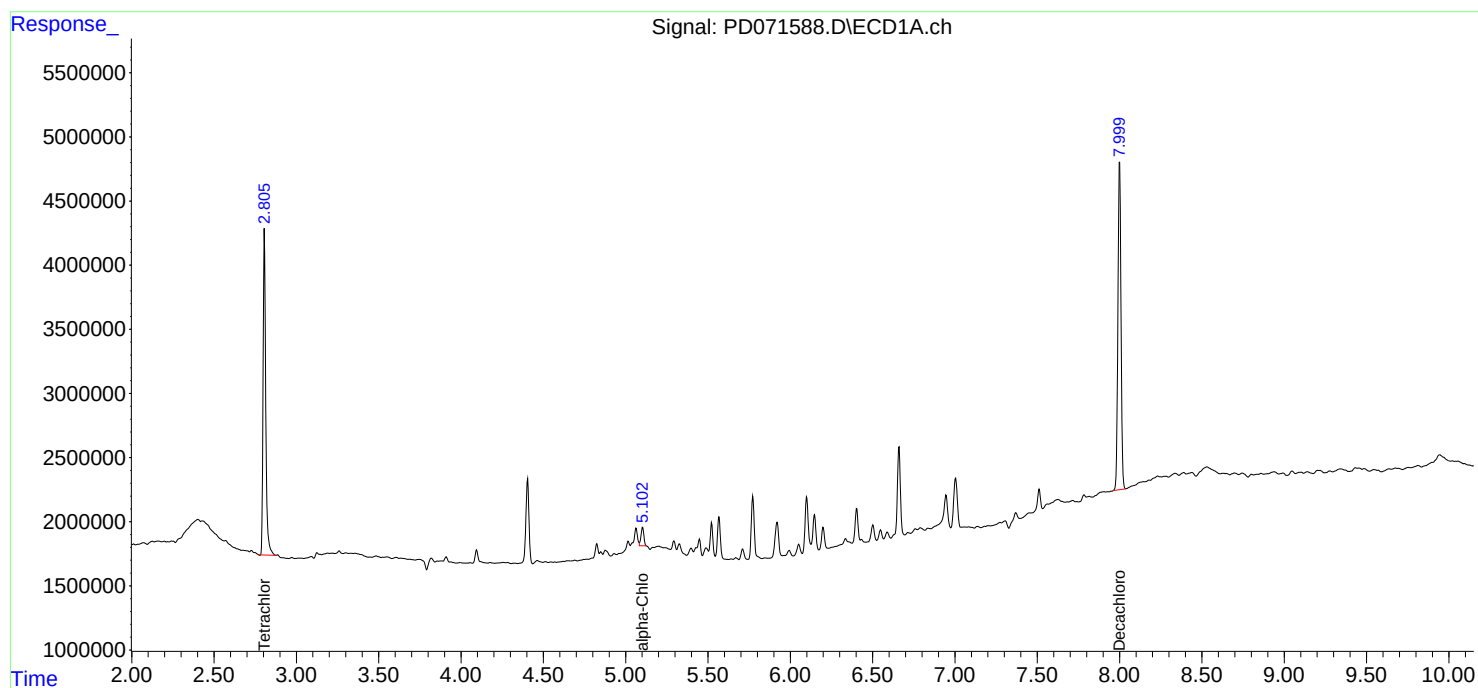

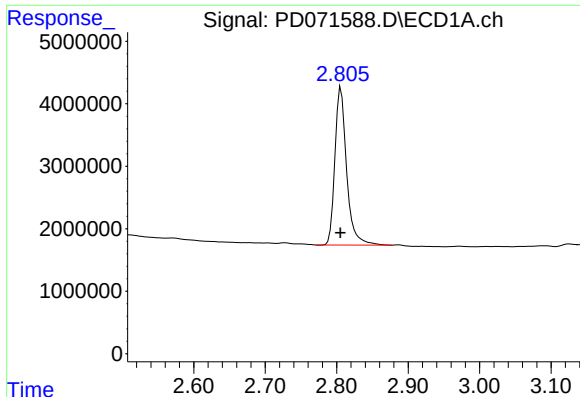


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.001 min
Response: 28702193
Conc: 10.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
NB-08-081522


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/17/2022
Supervised By :Ankita Jodhani 08/17/2022

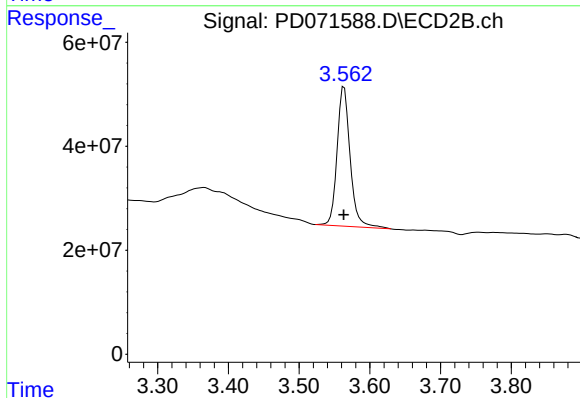


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 343381225
Conc: 11.72 ng/ml

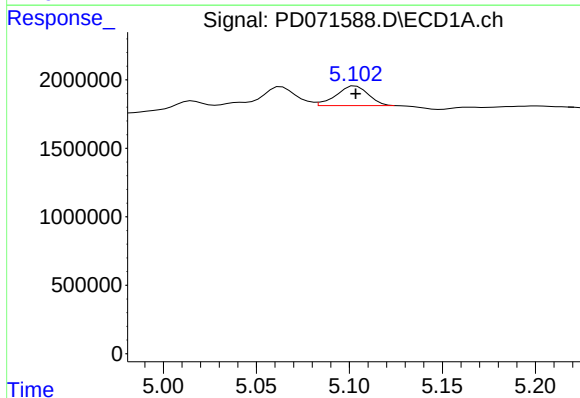


#11 alpha-Chlordane

R.T.: 5.102 min
Delta R.T.: -0.001 min
Response: 1700361
Conc: 0.44 ng/ml m

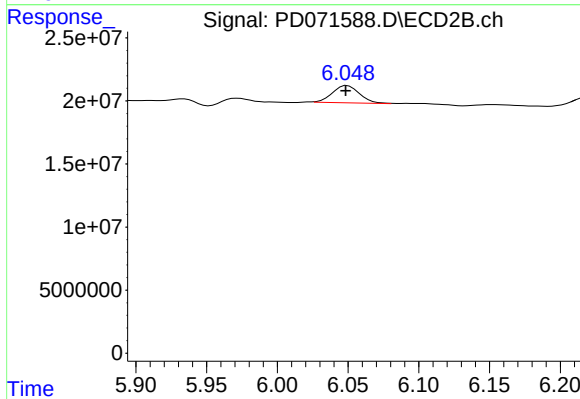

#11 alpha-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 18144616
Conc: 1.09 ng/ml m

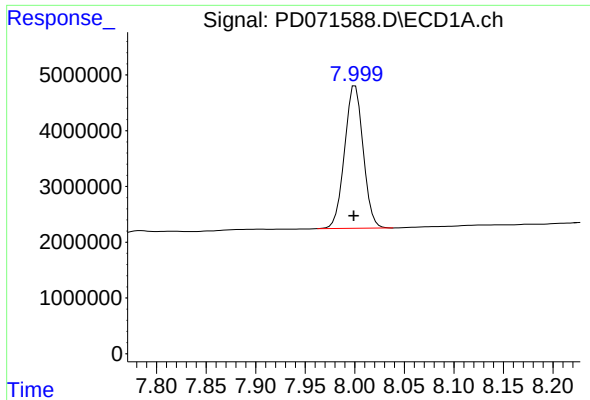

#28 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: 0.001 min
Response: 33395917
Conc: 11.50 ng/ml

Instrument :

ECD_D

ClientSampleId :


NB-08-081522

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/17/2022

Supervised By :Ankita Jodhani 08/17/2022

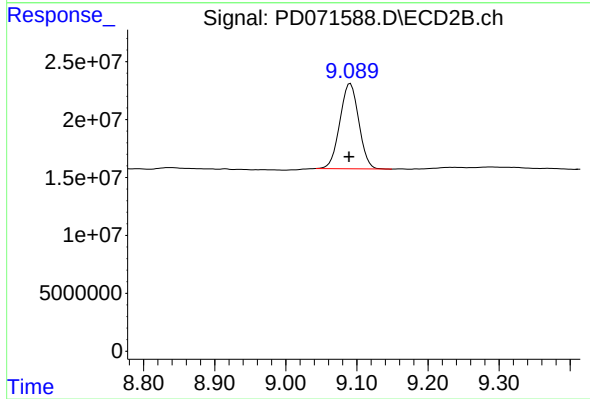

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.002 min
Response: 136200526
Conc: 13.35 ng/ml