

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
 Data File : PD084480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 10:26
 Operator : AR\AJ
 Sample : PIBLK064
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK223

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 23:46:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.582	2.926	20468486	132.4E6	24.414	25.147
2)	SA Decachlor...	9.113	8.136	42332793	105.2E6	24.339	28.005
Target Compounds							
10)	B trans-Chl...	6.026f	0.000	931428	0	0.564	N.D. #
11)	B cis-Chlor...	6.026f	0.000	931428	0	0.541	N.D. #
12)	B 4,4'-DDE	6.262	0.000	1254910	0	0.717	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
Data File : PD084480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 10:26
Operator : AR\AJ
Sample : PIBLK064
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 23:46:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

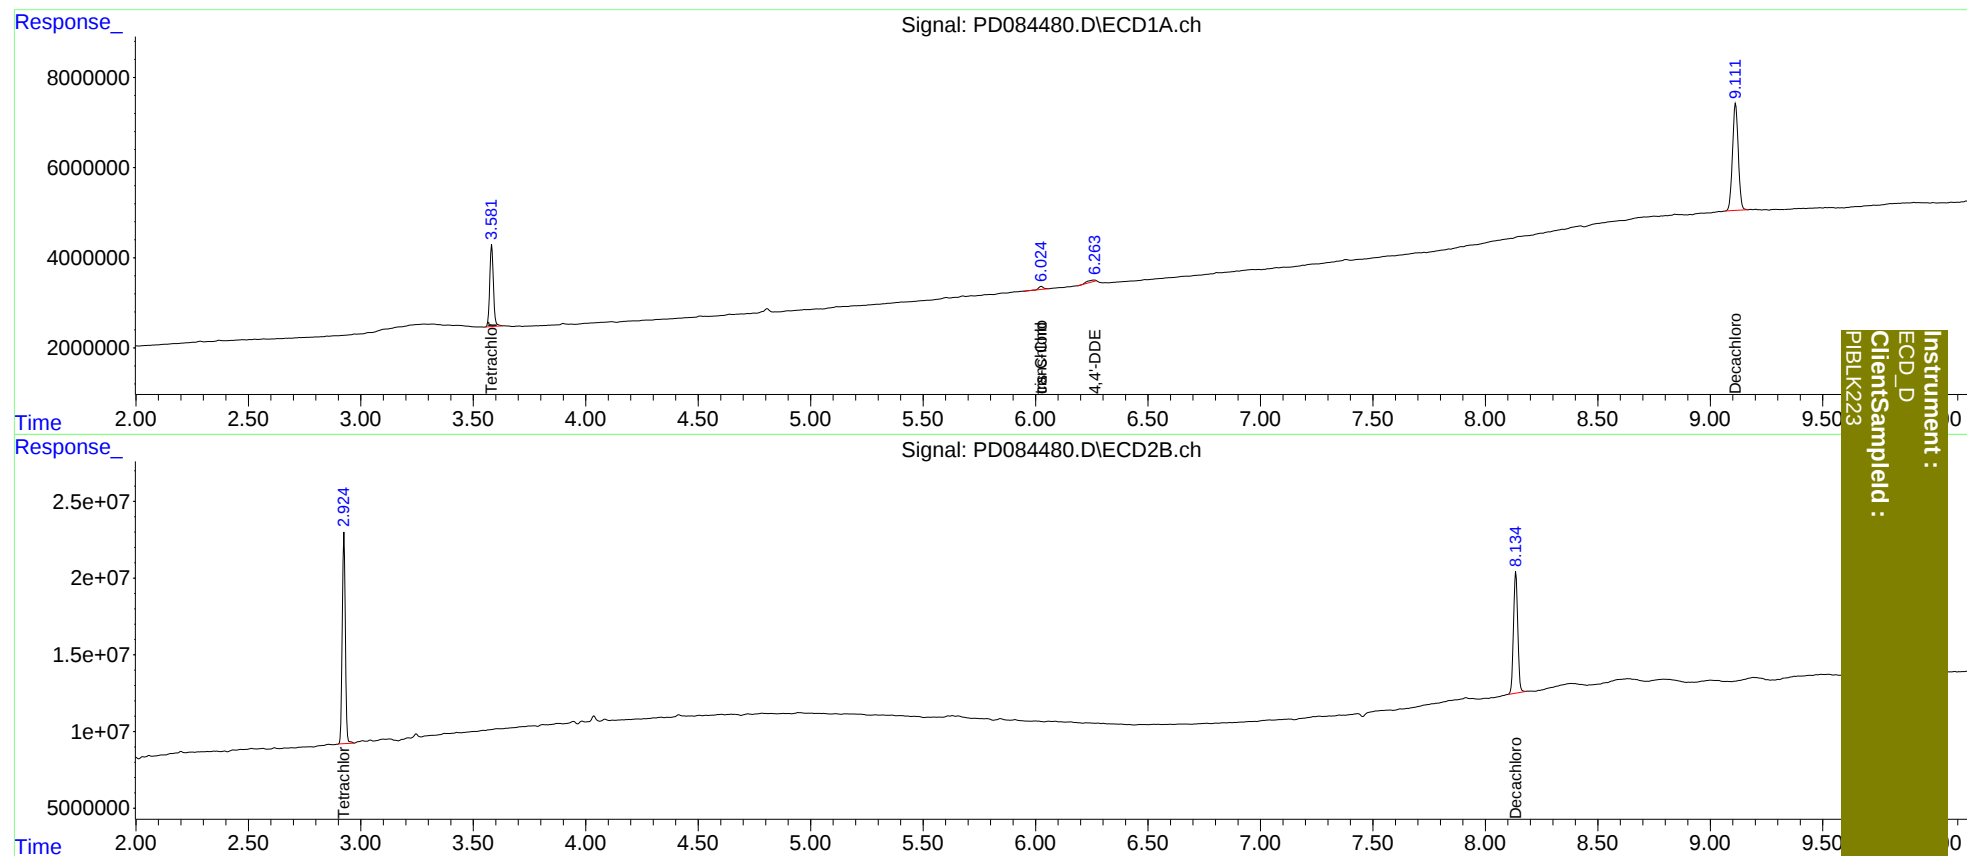


Instrument :
ECD_D
ClientSampled :
PIBLK223

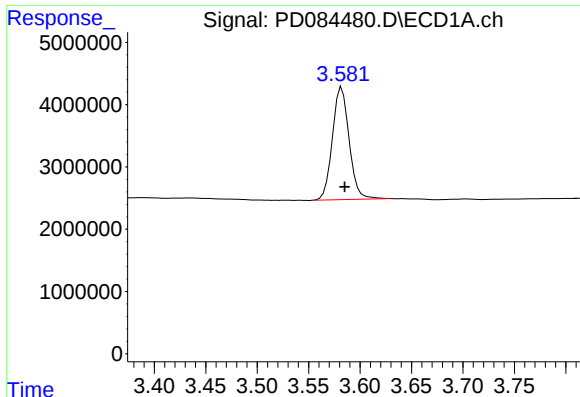

#1 Tetrachloro-m-xylene


R.T.: 3.582 min
Delta R.T.: -0.003 min
Response: 20468486
Conc: 24.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK223

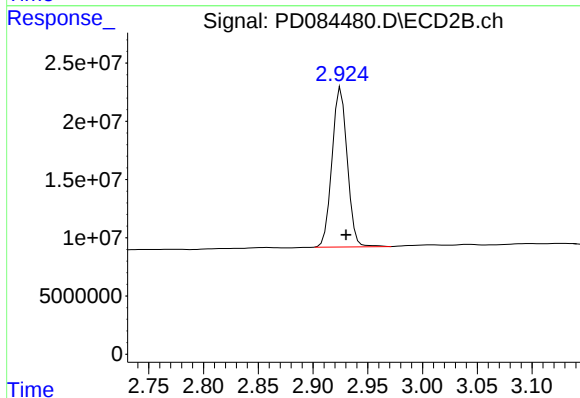


#1 Tetrachloro-m-xylene

R.T.: 2.926 min
Delta R.T.: -0.005 min
Response: 132378255
Conc: 25.15 ng/ml

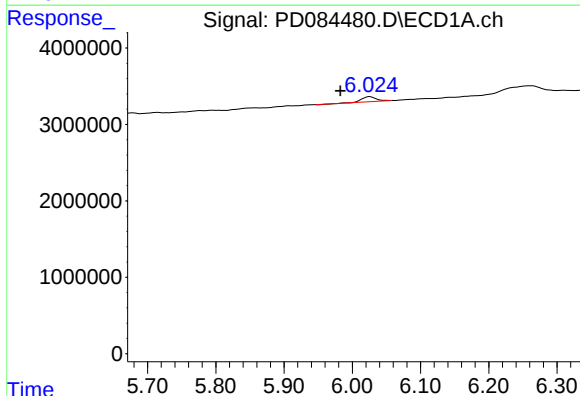


#10 trans-Chlordane

R.T.: 6.026 min
Delta R.T.: 0.043 min
Response: 931428
Conc: 0.56 ng/ml

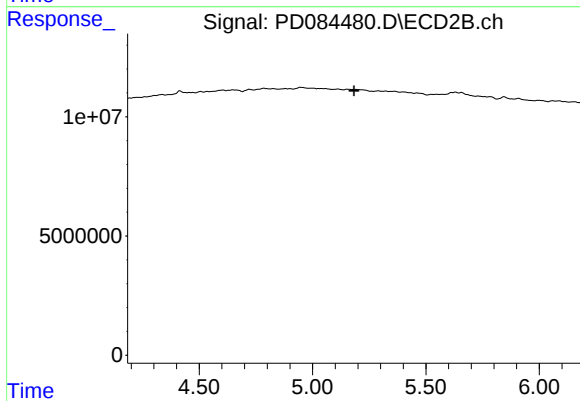

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

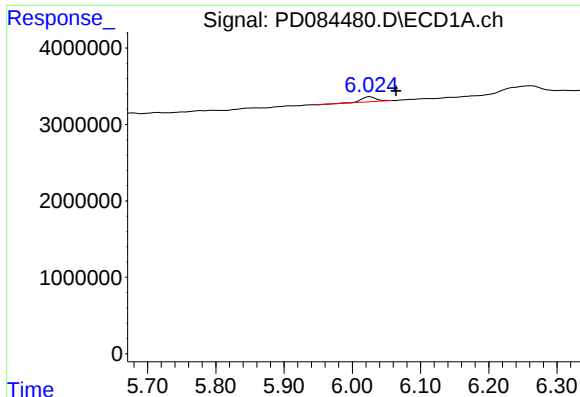

#11 cis-Chlordane


R.T.: 6.026 min
Delta R.T.: -0.038 min
Response: 931428
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK223

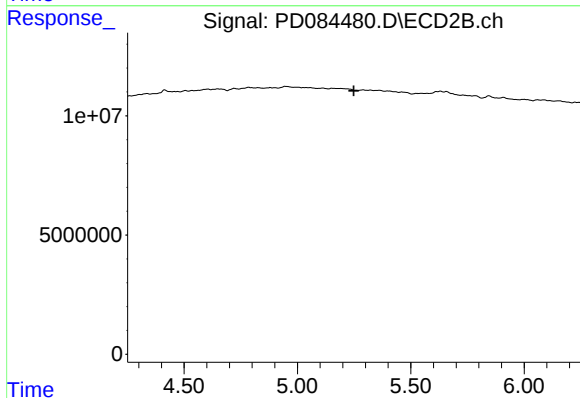


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

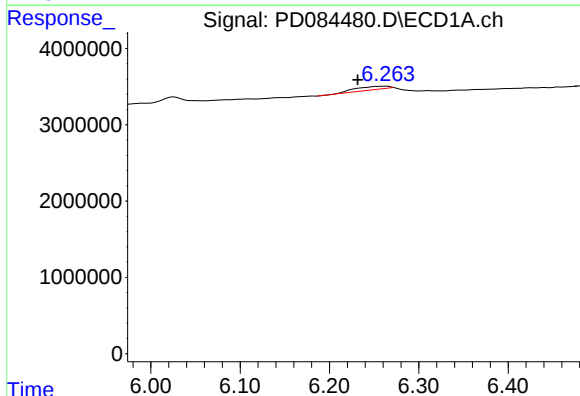


#12 4,4'-DDE

R.T.: 6.262 min
Delta R.T.: 0.030 min
Response: 1254910
Conc: 0.72 ng/ml

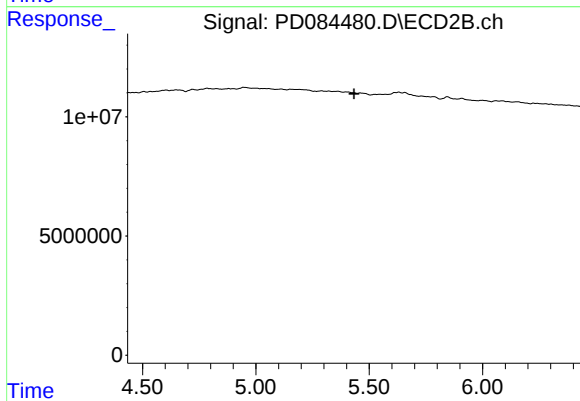

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 5.434 min
Response: 0
Conc: N.D.

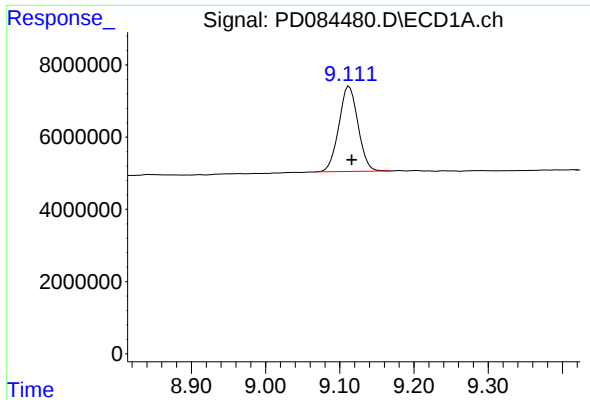

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.003 min
Response: 42332793
Conc: 24.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK223

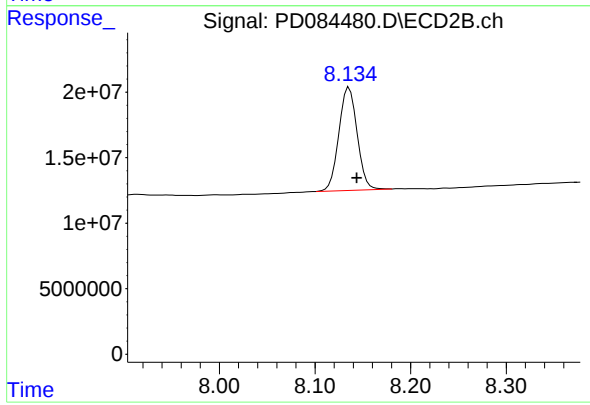

#27 Decachlorobiphenyl

R.T.: 8.136 min
Delta R.T.: -0.008 min
Response: 105241695
Conc: 28.01 ng/ml