

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
 Data File : PD084504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 16:38
 Operator : AR\AJ
 Sample : P3502-18MSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXU9MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 23:53:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.583	2.927	9272850	57875929	11.061	10.994
27) SA Decachlor...	9.106	8.108	20175206	717.7E6	11.600m	190.989m#
Target Compounds						
2) A alpha-BHC	4.031	3.441	80810709	408.3E6	53.392	50.085
3) MA gamma-BHC...	4.361	3.776	139.2E6	586.4E6	89.385	76.088
4) MA Heptachlor	4.961	4.132	86788013	353.3E6	49.725	46.874m
5) MB Aldrin	5.303	4.420	86439507	345.3E6	48.979	47.118
6) B beta-BHC	4.543	4.069	41632364	174.0E6	57.622	48.389
7) B delta-BHC	4.792	4.308	109.5E6	452.5E6	63.381	53.944
8) B Heptachlo...	5.722	4.925	78420060	305.1E6	46.139	45.723
9) A Endosulfan I	6.106	5.300	78348511	273.8E6	49.184	46.155m
10) B trans-Chl...	5.977	5.179	78900726	300.4E6	47.785	47.137
11) B cis-Chlor...	6.059	5.244	81433625	301.2E6	47.325	47.851
12) B 4,4'-DDE	6.226	5.428	163.4E6	577.6E6	93.424	94.710
13) MA Dieldrin	6.379	5.568	171.6E6	558.1E6	95.520	90.716
14) MA Endrin	6.607	5.845	151.0E6	509.9E6	100.825	92.367
15) B Endosulfa...	6.817	6.136	148.9E6	466.7E6	90.319	89.878
16) A 4,4'-DDD	6.735	5.983	135.2E6	418.2E6	105.107	85.239m
17) MA 4,4'-DDT	7.051	6.240	123.6E6	447.1E6	91.189	90.257
18) B Endrin al...	6.945	6.315	106.6E6	320.6E6	93.802	85.695
19) B Endosulfa...	7.179	6.555	145.4E6	1010.6E6	95.770	216.461m#
20) A Methoxychlor	7.521	6.812	346.0E6	994.7E6	433.892	461.901
21) B Endrin ke...	7.654	7.048	606.8E6	495.4E6	366.407m	95.131m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
Data File : PD084504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 16:38
Operator : AR\AJ
Sample : P3502-18MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 23:53:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

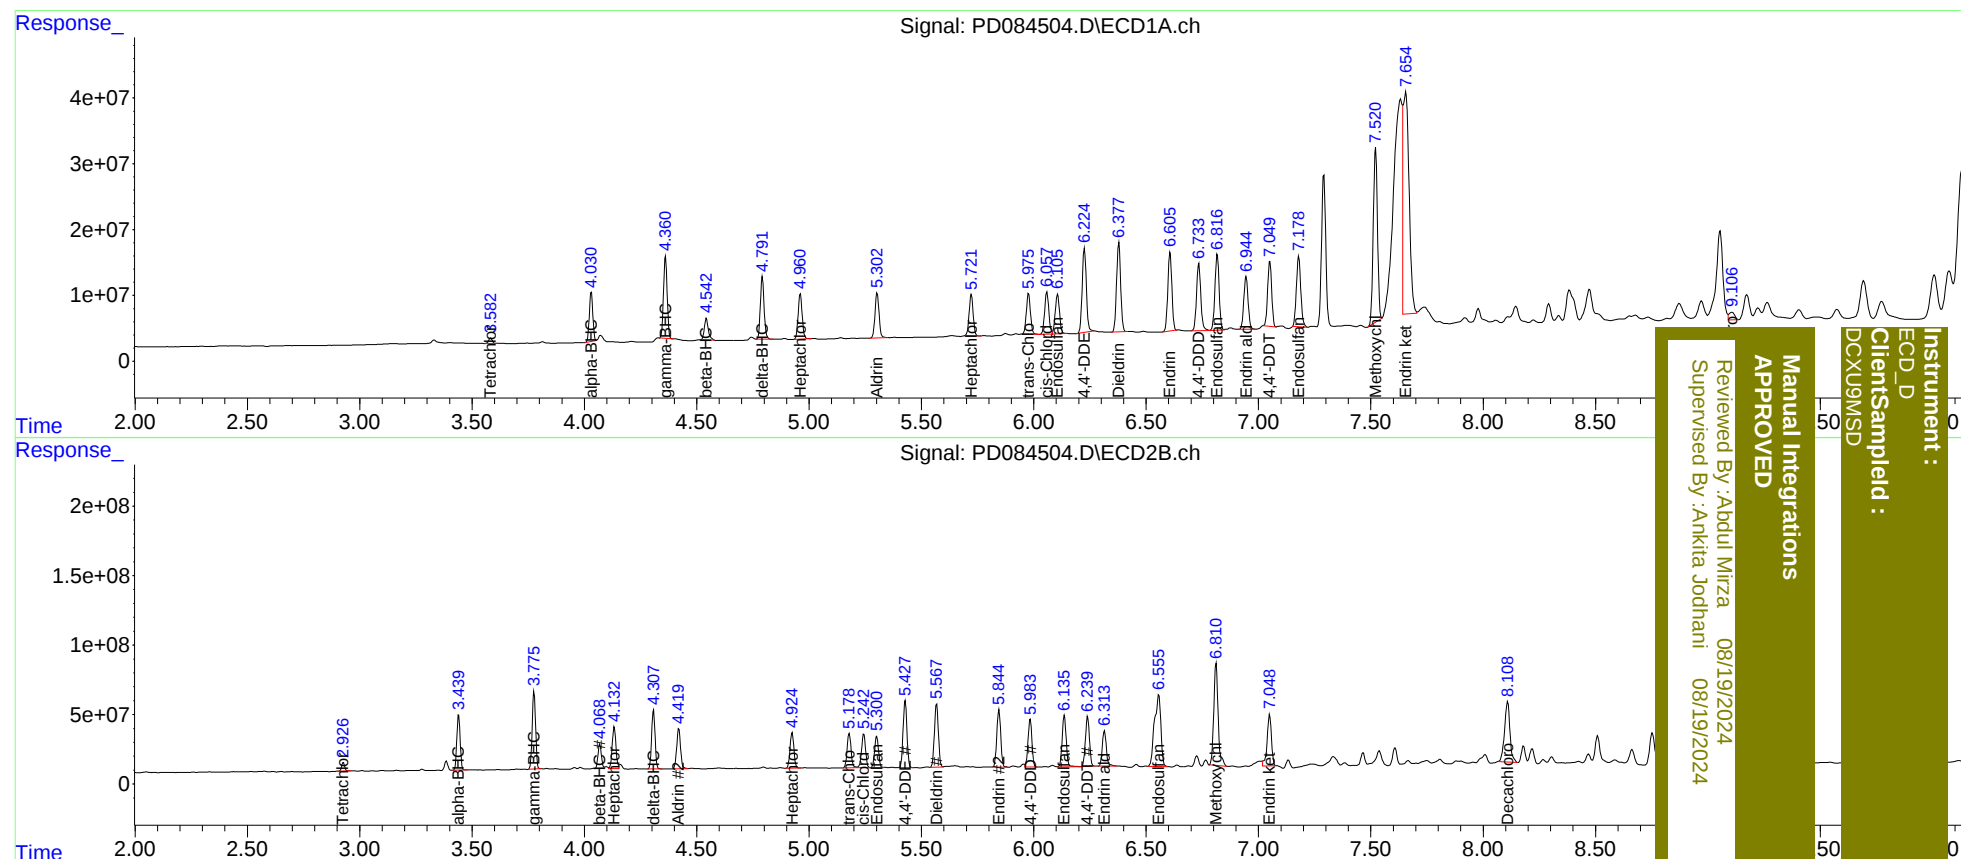

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Instrument :
ECD_D
Client Sampled :
DCXU9MSD