

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
 Data File : PD084503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 16:24
 Operator : AR\AJ
 Sample : P3502-17MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXU9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 23:52:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.583	2.927	8154633	51988220	9.727	9.876
2)	SA Decachlor...	9.106	8.108	17937099	677.5E6	10.313m	180.273m#
Target Compounds							
2)	A alpha-BHC	4.031	3.440	80574167	409.7E6	53.236	50.256
3)	MA gamma-BHC...	4.361	3.776	134.1E6	567.8E6	86.125	73.671
4)	MA Heptachlor	4.961	4.131	87036316	336.9E6	49.868	44.704m
5)	MB Aldrin	5.303	4.420	86777070	348.2E6	49.170	47.510
6)	B beta-BHC	4.543	4.067	41070907	184.7E6	56.845	51.348m
7)	B delta-BHC	4.792	4.307	107.5E6	447.3E6	62.270	53.320
8)	B Heptachlo...	5.722	4.924	78532379	306.5E6	46.205	45.940
9)	A Endosulfan I	6.105	5.299	79379027	274.1E6	49.831	46.202m
10)	B trans-Chl...	5.976	5.178	78948094	307.5E6	47.814	48.251
11)	B cis-Chlor...	6.058	5.243	81796602	303.4E6	47.536	48.211
12)	B 4,4'-DDE	6.225	5.428	167.7E6	583.0E6	95.866	95.593
13)	MA Dieldrin	6.378	5.567	176.2E6	566.9E6	98.085	92.147
14)	MA Endrin	6.606	5.844	151.8E6	516.3E6	101.335	93.518
15)	B Endosulfa...	6.816	6.135	150.5E6	477.1E6	91.307	91.879
16)	A 4,4'-DDD	6.734	5.982	135.8E6	434.5E6	105.552	88.575m
17)	MA 4,4'-DDT	7.050	6.239	124.4E6	455.0E6	91.756	91.850
18)	B Endrin al...	6.945	6.314	105.3E6	324.0E6	92.640	86.592
19)	B Endosulfa...	7.180	6.544	146.6E6	421.1E6	96.583	90.198m
20)	A Methoxychlor	7.521	6.812	343.5E6	996.5E6	430.757	462.756
21)	B Endrin ke...	7.656	7.048	437.7E6	419.8E6	264.302m	80.608m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081624\
Data File : PD084503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 16:24
Operator : AR\AJ
Sample : P3502-17MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 23:52:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

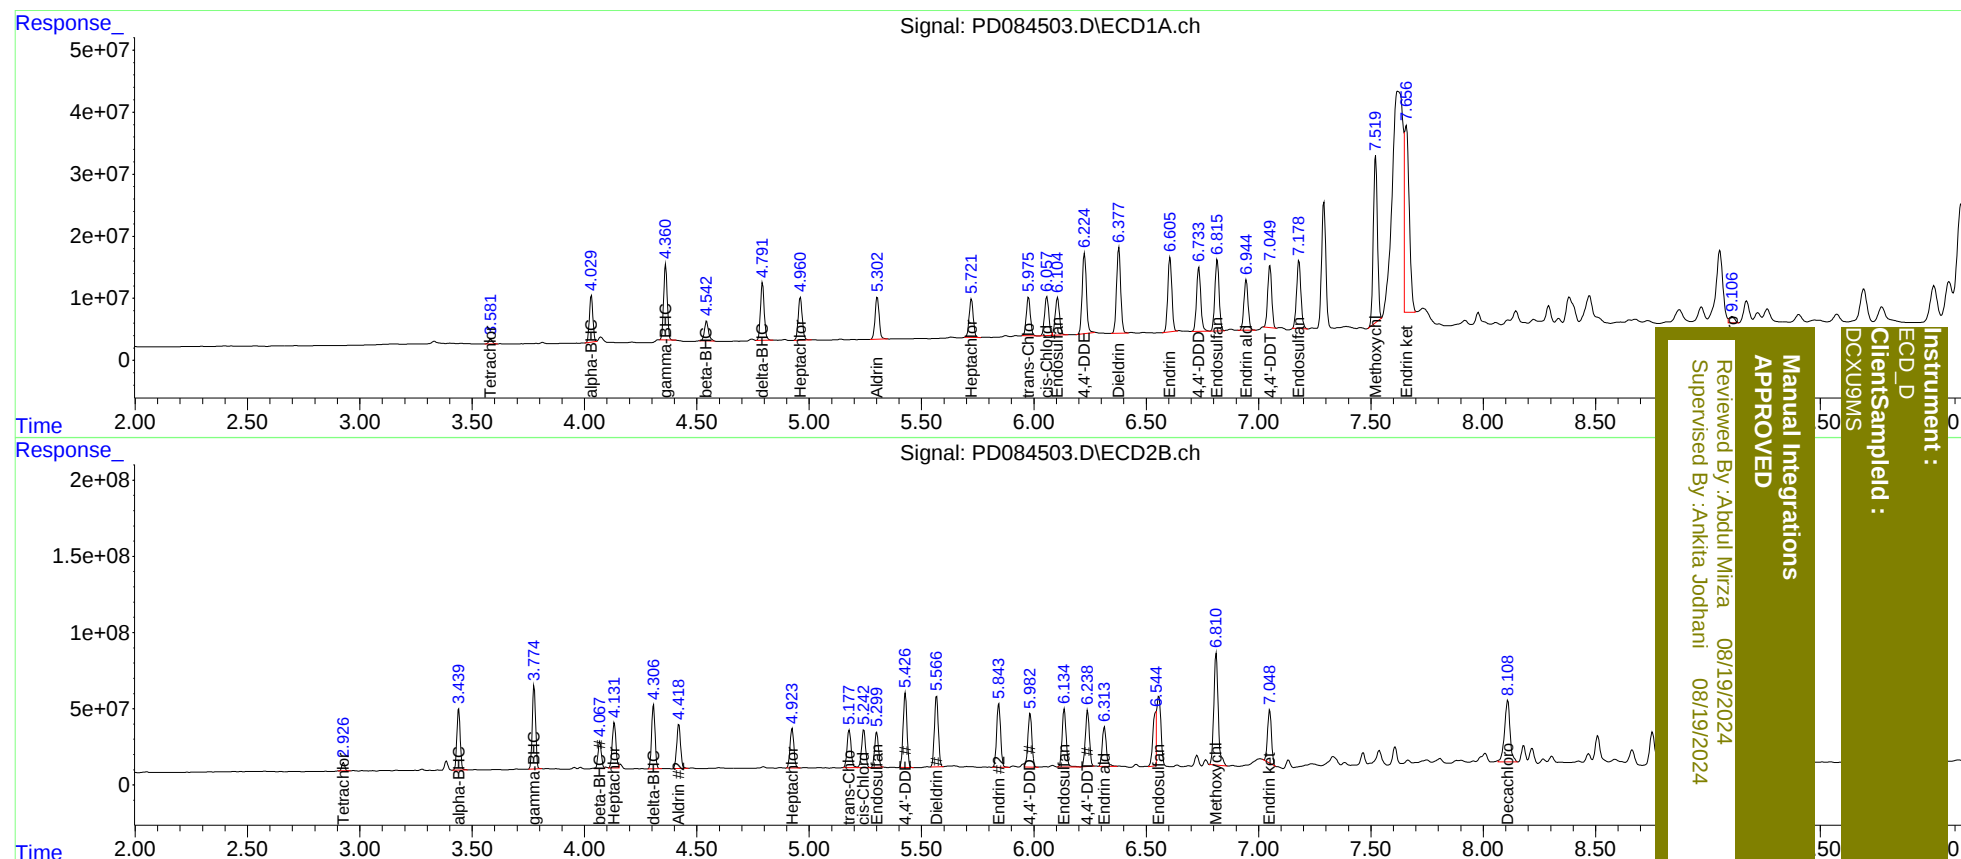

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/19/2024
Supervised By: Ankita Jodhani 08/19/2024

Instrument :
ECD_D
Client Sampled :
DCXU9MS